

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045088.D
 Acq On : 04 Oct 2021 11:56
 Operator : SY/MD
 Sample : VU1004WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK009

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU045088.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	93	rBV	183909	209077	15.51%	2.106%
2	1.916	170	179	193	rVB	147062	194784	14.45%	1.962%
3	2.572	370	383	405	rBV	289041	482940	35.84%	4.865%
4	2.691	417	420	423	rVV2	243	174	0.01%	0.002%
5	2.793	449	452	454	rBV	381	254	0.02%	0.003%
6	2.961	494	504	508	rBV3	673	1035	0.08%	0.010%
7	3.054	523	533	543	rVB	3765	6634	0.49%	0.067%
8	3.176	567	571	574	rVB2	168	168	0.01%	0.002%
9	3.208	577	581	586	rBV2	209	283	0.02%	0.003%
10	3.285	601	605	608	rBV	243	169	0.01%	0.002%
11	3.401	637	641	645	rBV2	166	202	0.01%	0.002%
12	3.523	676	679	686	rBV2	206	247	0.02%	0.002%
13	3.584	694	698	702	rBV2	170	189	0.01%	0.002%
14	3.871	784	787	792	rVB2	189	175	0.01%	0.002%
15	3.903	792	797	801	rBV	249	163	0.01%	0.002%
16	3.935	804	807	814	rBV	194	229	0.02%	0.002%
17	3.967	814	817	822	rVB	243	204	0.02%	0.002%
18	3.999	822	827	832	rBV2	252	329	0.02%	0.003%
19	4.195	885	888	894	rVV2	135	164	0.01%	0.002%
20	4.260	901	908	912	rBV2	248	402	0.03%	0.004%
21	4.436	958	963	967	rBV	269	282	0.02%	0.003%
22	4.530	985	992	997	rBV	201	325	0.02%	0.003%
23	4.562	998	1002	1008	rVB	231	260	0.02%	0.003%
24	4.633	1008	1024	1056	rBV2	137569	352765	26.18%	3.553%
25	5.070	1141	1160	1182	rBV	237845	520982	38.66%	5.248%
26	5.221	1205	1207	1210	rVB	391	193	0.01%	0.002%
27	5.369	1249	1253	1255	rBV	572	436	0.03%	0.004%
28	5.385	1255	1258	1263	rVB3	376	374	0.03%	0.004%
29	5.497	1288	1293	1295	rVB2	254	200	0.01%	0.002%
30	5.533	1297	1304	1305	rBV	171	214	0.02%	0.002%
31	5.607	1324	1327	1333	rVB2	205	193	0.01%	0.002%
32	5.732	1343	1366	1395	rBV2	501547	1347643	100.00%	13.575%
33	5.854	1402	1404	1410	rVB2	362	317	0.02%	0.003%
34	6.006	1449	1451	1457	rVB3	272	236	0.02%	0.002%
35	6.124	1485	1488	1491	rBV3	424	335	0.02%	0.003%
36	6.253	1514	1528	1551	rBV	340998	653787	48.51%	6.586%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045088.D
 Acq On : 04 Oct 2021 11:56
 Operator : SY/MD
 Sample : VU1004WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 VBLK009

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.378	1565	1567	1571	rVB3	408	193	0.01%	0.002%
38	6.497	1599	1604	1606	rVV2	282	235	0.02%	0.002%
39	6.536	1607	1616	1624	rVB8	3114	6040	0.45%	0.061%
40	6.697	1649	1666	1692	rBV	316284	615871	45.70%	6.204%
41	7.018	1760	1766	1769	rBV2	198	264	0.02%	0.003%
42	7.041	1769	1773	1774	rBV	292	196	0.01%	0.002%
43	7.189	1811	1819	1828	rBV3	1437	2399	0.18%	0.024%
44	7.385	1875	1880	1882	rBV2	199	201	0.01%	0.002%
45	7.475	1905	1908	1912	rBV2	202	192	0.01%	0.002%
46	7.571	1924	1938	1961	rBV	177226	310367	23.03%	3.126%
47	7.687	1970	1974	1977	rBV4	540	517	0.04%	0.005%
48	7.800	2004	2009	2017	rVB4	1247	1563	0.12%	0.016%
49	7.903	2027	2041	2056	rBV	614829	1047280	77.71%	10.550%
50	8.185	2117	2129	2151	rVV	123662	209947	15.58%	2.115%
51	8.321	2168	2171	2177	rVB4	408	379	0.03%	0.004%
52	8.513	2226	2231	2236	rBV2	315	366	0.03%	0.004%
53	8.639	2257	2270	2303	rBV	420114	745527	55.32%	7.510%
54	8.922	2355	2358	2364	rBV2	164	194	0.01%	0.002%
55	8.986	2371	2378	2382	rBV2	212	342	0.03%	0.003%
56	9.423	2500	2514	2549	rBV	479352	810338	60.13%	8.163%
57	9.571	2556	2560	2567	rBV2	450	673	0.05%	0.007%
58	9.700	2593	2600	2605	rBV2	881	1076	0.08%	0.011%
59	9.931	2670	2672	2678	rBV2	159	157	0.01%	0.002%
60	10.076	2714	2717	2722	rBV2	195	201	0.01%	0.002%
61	10.102	2722	2725	2726	rBV	410	241	0.02%	0.002%
62	10.192	2750	2753	2756	rBV2	191	161	0.01%	0.002%
63	10.346	2798	2801	2806	rVB	208	171	0.01%	0.002%
64	10.369	2806	2808	2812	rBV	206	188	0.01%	0.002%
65	10.446	2826	2832	2836	rVB2	235	258	0.02%	0.003%
66	10.494	2841	2847	2852	rBV3	367	437	0.03%	0.004%
67	10.610	2880	2883	2890	rVB2	268	300	0.02%	0.003%
68	10.642	2890	2893	2895	rBV2	377	197	0.01%	0.002%
69	10.674	2895	2903	2912	rVV2	4464	6707	0.50%	0.068%
70	10.761	2917	2930	2951	rVV	422554	672733	49.92%	6.777%
71	10.873	2959	2965	2969	rBV2	866	947	0.07%	0.010%
72	10.928	2978	2982	2988	rVB3	323	331	0.02%	0.003%
73	11.092	3029	3033	3035	rBV	241	228	0.02%	0.002%
74	11.211	3063	3070	3078	rBV3	410	544	0.04%	0.005%
75	11.381	3121	3123	3126	rVV4	393	254	0.02%	0.003%
76	11.462	3136	3148	3161	rBV6	3261	5791	0.43%	0.058%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045088.D
 Acq On : 04 Oct 2021 11:56
 Operator : SY/MD
 Sample : VU1004WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK009

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.520	3162	3166	3169	rBV2	164	153	0.01%	0.002%
78	11.571	3178	3182	3183	rBV	305	225	0.02%	0.002%
79	11.584	3184	3186	3192	rVB2	479	467	0.03%	0.005%
80	11.700	3214	3222	3230	rBV5	1658	2462	0.18%	0.025%
81	11.748	3230	3237	3244	rBV5	719	859	0.06%	0.009%
82	11.816	3245	3258	3273	rBV	479434	761308	56.49%	7.669%
83	11.928	3288	3293	3294	rBV3	730	579	0.04%	0.006%
84	11.973	3304	3307	3317	rVB4	2972	4179	0.31%	0.042%
85	12.012	3317	3319	3327	rBV3	261	249	0.02%	0.003%
86	12.082	3338	3341	3345	rBV	329	273	0.02%	0.003%
87	12.198	3357	3377	3396	rBV	565691	919266	68.21%	9.260%
88	12.340	3415	3421	3428	rVB3	807	1081	0.08%	0.011%
89	12.513	3471	3475	3476	rBV2	259	217	0.02%	0.002%
90	12.893	3591	3593	3599	rBV2	181	199	0.01%	0.002%
91	12.970	3615	3617	3621	rVB	320	197	0.01%	0.002%
92	13.060	3640	3645	3648	rBV2	200	197	0.01%	0.002%
93	13.217	3692	3694	3696	rBV2	449	300	0.02%	0.003%
94	13.436	3757	3762	3763	rBV	195	174	0.01%	0.002%
95	13.725	3849	3852	3855	rBV2	273	226	0.02%	0.002%
96	13.754	3859	3861	3867	rVV	235	220	0.02%	0.002%
97	13.851	3882	3891	3899	rVB5	1684	2252	0.17%	0.023%
98	14.095	3956	3967	3979	rBV	5549	9041	0.67%	0.091%
99	14.336	4036	4042	4049	rVB3	2254	2617	0.19%	0.026%
100	14.735	4163	4166	4168	rBV2	275	172	0.01%	0.002%




Sum of corrected areas: 9927283

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045088.D
Acq On : 04 Oct 2021 11:56
Operator : SY/MD
Sample : VU1004WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK009

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

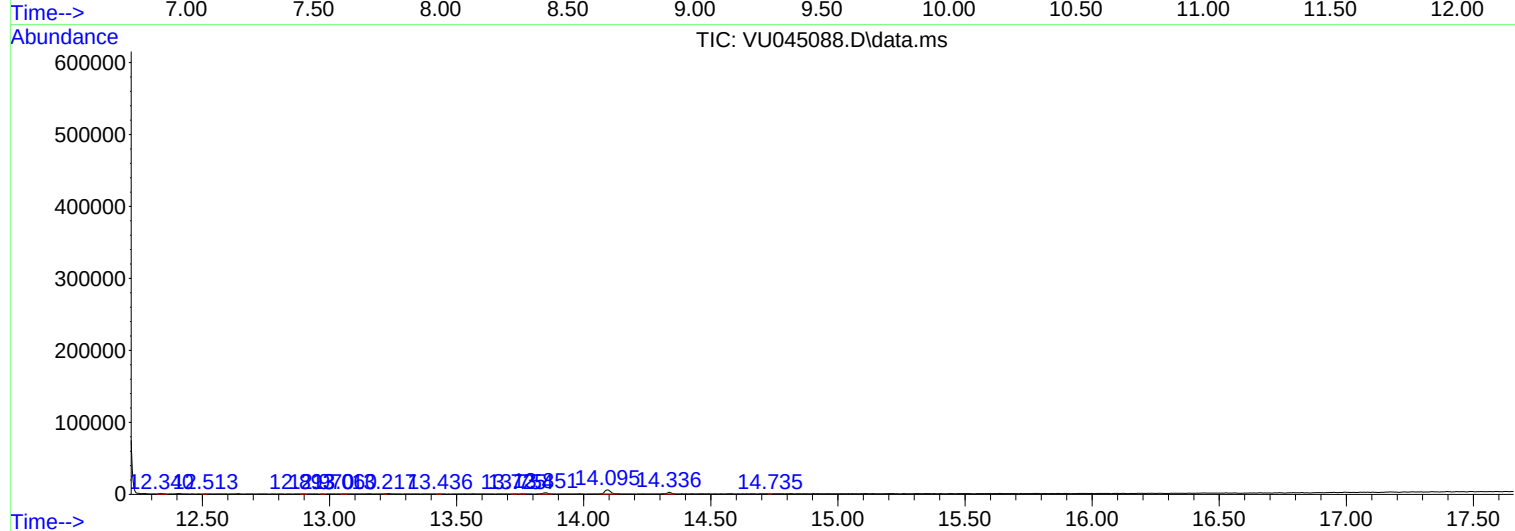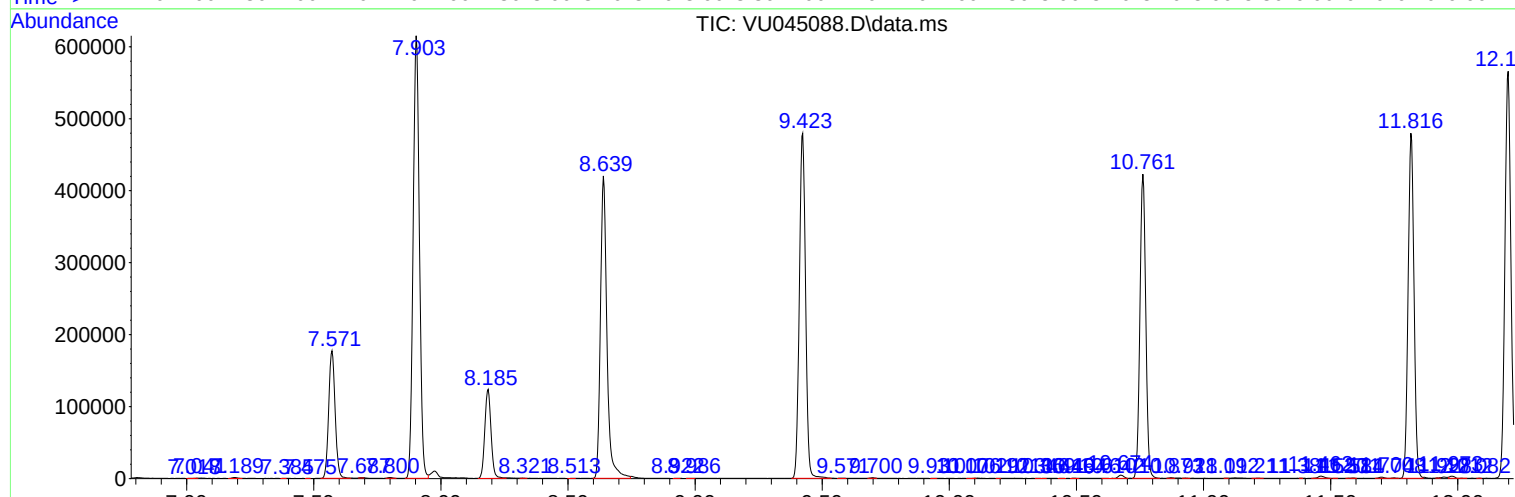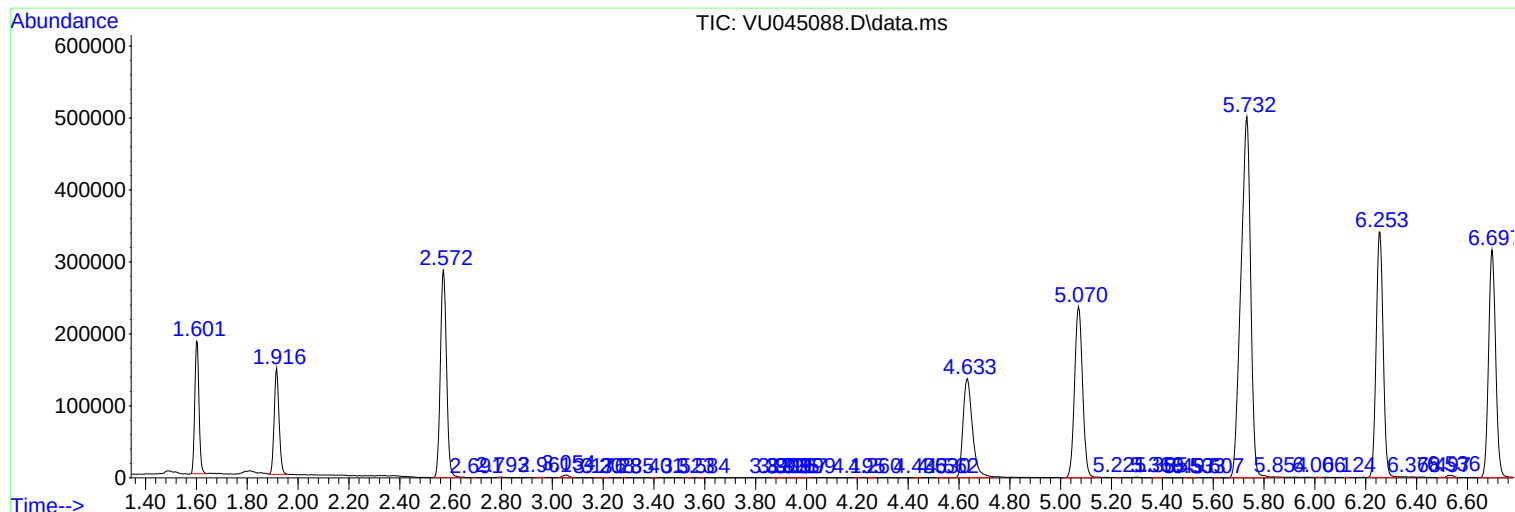

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045088.D
Acq On : 04 Oct 2021 11:56
Operator : SY/MD
Sample : VU1004WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK009

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045088.D
Acq On : 04 Oct 2021 11:56
Operator : SY/MD
Sample : VU1004WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK009

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
