

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045089.D
 Acq On : 04 Oct 2021 12:29
 Operator : SY/MD
 Sample : M3997-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	38	42	64	rVB5	10820	20636	1.02%	0.189%
2	1.601	74	81	98	rBV	133769	153123	7.57%	1.406%
3	1.909	169	177	190	rVB	114608	153992	7.61%	1.413%
4	2.572	370	383	398	rBV	222332	370324	18.30%	3.399%
5	2.787	446	450	451	rBV	384	244	0.01%	0.002%
6	2.890	480	482	488	rVV	166	195	0.01%	0.002%
7	2.925	488	493	497	rVB2	192	203	0.01%	0.002%
8	2.961	497	504	514	rVB3	566	1200	0.06%	0.011%
9	3.038	526	528	529	rBV	318	156	0.01%	0.001%
10	3.147	559	562	565	rVB	184	140	0.01%	0.001%
11	3.192	565	576	588	rBV3	1412	3187	0.16%	0.029%
12	3.266	595	599	603	rVB2	250	221	0.01%	0.002%
13	3.292	603	607	612	rBV2	185	231	0.01%	0.002%
14	3.321	612	616	618	rBV	154	154	0.01%	0.001%
15	3.372	622	632	644	rVB3	2788	6222	0.31%	0.057%
16	3.469	656	662	665	rBV2	171	162	0.01%	0.001%
17	3.755	748	751	756	rBV	197	205	0.01%	0.002%
18	3.848	776	780	782	rBV2	152	140	0.01%	0.001%
19	4.064	843	847	852	rBV2	160	233	0.01%	0.002%
20	4.176	876	882	887	rBV	281	478	0.02%	0.004%
21	4.391	941	949	951	rBV2	186	288	0.01%	0.003%
22	4.629	1008	1023	1057	rBV	131293	321315	15.88%	2.949%
23	5.070	1142	1160	1179	rBV	207130	457471	22.61%	4.199%
24	5.182	1193	1195	1199	rVB2	330	195	0.01%	0.002%
25	5.211	1202	1204	1207	rBV2	362	187	0.01%	0.002%
26	5.231	1207	1210	1213	rVV3	265	172	0.01%	0.002%
27	5.289	1223	1228	1231	rBV	584	609	0.03%	0.006%
28	5.385	1252	1258	1261	rBV3	313	226	0.01%	0.002%
29	5.584	1317	1320	1326	rVV2	232	280	0.01%	0.003%
30	5.732	1342	1366	1400	rBV2	418256	1152207	56.95%	10.576%
31	5.957	1433	1436	1440	rBV3	232	195	0.01%	0.002%
32	6.044	1460	1463	1465	rBV2	263	168	0.01%	0.002%
33	6.086	1473	1476	1480	rBV2	199	143	0.01%	0.001%
34	6.112	1480	1484	1488	rBV2	336	376	0.02%	0.003%
35	6.176	1501	1504	1505	rBV	284	205	0.01%	0.002%
36	6.186	1505	1507	1509	rVV	327	151	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045089.D
 Acq On : 04 Oct 2021 12:29
 Operator : SY/MD
 Sample : M3997-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.205	1509	1513	1514	rVV2	257	199	0.01%	0.002%
38	6.253	1514	1528	1550	rVV	344790	648664	32.06%	5.954%
39	6.543	1605	1618	1632	rVB9	5378	10337	0.51%	0.095%
40	6.697	1650	1666	1692	rBV	279349	537334	26.56%	4.932%
41	6.803	1692	1699	1700	rBV3	635	569	0.03%	0.005%
42	7.034	1767	1771	1772	rBV	395	252	0.01%	0.002%
43	7.121	1796	1798	1804	rVB2	179	170	0.01%	0.002%
44	7.240	1829	1835	1837	rBV2	230	206	0.01%	0.002%
45	7.401	1881	1885	1889	rVB2	252	251	0.01%	0.002%
46	7.436	1890	1896	1900	rBB2	143	159	0.01%	0.001%
47	7.481	1907	1910	1913	rBV2	208	165	0.01%	0.002%
48	7.571	1923	1938	1964	rBV	151799	265822	13.14%	2.440%
49	7.694	1969	1976	1984	rVB3	1362	2072	0.10%	0.019%
50	7.758	1994	1996	1999	rBV2	188	157	0.01%	0.001%
51	7.796	2003	2008	2021	rVB5	879	1370	0.07%	0.013%
52	7.854	2021	2026	2027	rBV	213	182	0.01%	0.002%
53	7.903	2027	2041	2056	rBV	501811	855673	42.29%	7.854%
54	8.121	2106	2109	2114	rVB2	178	149	0.01%	0.001%
55	8.186	2117	2129	2148	rBV	105451	178730	8.83%	1.641%
56	8.401	2191	2196	2200	rBV2	173	195	0.01%	0.002%
57	8.430	2200	2205	2209	rBV2	231	221	0.01%	0.002%
58	8.468	2214	2217	2218	rBV	349	200	0.01%	0.002%
59	8.559	2230	2245	2259	rBV	1201998	2023138	100.00%	18.570%
60	8.639	2259	2270	2311	rVB	422107	739353	36.54%	6.787%
61	8.986	2374	2378	2381	rBV2	351	312	0.02%	0.003%
62	9.208	2443	2447	2450	rBV2	175	165	0.01%	0.002%
63	9.288	2469	2472	2475	rVB2	221	161	0.01%	0.001%
64	9.420	2501	2513	2534	rBV	483281	797887	39.44%	7.324%
65	9.578	2557	2562	2565	rVB	411	394	0.02%	0.004%
66	9.697	2593	2599	2606	rBV2	782	1050	0.05%	0.010%
67	9.751	2610	2616	2619	rBV2	177	225	0.01%	0.002%
68	9.870	2648	2653	2659	rVB2	187	241	0.01%	0.002%
69	9.980	2685	2687	2690	rBV	339	224	0.01%	0.002%
70	10.031	2698	2703	2707	rBV2	239	316	0.02%	0.003%
71	10.060	2707	2712	2714	rVB2	146	152	0.01%	0.001%
72	10.102	2720	2725	2728	rBV	363	304	0.02%	0.003%
73	10.343	2797	2800	2804	rBV2	182	165	0.01%	0.002%
74	10.362	2804	2806	2809	rBV	190	147	0.01%	0.001%
75	10.491	2842	2846	2850	rBV2	276	249	0.01%	0.002%
76	10.558	2864	2867	2870	rBV	203	144	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045089.D
 Acq On : 04 Oct 2021 12:29
 Operator : SY/MD
 Sample : M3997-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.674	2897	2903	2910	rVB2	2076	2595	0.13%	0.024%
78	10.761	2917	2930	2951	rBV	391768	622245	30.76%	5.712%
79	10.867	2956	2963	2965	rBV3	451	422	0.02%	0.004%
80	11.044	3014	3018	3023	rBV2	262	324	0.02%	0.003%
81	11.102	3031	3036	3039	rBV2	357	435	0.02%	0.004%
82	11.182	3058	3061	3064	rBV2	248	226	0.01%	0.002%
83	11.272	3085	3089	3095	rBV2	191	212	0.01%	0.002%
84	11.324	3102	3105	3110	rVV2	171	193	0.01%	0.002%
85	11.462	3143	3148	3161	rVB6	1723	2788	0.14%	0.026%
86	11.581	3182	3185	3188	rBV2	252	165	0.01%	0.002%
87	11.664	3208	3211	3213	rVV	250	182	0.01%	0.002%
88	11.677	3213	3215	3217	rVV	288	169	0.01%	0.002%
89	11.697	3217	3221	3228	rVB4	959	1039	0.05%	0.010%
90	11.816	3245	3258	3278	rBV	484092	750946	37.12%	6.893%
91	11.973	3303	3307	3317	rVB5	1313	1840	0.09%	0.017%
92	12.198	3363	3377	3397	rBV	489393	790760	39.09%	7.258%
93	12.340	3416	3421	3423	rVB3	523	436	0.02%	0.004%
94	12.410	3441	3443	3448	rBV2	420	348	0.02%	0.003%
95	12.446	3451	3454	3456	rBV	219	168	0.01%	0.002%
96	13.227	3694	3697	3702	rVB2	386	367	0.02%	0.003%
97	13.449	3762	3766	3769	rBV2	218	222	0.01%	0.002%
98	13.664	3830	3833	3835	rBV2	210	173	0.01%	0.002%
99	14.095	3960	3967	3977	rVB2	2490	3612	0.18%	0.033%
100	14.333	4038	4041	4049	rVB3	1165	1230	0.06%	0.011%




Sum of corrected areas: 10894435

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045089.D
Acq On : 04 Oct 2021 12:29
Operator : SY/MD
Sample : M3997-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

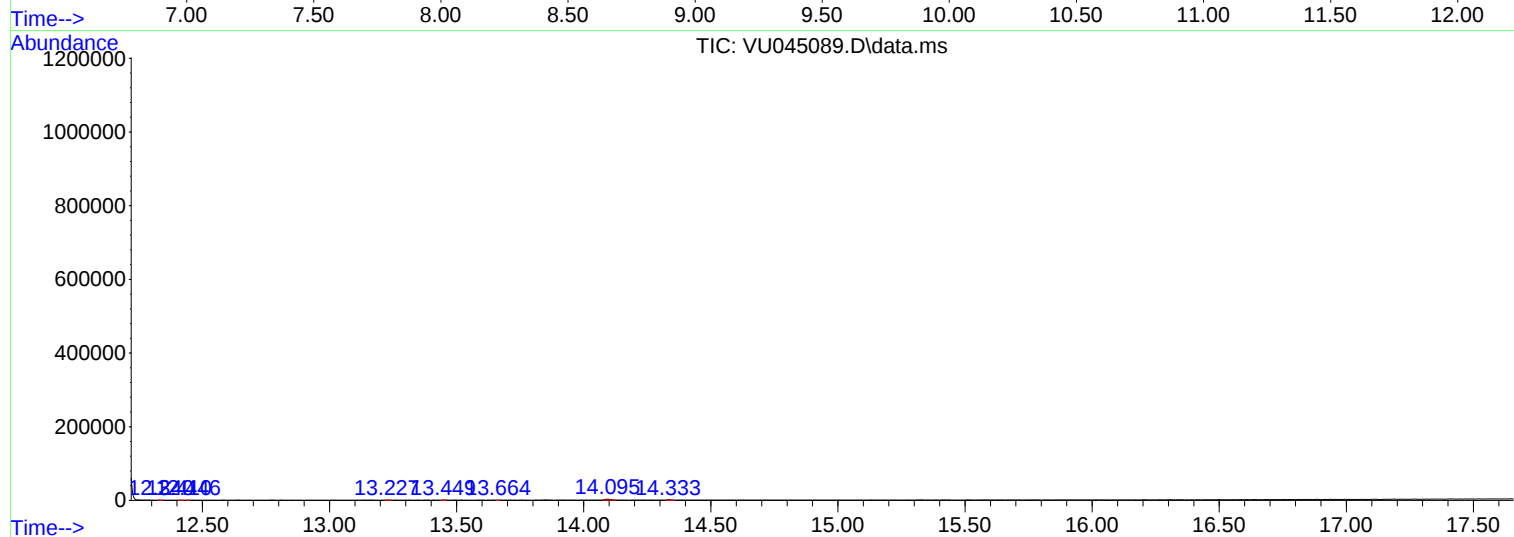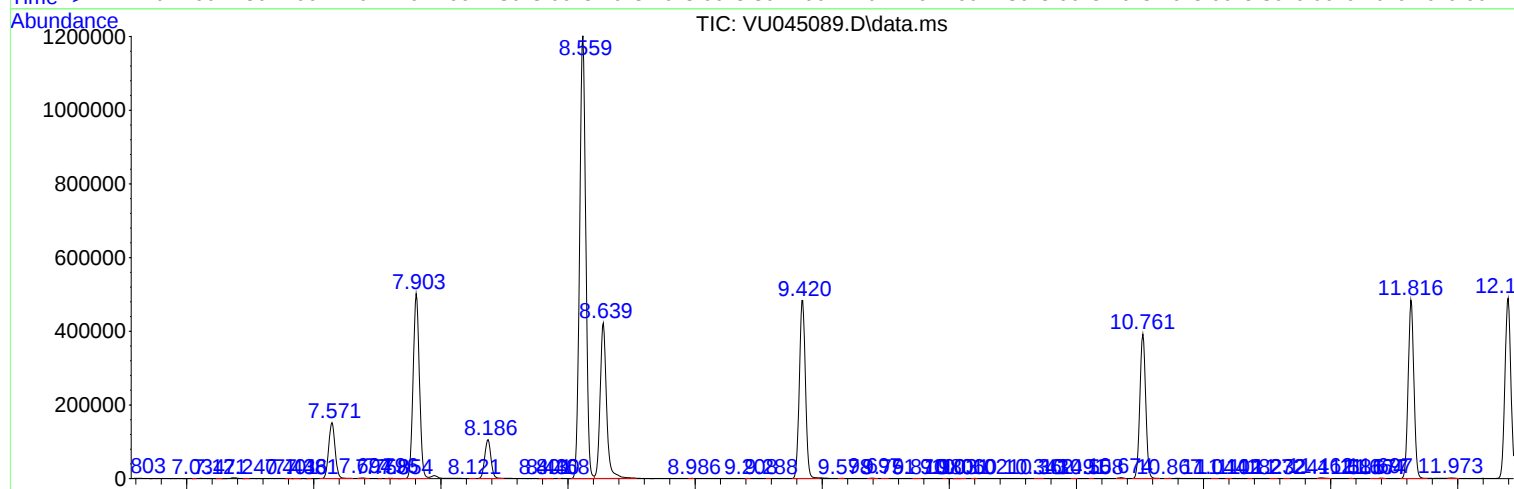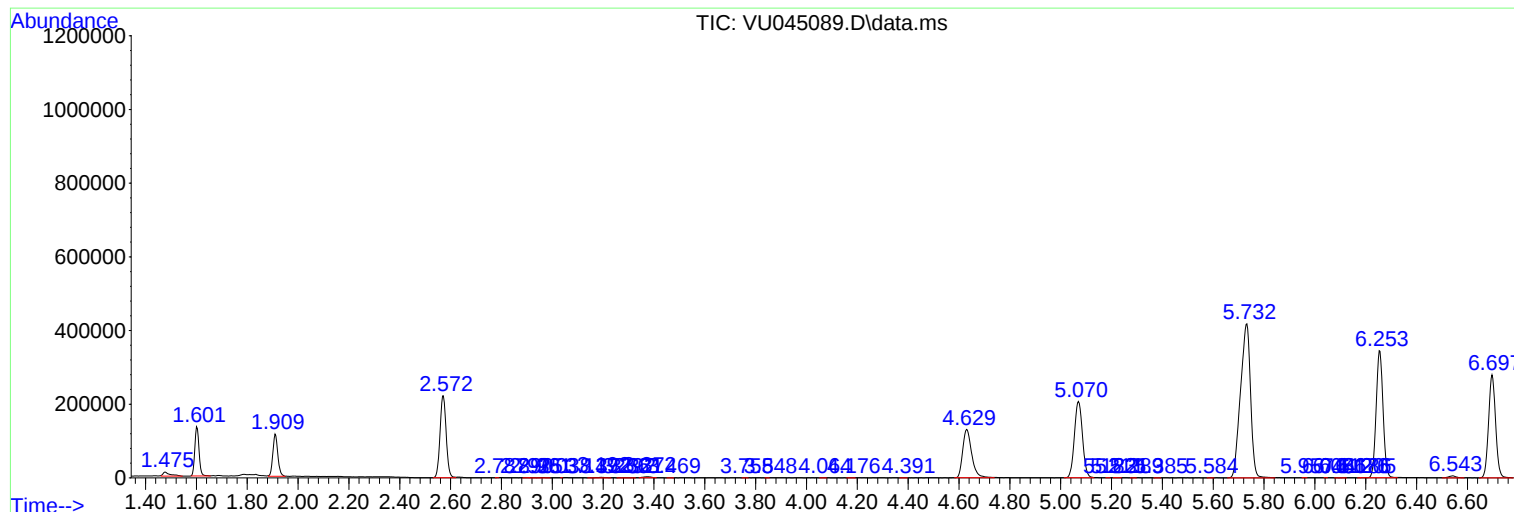

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045089.D
Acq On : 04 Oct 2021 12:29
Operator : SY/MD
Sample : M3997-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045089.D
Acq On : 04 Oct 2021 12:29
Operator : SY/MD
Sample : M3997-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc