

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045090.D
 Acq On : 04 Oct 2021 12:52
 Operator : SY/MD
 Sample : M3997-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rBV	168269	192520	14.73%	2.040%
2	1.909	169	177	191	rVB	133144	183670	14.05%	1.947%
3	2.568	369	382	412	rVV	267714	448040	34.27%	4.749%
4	2.797	447	453	459	rVV2	528	690	0.05%	0.007%
5	2.884	476	480	484	rVB	209	188	0.01%	0.002%
6	2.957	496	503	511	rBV3	447	855	0.07%	0.009%
7	3.051	523	532	542	rVB2	3844	6705	0.51%	0.071%
8	3.234	581	589	590	rBV	193	232	0.02%	0.002%
9	3.337	613	621	623	rBV2	197	317	0.02%	0.003%
10	3.398	634	640	644	rBV	227	272	0.02%	0.003%
11	3.427	644	649	651	rBV	146	176	0.01%	0.002%
12	3.646	712	717	722	rBV2	193	207	0.02%	0.002%
13	3.935	805	807	812	rVB2	260	174	0.01%	0.002%
14	4.031	836	837	843	rVB	162	152	0.01%	0.002%
15	4.086	851	854	858	rBV2	246	228	0.02%	0.002%
16	4.199	884	889	891	rBV2	195	160	0.01%	0.002%
17	4.244	901	903	910	rVB2	170	161	0.01%	0.002%
18	4.549	991	998	1001	rBV2	228	267	0.02%	0.003%
19	4.633	1007	1024	1062	rBV	138702	357126	27.32%	3.785%
20	4.777	1066	1069	1072	rBV4	271	186	0.01%	0.002%
21	4.951	1120	1123	1126	rVB2	292	171	0.01%	0.002%
22	5.070	1141	1160	1181	rBV	229498	503506	38.51%	5.336%
23	5.189	1195	1197	1200	rVB2	278	178	0.01%	0.002%
24	5.208	1200	1203	1205	rBV2	250	149	0.01%	0.002%
25	5.295	1224	1230	1237	rVB3	633	954	0.07%	0.010%
26	5.375	1251	1255	1266	rVB3	397	647	0.05%	0.007%
27	5.456	1277	1280	1286	rBV	184	241	0.02%	0.003%
28	5.729	1342	1365	1388	rBV2	480461	1307415	100.00%	13.857%
29	5.967	1436	1439	1442	rBV2	284	195	0.01%	0.002%
30	6.089	1473	1477	1480	rBV	262	218	0.02%	0.002%
31	6.144	1492	1494	1498	rBV3	235	196	0.01%	0.002%
32	6.253	1512	1528	1547	rBV	326620	610617	46.70%	6.472%
33	6.440	1583	1586	1591	rVB2	279	252	0.02%	0.003%
34	6.472	1594	1596	1598	rBV	328	177	0.01%	0.002%
35	6.488	1598	1601	1606	rVB2	226	221	0.02%	0.002%
36	6.536	1606	1616	1624	rBV4	3223	5143	0.39%	0.055%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045090.D
 Acq On : 04 Oct 2021 12:52
 Operator : SY/MD
 Sample : M3997-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.588	1626	1632	1635	rBV2	246	308	0.02%	0.003%
38	6.697	1650	1666	1688	rBV	307184	601031	45.97%	6.370%
39	6.806	1695	1700	1702	rBV2	779	680	0.05%	0.007%
40	6.864	1715	1718	1721	rBV2	223	206	0.02%	0.002%
41	6.906	1726	1731	1735	rBV2	161	236	0.02%	0.003%
42	6.973	1750	1752	1755	rVB	230	153	0.01%	0.002%
43	7.054	1771	1777	1783	rVB3	751	1068	0.08%	0.011%
44	7.086	1783	1787	1791	rVB2	217	222	0.02%	0.002%
45	7.105	1791	1793	1796	rBV2	189	154	0.01%	0.002%
46	7.186	1810	1818	1827	rVV2	1315	2148	0.16%	0.023%
47	7.401	1881	1885	1888	rVB2	170	157	0.01%	0.002%
48	7.469	1903	1906	1910	rVB2	217	187	0.01%	0.002%
49	7.504	1913	1917	1921	rVB2	231	191	0.01%	0.002%
50	7.571	1925	1938	1954	rBV	170597	298132	22.80%	3.160%
51	7.694	1968	1976	1985	rVB3	920	1671	0.13%	0.018%
52	7.800	2004	2009	2016	rVB3	604	706	0.05%	0.007%
53	7.903	2026	2041	2056	rBV	578909	987288	75.51%	10.464%
54	7.973	2057	2063	2074	rVB	8222	13269	1.01%	0.141%
55	8.182	2115	2128	2149	rBV	120203	201779	15.43%	2.139%
56	8.559	2238	2245	2252	rBV2	1700	2083	0.16%	0.022%
57	8.639	2257	2270	2299	rBV	428007	740708	56.65%	7.850%
58	9.076	2403	2406	2413	rBV2	239	345	0.03%	0.004%
59	9.349	2487	2491	2495	rBV	152	171	0.01%	0.002%
60	9.420	2500	2513	2541	rBV	455260	749869	57.36%	7.948%
61	9.568	2554	2559	2566	rVV2	316	463	0.04%	0.005%
62	9.652	2574	2585	2588	rBV2	326	583	0.04%	0.006%
63	9.681	2591	2594	2595	rVV2	321	215	0.02%	0.002%
64	9.697	2595	2599	2606	rVB4	903	1109	0.08%	0.012%
65	9.944	2671	2676	2679	rBV2	155	164	0.01%	0.002%
66	10.105	2723	2726	2730	rBV	335	250	0.02%	0.003%
67	10.237	2761	2767	2770	rBV2	293	336	0.03%	0.004%
68	10.452	2830	2834	2839	rBV2	161	226	0.02%	0.002%
69	10.571	2868	2871	2874	rBV2	273	212	0.02%	0.002%
70	10.642	2888	2893	2895	rBV2	327	278	0.02%	0.003%
71	10.674	2896	2903	2911	rVB	3847	5499	0.42%	0.058%
72	10.761	2917	2930	2950	rBV	412127	669347	51.20%	7.094%
73	10.874	2959	2965	2967	rBV3	682	729	0.06%	0.008%
74	10.960	2989	2992	2996	rBV2	156	149	0.01%	0.002%
75	11.047	3015	3019	3021	rBV2	243	219	0.02%	0.002%
76	11.124	3036	3043	3047	rBV6	721	882	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045090.D
 Acq On : 04 Oct 2021 12:52
 Operator : SY/MD
 Sample : M3997-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

77	11.147	3047	3050	3051	rBV	315	186	0.01%	0.002%
78	11.205	3066	3068	3071	rVB2	272	169	0.01%	0.002%
79	11.285	3090	3093	3095	rBV	261	160	0.01%	0.002%
80	11.391	3123	3126	3129	rBV3	365	286	0.02%	0.003%
81	11.462	3138	3148	3159	rVB6	2603	4956	0.38%	0.053%
82	11.517	3159	3165	3167	rBV2	277	358	0.03%	0.004%
83	11.578	3179	3184	3185	rBV	282	212	0.02%	0.002%
84	11.700	3216	3222	3230	rVB5	1455	1975	0.15%	0.021%
85	11.816	3245	3258	3273	rBV	426371	670369	51.27%	7.105%
86	11.941	3293	3297	3298	rBV	805	533	0.04%	0.006%
87	12.195	3360	3376	3399	rBV	518373	843523	64.52%	8.940%
88	12.327	3414	3417	3418	rBV	506	267	0.02%	0.003%
89	12.375	3425	3432	3435	rBV2	281	361	0.03%	0.004%
90	12.401	3437	3440	3445	rVB2	378	326	0.02%	0.003%
91	12.636	3511	3513	3515	rBV2	275	152	0.01%	0.002%
92	12.906	3594	3597	3600	rBV2	365	304	0.02%	0.003%
93	13.044	3635	3640	3644	rBV	230	322	0.02%	0.003%
94	13.099	3655	3657	3662	rBV	207	194	0.01%	0.002%
95	13.150	3669	3673	3675	rBV2	397	326	0.02%	0.003%
96	13.844	3886	3889	3897	rVB4	416	471	0.04%	0.005%
97	14.092	3959	3966	3976	rBV3	1592	2380	0.18%	0.025%
98	14.340	4038	4043	4049	rBV4	464	561	0.04%	0.006%
99	14.848	4198	4201	4202	rBV2	365	220	0.02%	0.002%
100	15.060	4262	4267	4272	rBV2	440	556	0.04%	0.006%




Sum of corrected areas: 9435196

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045090.D
Acq On : 04 Oct 2021 12:52
Operator : SY/MD
Sample : M3997-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

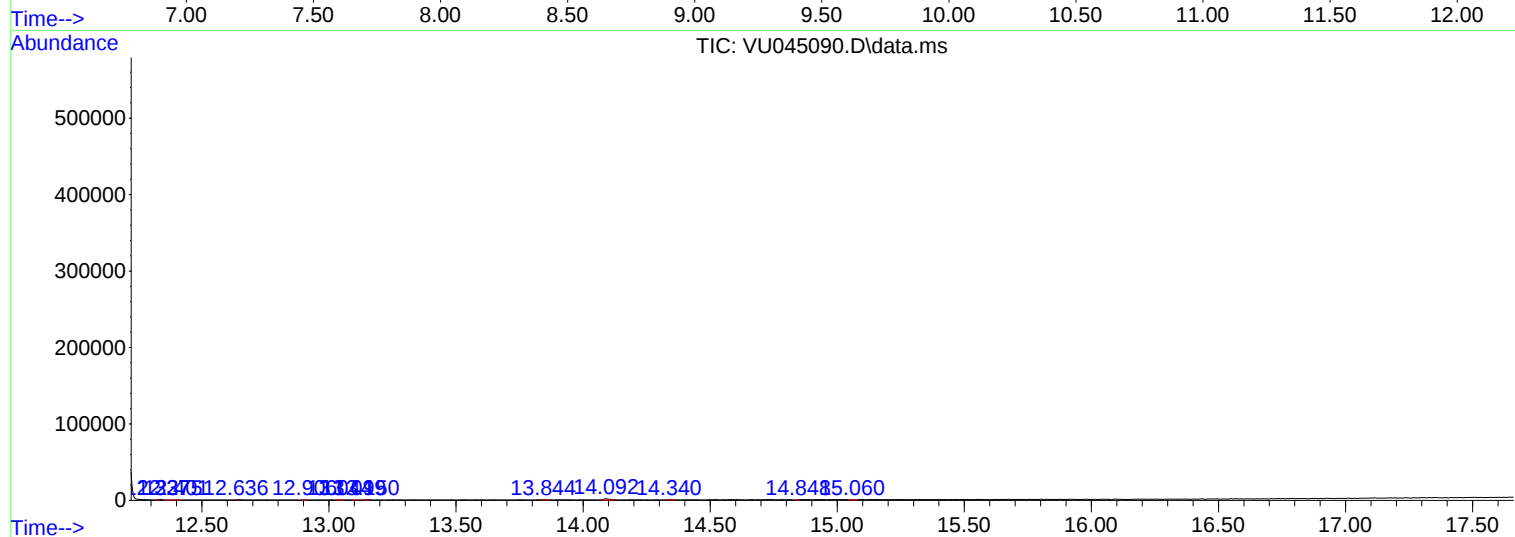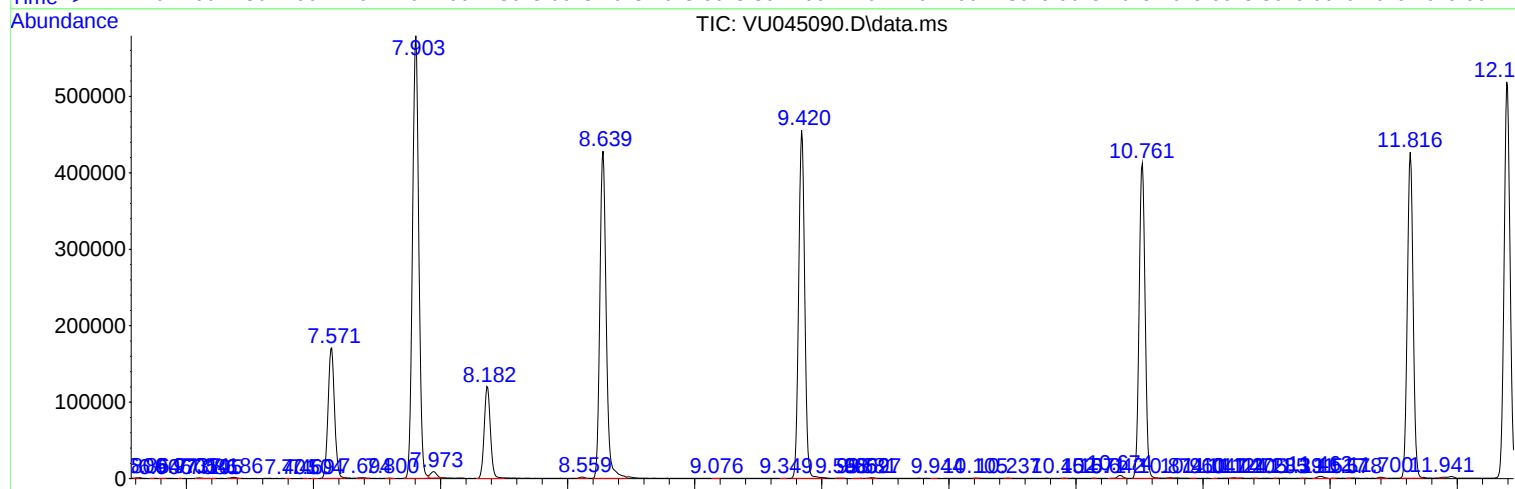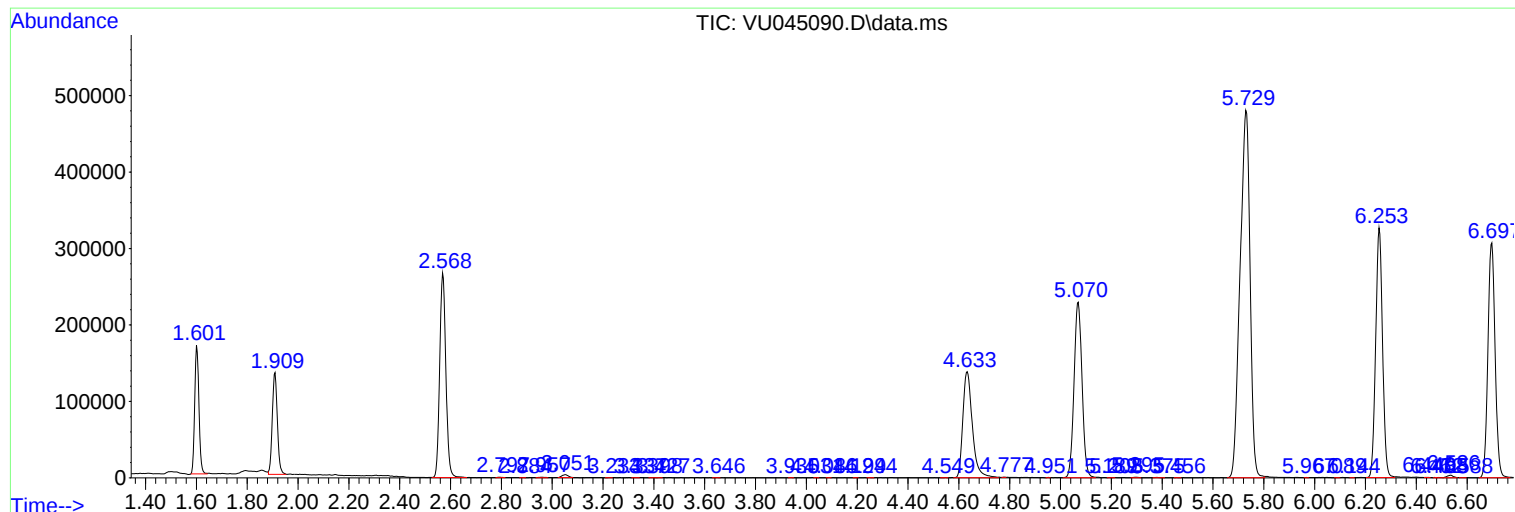

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045090.D
Acq On : 04 Oct 2021 12:52
Operator : SY/MD
Sample : M3997-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045090.D
Acq On : 04 Oct 2021 12:52
Operator : SY/MD
Sample : M3997-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------