

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045092.D
 Acq On : 04 Oct 2021 13:38
 Operator : SY/MD
 Sample : M3996-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU045092.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	37	42	51	rBV	18057	19504	1.62%	0.197%
2	1.601	72	81	93	rVB	151378	185925	15.42%	1.882%
3	1.913	170	178	193	rVB	120558	163568	13.57%	1.655%
4	2.572	370	383	396	rBV	229514	385707	31.99%	3.903%
5	2.639	397	404	420	rVB	11830	22190	1.84%	0.225%
6	2.739	431	435	439	rBV2	178	188	0.02%	0.002%
7	2.797	443	453	471	rVV	6136	11049	0.92%	0.112%
8	2.887	475	481	486	rBV2	205	345	0.03%	0.003%
9	2.951	498	501	503	rBV	359	224	0.02%	0.002%
10	3.002	514	517	519	rBV2	186	135	0.01%	0.001%
11	3.051	526	532	537	rBV2	477	546	0.05%	0.006%
12	3.089	541	544	546	rBV2	207	130	0.01%	0.001%
13	3.192	561	576	597	rBV	14499	34651	2.87%	0.351%
14	3.372	620	632	647	rVB3	4653	10313	0.86%	0.104%
15	3.456	652	658	662	rVB2	182	245	0.02%	0.002%
16	3.498	668	671	675	rVB	186	136	0.01%	0.001%
17	3.530	678	681	685	rVB2	214	154	0.01%	0.002%
18	3.620	706	709	711	rBV2	176	147	0.01%	0.001%
19	3.652	717	719	725	rVB2	155	183	0.02%	0.002%
20	3.723	736	741	745	rVB2	153	158	0.01%	0.002%
21	3.838	772	777	780	rBV2	118	143	0.01%	0.001%
22	4.102	856	859	862	rBV2	196	175	0.01%	0.002%
23	4.199	882	889	893	rBV	220	326	0.03%	0.003%
24	4.321	924	927	929	rBV	183	132	0.01%	0.001%
25	4.337	929	932	936	rVB2	175	132	0.01%	0.001%
26	4.372	936	943	946	rBV	134	173	0.01%	0.002%
27	4.420	952	958	962	rBV2	297	332	0.03%	0.003%
28	4.578	1003	1007	1009	rBV2	166	152	0.01%	0.002%
29	4.633	1009	1024	1061	rBV	144343	391970	32.51%	3.967%
30	4.877	1097	1100	1104	rBV2	254	157	0.01%	0.002%
31	4.928	1112	1116	1119	rBV2	193	169	0.01%	0.002%
32	4.986	1129	1134	1138	rBV3	204	179	0.01%	0.002%
33	5.070	1141	1160	1181	rBV	219067	477046	39.56%	4.828%
34	5.244	1211	1214	1219	rVB2	278	180	0.01%	0.002%
35	5.282	1223	1226	1228	rVV	334	236	0.02%	0.002%
36	5.301	1228	1232	1237	rVB3	520	628	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045092.D
 Acq On : 04 Oct 2021 13:38
 Operator : SY/MD
 Sample : M3996-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.382	1255	1257	1263	rVV4	318	245	0.02%	0.002%
38	5.491	1288	1291	1293	rBV	160	133	0.01%	0.001%
39	5.578	1315	1318	1321	rVB2	258	173	0.01%	0.002%
40	5.600	1321	1325	1327	rBV	165	142	0.01%	0.001%
41	5.729	1340	1365	1394	rBV2	437472	1205801	100.00%	12.203%
42	6.028	1453	1458	1461	rBV3	163	211	0.02%	0.002%
43	6.051	1461	1465	1467	rBV	234	237	0.02%	0.002%
44	6.163	1490	1500	1509	rVV2	2551	5108	0.42%	0.052%
45	6.253	1514	1528	1548	rBV	331132	631695	52.39%	6.393%
46	6.501	1601	1605	1607	rBV	202	136	0.01%	0.001%
47	6.546	1607	1619	1631	rVV4	20032	38928	3.23%	0.394%
48	6.697	1650	1666	1686	rBV	286224	561293	46.55%	5.680%
49	7.186	1809	1818	1828	rVB5	2644	4252	0.35%	0.043%
50	7.571	1924	1938	1955	rBV	156928	274298	22.75%	2.776%
51	7.633	1955	1957	1962	rVB3	574	416	0.03%	0.004%
52	7.690	1968	1975	1976	rBV3	1255	1428	0.12%	0.014%
53	7.903	2027	2041	2056	rBV	522373	888682	73.70%	8.993%
54	7.970	2057	2062	2073	rVB	8297	13437	1.11%	0.136%
55	8.182	2116	2128	2153	rBV	108133	186606	15.48%	1.888%
56	8.475	2216	2219	2226	rVB2	252	203	0.02%	0.002%
57	8.555	2231	2244	2258	rBV	351089	590564	48.98%	5.976%
58	8.639	2258	2270	2300	rVV	457382	785745	65.16%	7.952%
59	8.851	2333	2336	2339	rVB2	239	143	0.01%	0.001%
60	8.890	2345	2348	2354	rBV2	159	128	0.01%	0.001%
61	9.321	2478	2482	2485	rBV	175	179	0.01%	0.002%
62	9.420	2499	2513	2552	rBV	474709	776851	64.43%	7.862%
63	9.600	2566	2569	2570	rBV2	230	135	0.01%	0.001%
64	9.697	2593	2599	2606	rVB3	991	1145	0.09%	0.012%
65	9.793	2628	2629	2636	rVB2	239	157	0.01%	0.002%
66	9.845	2636	2645	2648	rBV2	190	349	0.03%	0.004%
67	9.883	2655	2657	2663	rBV2	151	160	0.01%	0.002%
68	9.919	2663	2668	2669	rBV	141	140	0.01%	0.001%
69	10.134	2721	2735	2744	rBV3	5767	9632	0.80%	0.097%
70	10.221	2758	2762	2763	rBV	326	191	0.02%	0.002%
71	10.237	2763	2767	2776	rVB2	666	1034	0.09%	0.010%
72	10.533	2855	2859	2866	rBV2	275	379	0.03%	0.004%
73	10.674	2896	2903	2911	rVB3	1601	2444	0.20%	0.025%
74	10.758	2917	2929	2951	rVB	408017	655015	54.32%	6.629%
75	10.851	2955	2958	2961	rBV	159	159	0.01%	0.002%
76	10.870	2961	2964	2966	rBV	278	165	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045092.D
 Acq On : 04 Oct 2021 13:38
 Operator : SY/MD
 Sample : M3996-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.970	2992	2995	3000	rVB	225	210	0.02%	0.002%
78	10.996	3000	3003	3006	rBV3	263	217	0.02%	0.002%
79	11.050	3013	3020	3029	rBV3	1782	2460	0.20%	0.025%
80	11.115	3037	3040	3041	rBV2	223	141	0.01%	0.001%
81	11.214	3066	3071	3075	rBV2	220	237	0.02%	0.002%
82	11.462	3141	3148	3158	rBV4	1440	2225	0.18%	0.023%
83	11.578	3175	3184	3193	rVB2	3745	5505	0.46%	0.056%
84	11.700	3215	3222	3228	rBV5	795	1168	0.10%	0.012%
85	11.816	3245	3258	3279	rBV	449891	702779	58.28%	7.112%
86	11.938	3294	3296	3301	rBV4	352	322	0.03%	0.003%
87	12.066	3326	3336	3352	rBV	9718	17084	1.42%	0.173%
88	12.195	3363	3376	3397	rVB	496484	799044	66.27%	8.086%
89	12.333	3415	3419	3428	rVB2	546	540	0.04%	0.005%
90	12.526	3476	3479	3482	rBV2	253	176	0.01%	0.002%
91	12.681	3523	3527	3530	rBV2	192	166	0.01%	0.002%
92	12.944	3607	3609	3612	rBV	217	172	0.01%	0.002%
93	13.153	3671	3674	3678	rBV3	294	238	0.02%	0.002%
94	13.446	3763	3765	3769	rBV2	211	164	0.01%	0.002%
95	13.600	3809	3813	3819	rBV2	244	282	0.02%	0.003%
96	14.099	3963	3968	3979	rVB3	767	1483	0.12%	0.015%
97	14.340	4041	4043	4046	rBV2	350	177	0.01%	0.002%
98	14.536	4099	4104	4106	rBV2	429	365	0.03%	0.004%
99	14.761	4171	4174	4178	rVB2	390	261	0.02%	0.003%
100	14.790	4179	4183	4187	rBV2	383	378	0.03%	0.004%


Sum of corrected areas: 9881561

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045092.D
Acq On : 04 Oct 2021 13:38
Operator : SY/MD
Sample : M3996-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

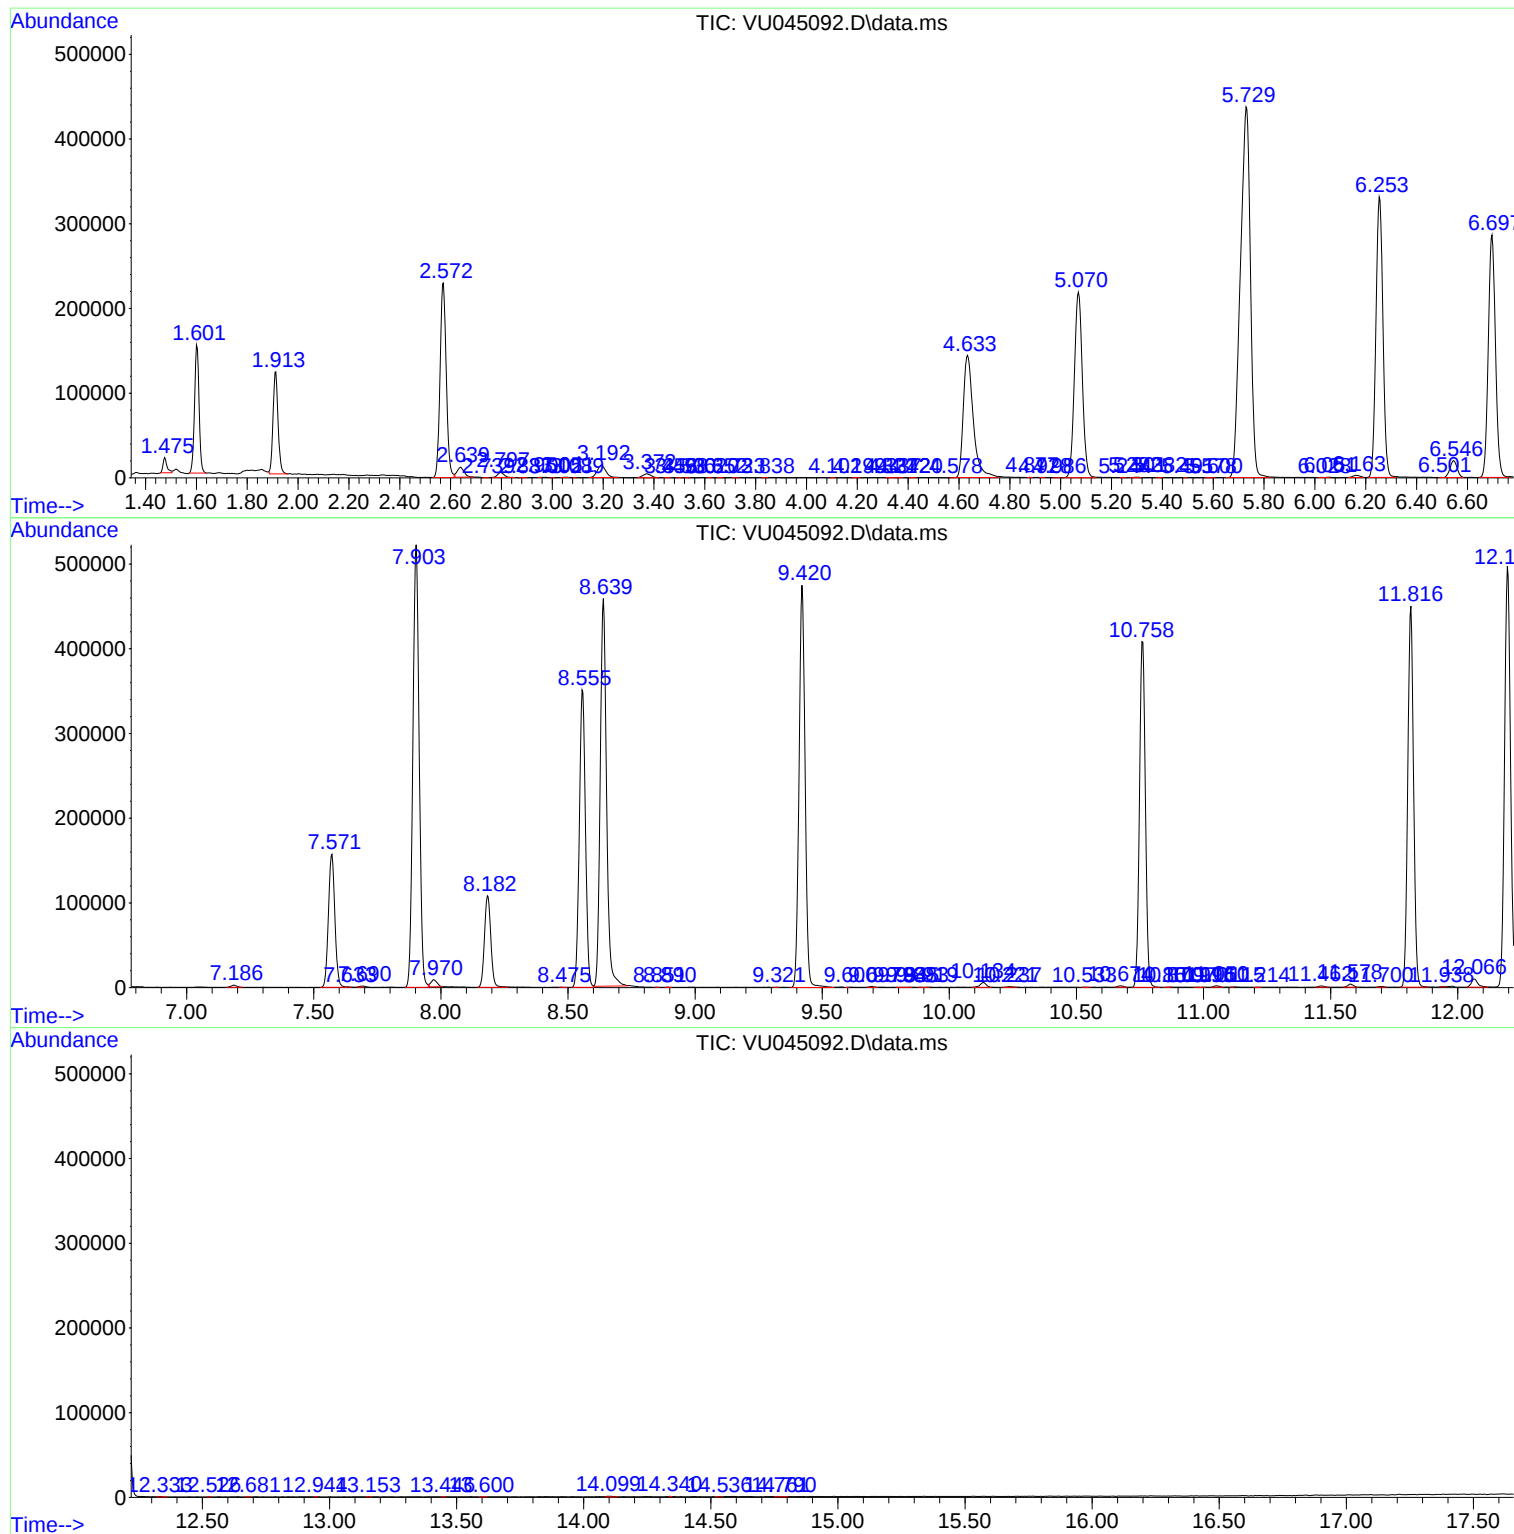

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045092.D
Acq On : 04 Oct 2021 13:38
Operator : SY/MD
Sample : M3996-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045092.D
Acq On : 04 Oct 2021 13:38
Operator : SY/MD
Sample : M3996-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
