

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045112.D
 Acq On : 04 Oct 2021 22:11
 Operator : SY/MD
 Sample : M4023-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	38	45	53	rBV3	6243	13287	0.06%	0.034%
2	1.601	74	81	93	rBV	126294	150360	0.68%	0.385%
3	1.900	166	174	191	rVB	89147	119871	0.54%	0.307%
4	2.501	358	361	369	rVB2	433	419	0.00%	0.001%
5	2.578	369	385	413	rBV4	927471	1680775	7.59%	4.299%
6	2.684	415	418	424	rVB3	361	292	0.00%	0.001%
7	2.781	445	448	449	rBV	446	292	0.00%	0.001%
8	2.903	483	486	493	rBV2	192	199	0.00%	0.001%
9	2.954	496	502	503	rBV2	472	463	0.00%	0.001%
10	3.047	515	531	558	rBV	579478	1143143	5.17%	2.924%
11	3.189	565	575	589	rVB2	1556	3935	0.02%	0.010%
12	3.250	589	594	597	rVB2	192	180	0.00%	0.000%
13	3.356	619	627	638	rVB3	1889	2810	0.01%	0.007%
14	3.539	681	684	688	rBV	197	222	0.00%	0.001%
15	3.588	696	699	707	rVB	228	227	0.00%	0.001%
16	3.691	730	731	735	rVB3	317	184	0.00%	0.000%
17	3.742	742	747	753	rVB2	269	374	0.00%	0.001%
18	3.781	753	759	761	rBV	188	230	0.00%	0.001%
19	3.874	773	788	805	rVB2	24983	58108	0.26%	0.149%
20	4.379	939	945	947	rBV	220	201	0.00%	0.001%
21	4.533	990	993	997	rBV2	155	162	0.00%	0.000%
22	4.668	1006	1035	1072	rBV2	657881	1804120	8.15%	4.615%
23	5.067	1140	1159	1180	rBV	219385	480648	2.17%	1.230%
24	5.215	1202	1205	1210	rVB2	431	323	0.00%	0.001%
25	5.321	1219	1238	1260	rBV	1246389	2796040	12.63%	7.152%
26	5.597	1318	1324	1326	rBV	350	251	0.00%	0.001%
27	5.729	1343	1365	1383	rBV2	436021	1199867	5.42%	3.069%
28	5.967	1434	1439	1441	rBV2	203	184	0.00%	0.000%
29	6.134	1484	1491	1492	rBV5	713	690	0.00%	0.002%
30	6.253	1513	1528	1550	rBV	379200	709111	3.20%	1.814%
31	6.414	1575	1578	1583	rVB2	204	208	0.00%	0.001%
32	6.472	1594	1596	1601	rVB2	309	272	0.00%	0.001%
33	6.549	1601	1620	1652	rBV	11961630	22130540	100.00%	56.611%
34	6.694	1655	1665	1685	rVB	289360	566520	2.56%	1.449%
35	6.986	1753	1756	1760	rVB2	363	280	0.00%	0.001%
36	7.044	1770	1774	1777	rBV	589	423	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045112.D
 Acq On : 04 Oct 2021 22:11
 Operator : SY/MD
 Sample : M4023-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.108	1790	1794	1798	rBV2	216	200	0.00%	0.001%
38	7.186	1810	1818	1827	rVB4	3604	5604	0.03%	0.014%
39	7.247	1834	1837	1841	rVB2	346	275	0.00%	0.001%
40	7.388	1875	1881	1886	rBV2	202	301	0.00%	0.001%
41	7.433	1890	1895	1901	rBV	204	317	0.00%	0.001%
42	7.497	1911	1915	1918	rVB3	403	252	0.00%	0.001%
43	7.568	1923	1937	1955	rBV	158491	281027	1.27%	0.719%
44	7.687	1966	1974	1984	rVB4	1562	2891	0.01%	0.007%
45	7.803	1996	2010	2018	rBV4	1279	2226	0.01%	0.006%
46	7.899	2025	2040	2054	rBV	525447	899237	4.06%	2.300%
47	7.973	2054	2063	2075	rVV	25664	44955	0.20%	0.115%
48	8.031	2078	2081	2085	rVV2	310	376	0.00%	0.001%
49	8.131	2106	2112	2117	rBV3	822	862	0.00%	0.002%
50	8.182	2117	2128	2146	rVV	112712	187315	0.85%	0.479%
51	8.404	2186	2197	2209	rVB2	20785	34785	0.16%	0.089%
52	8.494	2217	2225	2234	rVB4	1062	1599	0.01%	0.004%
53	8.555	2234	2244	2253	rVB3	3752	5536	0.03%	0.014%
54	8.642	2257	2271	2311	rBV	517462	916363	4.14%	2.344%
55	8.870	2341	2342	2348	rVB3	346	186	0.00%	0.000%
56	9.018	2383	2388	2391	rBV2	212	230	0.00%	0.001%
57	9.340	2486	2488	2494	rVB2	249	232	0.00%	0.001%
58	9.420	2499	2513	2529	rBV	526247	866795	3.92%	2.217%
59	9.539	2541	2550	2553	rBV3	7631	10815	0.05%	0.028%
60	9.575	2553	2561	2573	rVB	31812	49991	0.23%	0.128%
61	9.642	2578	2582	2585	rVB	303	259	0.00%	0.001%
62	9.693	2585	2598	2614	rBV	133558	218087	0.99%	0.558%
63	9.764	2615	2620	2629	rVB3	1267	1895	0.01%	0.005%
64	9.812	2632	2635	2639	rBV2	242	210	0.00%	0.001%
65	10.105	2714	2726	2744	rBV	84742	137340	0.62%	0.351%
66	10.247	2768	2770	2773	rVV	278	179	0.00%	0.000%
67	10.269	2775	2777	2780	rVV	278	166	0.00%	0.000%
68	10.404	2814	2819	2823	rVB2	217	263	0.00%	0.001%
69	10.430	2823	2827	2834	rBV2	231	384	0.00%	0.001%
70	10.488	2838	2845	2848	rBV3	931	1009	0.00%	0.003%
71	10.674	2895	2903	2912	rVB3	1664	2512	0.01%	0.006%
72	10.761	2917	2930	2949	rBV	460278	745977	3.37%	1.908%
73	10.861	2960	2961	2966	rBV	478	406	0.00%	0.001%
74	10.996	2998	3003	3009	rBV2	951	1250	0.01%	0.003%
75	11.066	3020	3025	3026	rBV	235	213	0.00%	0.001%
76	11.095	3028	3034	3038	rVV2	670	866	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045112.D
 Acq On : 04 Oct 2021 22:11
 Operator : SY/MD
 Sample : M4023-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.192	3059	3064	3066	rBV2	210	210	0.00%	0.001%
78	11.356	3112	3115	3118	rBV	231	180	0.00%	0.000%
79	11.394	3123	3127	3132	rVV	226	278	0.00%	0.001%
80	11.423	3133	3136	3138	rVV2	385	277	0.00%	0.001%
81	11.472	3140	3151	3160	rVV4	3955	5823	0.03%	0.015%
82	11.529	3162	3169	3178	rVV2	1527	2047	0.01%	0.005%
83	11.697	3216	3221	3222	rBV3	752	595	0.00%	0.002%
84	11.748	3232	3237	3245	rBV	793	872	0.00%	0.002%
85	11.816	3245	3258	3277	rBV	552538	868727	3.93%	2.222%
86	11.976	3303	3308	3314	rVB3	1033	1157	0.01%	0.003%
87	12.121	3350	3353	3356	rBV3	320	271	0.00%	0.001%
88	12.195	3362	3376	3393	rVV	562954	903667	4.08%	2.312%
89	12.520	3473	3477	3481	rVB	267	255	0.00%	0.001%
90	12.571	3488	3493	3499	rBV3	429	581	0.00%	0.001%
91	12.726	3537	3541	3544	rBV	203	174	0.00%	0.000%
92	12.957	3609	3613	3618	rVB3	540	515	0.00%	0.001%
93	13.455	3760	3768	3779	rBV5	829	1447	0.01%	0.004%
94	14.095	3957	3967	3978	rBV	4556	6924	0.03%	0.018%
95	14.272	4020	4022	4027	rBV3	243	200	0.00%	0.001%
96	14.333	4037	4041	4045	rBV3	569	580	0.00%	0.001%
97	15.227	4312	4319	4328	rBV4	3208	5288	0.02%	0.014%
98	15.410	4370	4376	4388	rVB5	1682	2644	0.01%	0.007%
99	15.870	4517	4519	4523	rBV3	535	509	0.00%	0.001%
100	15.976	4548	4552	4555	rBV4	622	689	0.00%	0.002%




Sum of corrected areas: 39092507

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045112.D
Acq On : 04 Oct 2021 22:11
Operator : SY/MD
Sample : M4023-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

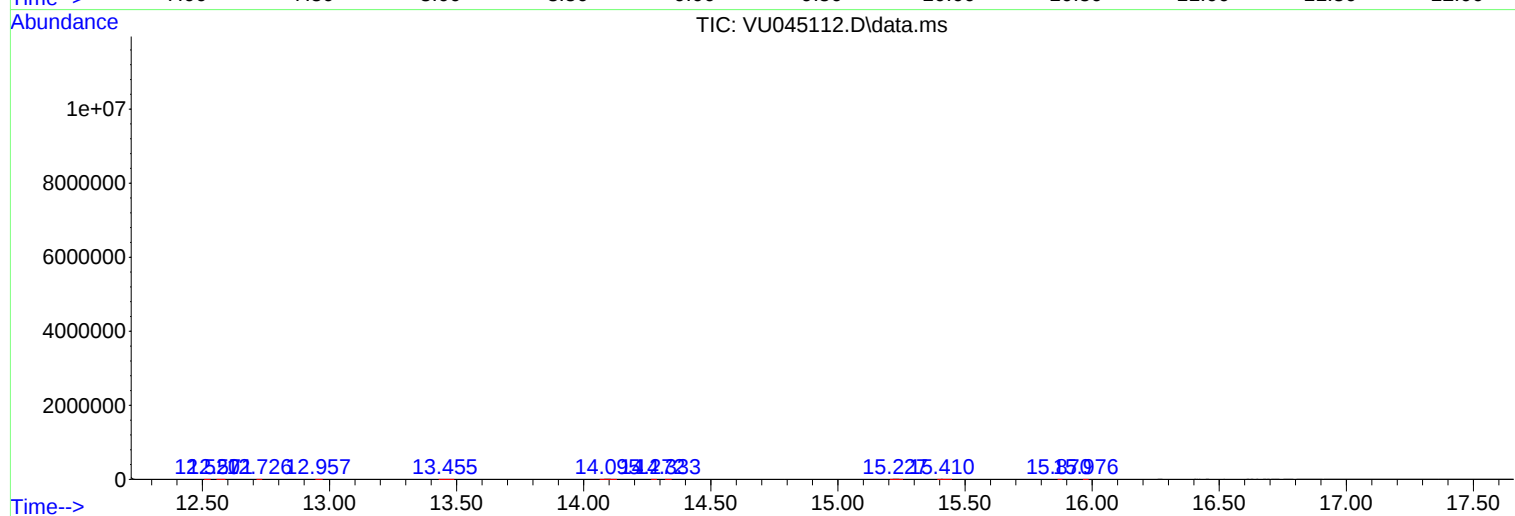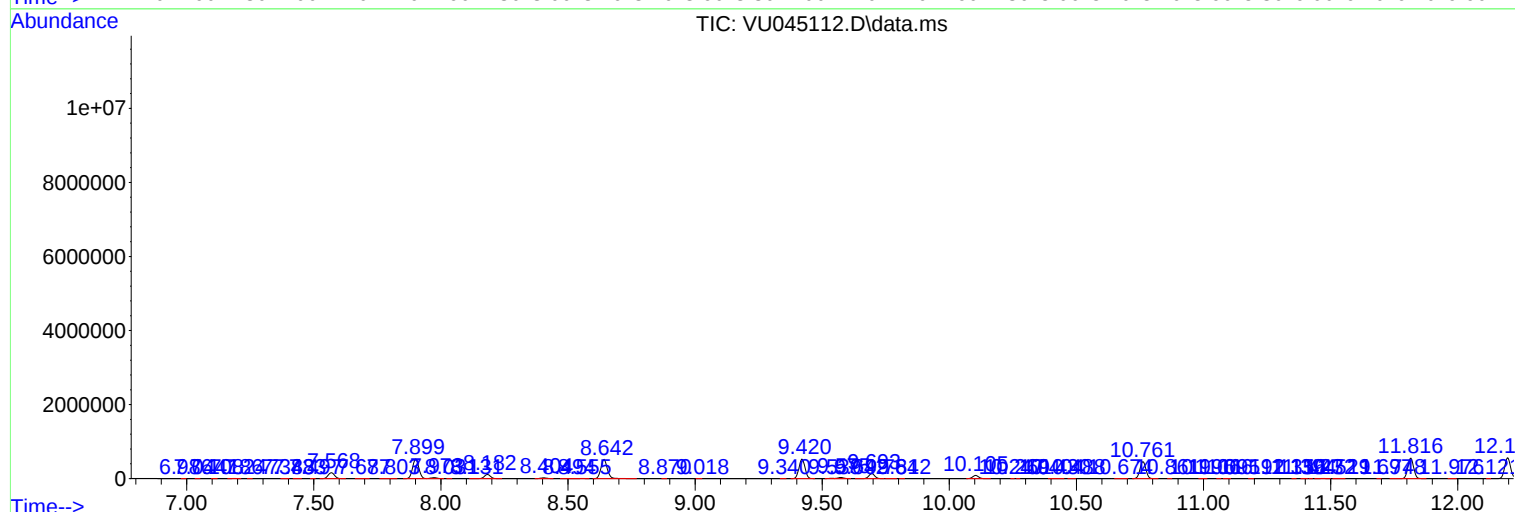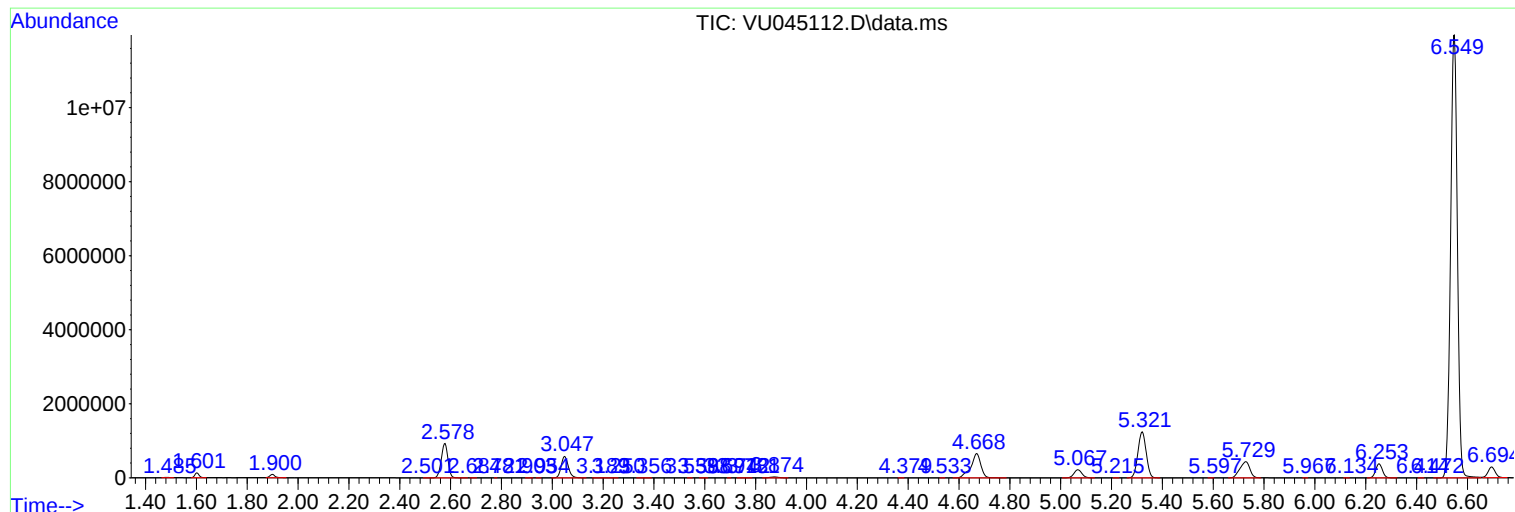

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045112.D
Acq On : 04 Oct 2021 22:11
Operator : SY/MD
Sample : M4023-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045112.D
Acq On : 04 Oct 2021 22:11
Operator : SY/MD
Sample : M4023-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
