

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045113.D
 Acq On : 04 Oct 2021 22:34
 Operator : SY/MD
 Sample : M4023-04 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	95	rBV	122783	150674	1.16%	0.584%
2	1.899	166	174	187	rVB	110221	155944	1.20%	0.604%
3	2.575	369	384	402	rBV4	533575	1027768	7.90%	3.982%
4	2.687	411	419	423	rVB3	457	523	0.00%	0.002%
5	2.748	435	438	441	rVB2	229	183	0.00%	0.001%
6	2.768	441	444	447	rBV2	220	221	0.00%	0.001%
7	2.790	447	451	457	rBV	475	624	0.00%	0.002%
8	2.864	470	474	479	rBV2	193	229	0.00%	0.001%
9	2.954	496	502	503	rBV2	423	339	0.00%	0.001%
10	3.047	516	531	560	rBV	319425	627427	4.82%	2.431%
11	3.150	560	563	566	rBV2	195	163	0.00%	0.001%
12	3.189	566	575	587	rBV	1446	3288	0.03%	0.013%
13	3.301	608	610	614	rVV	164	165	0.00%	0.001%
14	3.356	618	627	635	rVB4	1102	1784	0.01%	0.007%
15	3.430	646	650	657	rVB2	197	199	0.00%	0.001%
16	3.520	672	678	681	rBV	222	187	0.00%	0.001%
17	3.552	683	688	692	rBV2	152	212	0.00%	0.001%
18	3.874	774	788	804	rBV2	12894	29139	0.22%	0.113%
19	4.022	831	834	840	rVB2	245	207	0.00%	0.001%
20	4.057	840	845	847	rBV	251	241	0.00%	0.001%
21	4.343	930	934	938	rBV2	186	177	0.00%	0.001%
22	4.417	954	957	961	rVB	170	156	0.00%	0.001%
23	4.443	961	965	974	rBV2	233	405	0.00%	0.002%
24	4.478	974	976	981	rBV2	146	167	0.00%	0.001%
25	4.632	1005	1024	1026	rBV	165495	276357	2.12%	1.071%
26	4.854	1092	1093	1097	rVB2	296	178	0.00%	0.001%
27	5.067	1143	1159	1182	rBV	217559	479890	3.69%	1.859%
28	5.321	1218	1238	1257	rBV	668898	1497832	11.51%	5.803%
29	5.549	1304	1309	1315	rVV2	246	253	0.00%	0.001%
30	5.729	1343	1365	1402	rVV2	438404	1206239	9.27%	4.674%
31	6.034	1458	1460	1466	rBV2	281	165	0.00%	0.001%
32	6.128	1486	1489	1490	rVV3	367	199	0.00%	0.001%
33	6.140	1490	1493	1496	rVB2	611	434	0.00%	0.002%
34	6.253	1512	1528	1549	rBV	384579	719532	5.53%	2.788%
35	6.481	1595	1599	1601	rBV2	242	174	0.00%	0.001%
36	6.546	1601	1619	1652	rBV	6989305	13010264	100.00%	50.408%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045113.D
 Acq On : 04 Oct 2021 22:34
 Operator : SY/MD
 Sample : M4023-04 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.697	1654	1666	1684	rVB	288983	567524	4.36%	2.199%
38	6.931	1736	1739	1742	rBV	175	140	0.00%	0.001%
39	6.948	1742	1744	1749	rVB	187	136	0.00%	0.001%
40	7.047	1770	1775	1787	rVB3	552	1027	0.01%	0.004%
41	7.185	1810	1818	1827	rVV4	3412	5498	0.04%	0.021%
42	7.240	1830	1835	1841	rVB2	239	318	0.00%	0.001%
43	7.272	1841	1845	1850	rBV2	232	311	0.00%	0.001%
44	7.507	1914	1918	1921	rBV2	335	324	0.00%	0.001%
45	7.568	1925	1937	1956	rBV	161089	280105	2.15%	1.085%
46	7.690	1966	1975	1991	rBV5	1858	3306	0.03%	0.013%
47	7.774	1997	2001	2003	rBV2	176	163	0.00%	0.001%
48	7.793	2003	2007	2016	rVB4	684	1061	0.01%	0.004%
49	7.902	2026	2041	2055	rBV	522753	899186	6.91%	3.484%
50	7.973	2055	2063	2075	rVB	20550	33994	0.26%	0.132%
51	8.131	2108	2112	2117	rBV	417	377	0.00%	0.001%
52	8.182	2117	2128	2150	rBV	113443	187972	1.44%	0.728%
53	8.266	2150	2154	2162	rVB4	258	356	0.00%	0.001%
54	8.362	2181	2184	2188	rBV2	170	171	0.00%	0.001%
55	8.404	2188	2197	2207	rVB2	10278	16010	0.12%	0.062%
56	8.555	2238	2244	2252	rVB3	2790	3826	0.03%	0.015%
57	8.639	2257	2270	2299	rBV	513923	911253	7.00%	3.531%
58	9.311	2476	2479	2482	rBV2	155	152	0.00%	0.001%
59	9.420	2497	2513	2538	rBV	541208	878499	6.75%	3.404%
60	9.539	2543	2550	2553	rVV2	4292	5998	0.05%	0.023%
61	9.571	2553	2560	2572	rVB	23759	37180	0.29%	0.144%
62	9.693	2587	2598	2615	rBV	99146	159768	1.23%	0.619%
63	9.864	2646	2651	2654	rBV	228	199	0.00%	0.001%
64	9.890	2655	2659	2663	rVB	198	204	0.00%	0.001%
65	10.102	2714	2725	2739	rVV	54953	87482	0.67%	0.339%
66	10.484	2837	2844	2850	rBV3	831	960	0.01%	0.004%
67	10.674	2896	2903	2909	rBV3	1785	2341	0.02%	0.009%
68	10.761	2917	2930	2949	rBV	463573	747100	5.74%	2.895%
69	10.873	2962	2965	2967	rBV3	263	180	0.00%	0.001%
70	10.906	2972	2975	2980	rVB2	581	430	0.00%	0.002%
71	10.999	2998	3004	3006	rBV2	698	656	0.01%	0.003%
72	11.095	3027	3034	3037	rBV3	583	638	0.00%	0.002%
73	11.195	3061	3065	3069	rBV2	253	281	0.00%	0.001%
74	11.298	3091	3097	3100	rBV2	408	531	0.00%	0.002%
75	11.340	3107	3110	3113	rBV	211	195	0.00%	0.001%
76	11.468	3142	3150	3159	rVB4	3075	4457	0.03%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045113.D
 Acq On : 04 Oct 2021 22:34
 Operator : SY/MD
 Sample : M4023-04 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.529	3164	3169	3175	rVB4	588	703	0.01%	0.003%
78	11.700	3212	3222	3227	rBV3	960	1264	0.01%	0.005%
79	11.815	3245	3258	3274	rBV	552793	869062	6.68%	3.367%
80	11.941	3294	3297	3302	rBV3	383	269	0.00%	0.001%
81	12.005	3314	3317	3319	rBV2	212	150	0.00%	0.001%
82	12.095	3342	3345	3349	rVB	277	215	0.00%	0.001%
83	12.195	3363	3376	3395	rBV	549692	892869	6.86%	3.459%
84	12.494	3461	3469	3470	rBV2	349	345	0.00%	0.001%
85	12.529	3475	3480	3483	rBV2	227	211	0.00%	0.001%
86	12.571	3490	3493	3499	rVB2	507	598	0.00%	0.002%
87	12.606	3499	3504	3507	rBV	327	355	0.00%	0.001%
88	12.687	3526	3529	3532	rBV	321	187	0.00%	0.001%
89	12.883	3588	3590	3593	rBV2	255	158	0.00%	0.001%
90	13.034	3634	3637	3639	rVB	282	167	0.00%	0.001%
91	13.455	3761	3768	3774	rVB2	651	912	0.01%	0.004%
92	13.613	3813	3817	3822	rBV	201	199	0.00%	0.001%
93	13.729	3849	3853	3857	rBV2	318	310	0.00%	0.001%
94	13.844	3886	3889	3893	rVB4	353	293	0.00%	0.001%
95	14.095	3961	3967	3977	rVB2	2870	3831	0.03%	0.015%
96	14.330	4038	4040	4045	rVB	403	319	0.00%	0.001%
97	14.356	4045	4048	4053	rVB2	254	161	0.00%	0.001%
98	15.230	4312	4320	4332	rVB3	2040	3829	0.03%	0.015%
99	15.413	4372	4377	4380	rBV6	799	896	0.01%	0.003%
100	15.854	4511	4514	4517	rBV3	456	385	0.00%	0.001%




Sum of corrected areas: 25809936

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045113.D
Acq On : 04 Oct 2021 22:34
Operator : SY/MD
Sample : M4023-04 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

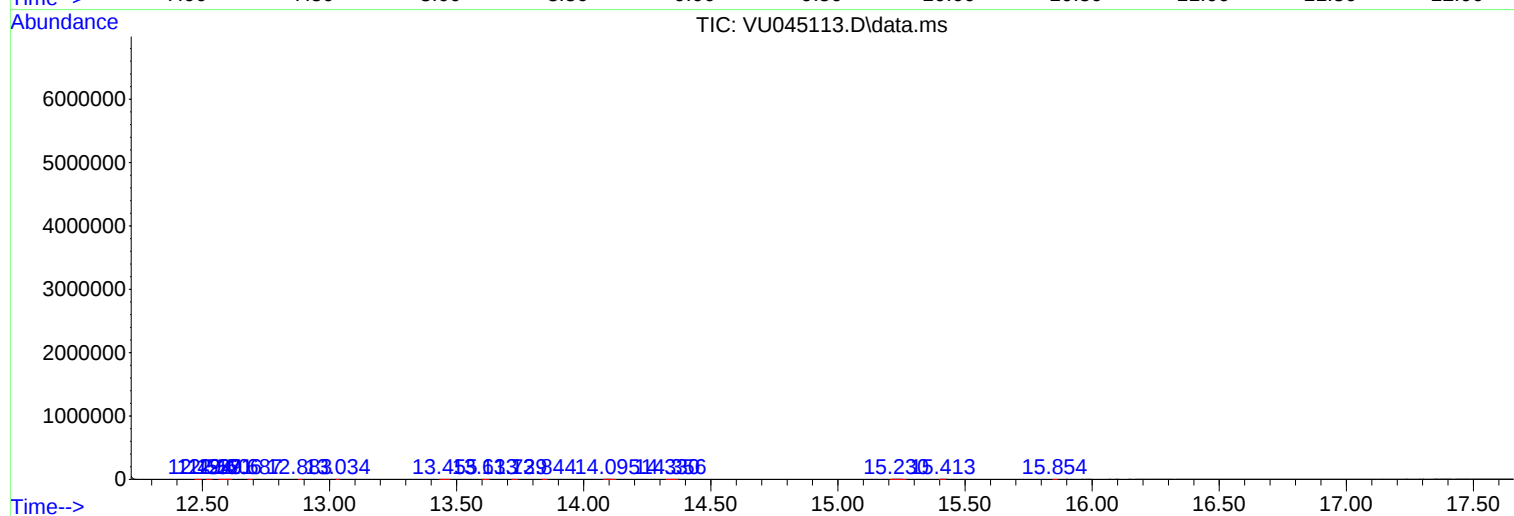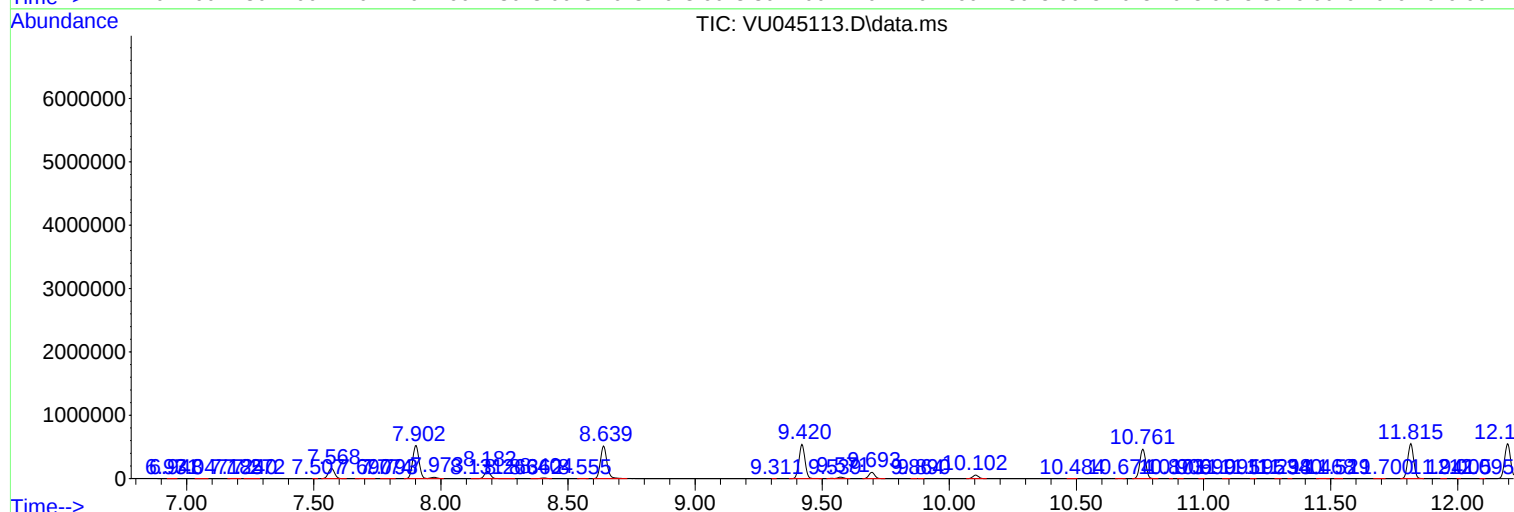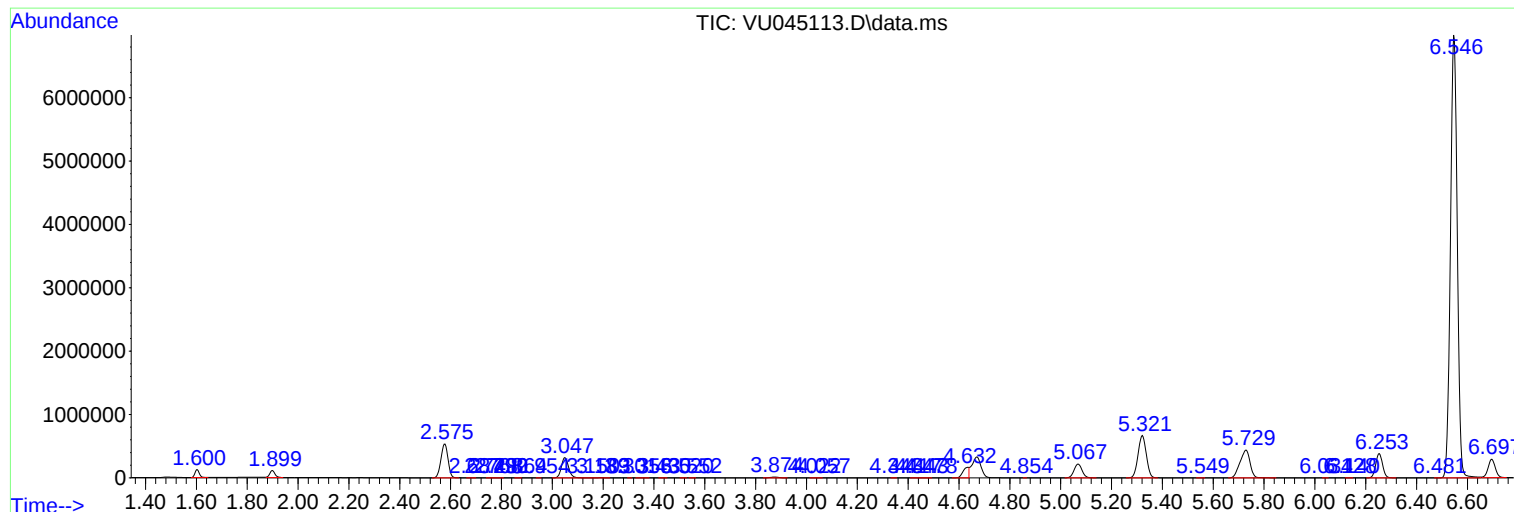

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045113.D
Acq On : 04 Oct 2021 22:34
Operator : SY/MD
Sample : M4023-04 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045113.D
Acq On : 04 Oct 2021 22:34
Operator : SY/MD
Sample : M4023-04 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
