

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045116.D
 Acq On : 04 Oct 2021 23:44
 Operator : SY/MD
 Sample : M4023-13 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	93	rBV	114979	135219	11.68%	1.349%
2	1.896	165	173	186	rVB	105218	149392	12.91%	1.491%
3	2.462	346	349	352	rVB	470	271	0.02%	0.003%
4	2.565	368	381	400	rBV2	221116	381350	32.95%	3.805%
5	2.739	431	435	438	rBV2	152	169	0.01%	0.002%
6	2.784	445	449	452	rBV2	402	385	0.03%	0.004%
7	2.826	459	462	467	rVB2	217	221	0.02%	0.002%
8	2.929	490	494	495	rBV	201	152	0.01%	0.002%
9	2.941	495	498	499	rBV	302	172	0.01%	0.002%
10	3.048	520	531	553	rVB3	10734	20630	1.78%	0.206%
11	3.134	553	558	562	rBV2	248	314	0.03%	0.003%
12	3.189	562	575	589	rVV2	1341	3143	0.27%	0.031%
13	3.356	616	627	643	rVB2	11825	22605	1.95%	0.226%
14	3.475	659	664	667	rBV2	236	230	0.02%	0.002%
15	3.539	682	684	690	rBV2	153	158	0.01%	0.002%
16	3.607	702	705	711	rBV2	183	252	0.02%	0.003%
17	3.665	716	723	725	rBV2	199	236	0.02%	0.002%
18	3.877	774	789	801	rVV2	3649	7713	0.67%	0.077%
19	4.006	823	829	834	rBV2	122	220	0.02%	0.002%
20	4.176	878	882	885	rBV2	227	226	0.02%	0.002%
21	4.449	964	967	971	rBV2	186	165	0.01%	0.002%
22	4.520	986	989	994	rVB2	217	216	0.02%	0.002%
23	4.629	1008	1023	1028	rBV	149070	311281	26.90%	3.106%
24	4.887	1100	1103	1106	rBV	196	180	0.02%	0.002%
25	4.970	1122	1129	1131	rBV3	306	368	0.03%	0.004%
26	5.067	1142	1159	1187	rBV	212006	464347	40.12%	4.633%
27	5.182	1191	1195	1199	rVB3	250	281	0.02%	0.003%
28	5.221	1203	1207	1209	rBV2	444	279	0.02%	0.003%
29	5.321	1221	1238	1255	rBV	54737	122559	10.59%	1.223%
30	5.539	1301	1306	1309	rBV2	181	158	0.01%	0.002%
31	5.581	1316	1319	1322	rBV2	197	170	0.01%	0.002%
32	5.729	1343	1365	1394	rBV2	424070	1157357	100.00%	11.547%
33	5.871	1406	1409	1416	rBV2	196	219	0.02%	0.002%
34	6.067	1467	1470	1473	rVB2	321	218	0.02%	0.002%
35	6.092	1473	1478	1481	rBV	235	257	0.02%	0.003%
36	6.141	1491	1493	1497	rBV2	236	167	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045116.D
 Acq On : 04 Oct 2021 23:44
 Operator : SY/MD
 Sample : M4023-13 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.253	1511	1528	1547	rBV	370632	702227	60.68%	7.006%
38	6.417	1575	1579	1583	rVB2	248	196	0.02%	0.002%
39	6.453	1585	1590	1596	rBV3	198	270	0.02%	0.003%
40	6.475	1596	1597	1604	rVB3	207	168	0.01%	0.002%
41	6.546	1604	1619	1647	rBV	241356	452435	39.09%	4.514%
42	6.694	1650	1665	1688	rBV	280378	545639	47.15%	5.444%
43	6.813	1696	1702	1708	rBV4	629	762	0.07%	0.008%
44	6.903	1728	1730	1735	rBV	157	140	0.01%	0.001%
45	7.047	1767	1775	1776	rBV2	497	558	0.05%	0.006%
46	7.182	1809	1817	1827	rVB3	2967	5050	0.44%	0.050%
47	7.234	1827	1833	1836	rVB2	196	227	0.02%	0.002%
48	7.260	1838	1841	1844	rVB2	225	161	0.01%	0.002%
49	7.478	1902	1909	1912	rBV2	167	196	0.02%	0.002%
50	7.568	1920	1937	1954	rBV	152260	263057	22.73%	2.625%
51	7.687	1967	1974	1989	rVB4	1661	2833	0.24%	0.028%
52	7.761	1995	1997	2000	rBV2	179	147	0.01%	0.001%
53	7.899	2027	2040	2056	rBV	501546	861632	74.45%	8.597%
54	7.973	2056	2063	2079	rVB	7886	13239	1.14%	0.132%
55	8.131	2110	2112	2115	rVB2	395	179	0.02%	0.002%
56	8.182	2115	2128	2147	rBV	104894	175162	15.13%	1.748%
57	8.404	2191	2197	2203	rVB3	1041	1217	0.11%	0.012%
58	8.481	2217	2221	2224	rBV2	174	188	0.02%	0.002%
59	8.533	2233	2237	2239	rBV2	188	161	0.01%	0.002%
60	8.555	2239	2244	2249	rVB4	1194	1241	0.11%	0.012%
61	8.639	2256	2270	2299	rBV	498089	875685	75.66%	8.737%
62	9.176	2434	2437	2440	rBV2	211	180	0.02%	0.002%
63	9.253	2458	2461	2468	rVB2	175	228	0.02%	0.002%
64	9.420	2499	2513	2535	rBV	525412	855030	73.88%	8.531%
65	9.571	2553	2560	2569	rVV	879	1356	0.12%	0.014%
66	9.626	2572	2577	2582	rBV2	134	191	0.02%	0.002%
67	9.694	2590	2598	2608	rVB2	1868	2551	0.22%	0.025%
68	10.105	2718	2726	2735	rVB4	946	1648	0.14%	0.016%
69	10.202	2750	2756	2760	rBV	245	330	0.03%	0.003%
70	10.533	2855	2859	2861	rBV2	189	152	0.01%	0.002%
71	10.542	2861	2862	2867	rVB	212	178	0.02%	0.002%
72	10.568	2867	2870	2872	rBV2	237	187	0.02%	0.002%
73	10.674	2894	2903	2912	rBV3	1478	2310	0.20%	0.023%
74	10.761	2917	2930	2952	rVB	462066	737730	63.74%	7.361%
75	10.867	2959	2963	2966	rVB2	442	342	0.03%	0.003%
76	11.002	2997	3005	3007	rBV3	404	507	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045116.D
 Acq On : 04 Oct 2021 23:44
 Operator : SY/MD
 Sample : M4023-13 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.089	3028	3032	3037	rBV4	586	668	0.06%	0.007%
78	11.182	3055	3061	3062	rBV2	303	252	0.02%	0.003%
79	11.221	3067	3073	3079	rVV	321	463	0.04%	0.005%
80	11.266	3083	3087	3091	rVB2	221	183	0.02%	0.002%
81	11.292	3091	3095	3100	rBV2	335	386	0.03%	0.004%
82	11.468	3139	3150	3157	rBV6	1545	2895	0.25%	0.029%
83	11.574	3179	3183	3188	rBV3	319	333	0.03%	0.003%
84	11.700	3212	3222	3227	rBV4	905	1184	0.10%	0.012%
85	11.816	3244	3258	3277	rVV	546258	853857	73.78%	8.519%
86	11.944	3295	3298	3302	rBV3	479	352	0.03%	0.004%
87	11.976	3302	3308	3317	rVB4	1243	1629	0.14%	0.016%
88	12.124	3352	3354	3361	rVB3	206	187	0.02%	0.002%
89	12.195	3361	3376	3395	rBV	538946	869452	75.12%	8.675%
90	12.263	3395	3397	3405	rVV2	602	671	0.06%	0.007%
91	12.398	3435	3439	3443	rBV2	217	252	0.02%	0.003%
92	12.764	3550	3553	3556	rBV2	283	261	0.02%	0.003%
93	13.102	3656	3658	3662	rVB2	245	166	0.01%	0.002%
94	13.819	3878	3881	3883	rBV2	216	160	0.01%	0.002%
95	13.912	3906	3910	3913	rBV2	297	294	0.03%	0.003%
96	13.960	3922	3925	3931	rBV3	356	314	0.03%	0.003%
97	14.092	3958	3966	3967	rBV	1124	1234	0.11%	0.012%
98	14.365	4049	4051	4054	rVB	277	146	0.01%	0.001%
99	14.385	4054	4057	4061	rVB3	272	190	0.02%	0.002%
100	14.661	4140	4143	4146	rBV2	292	192	0.02%	0.002%


Sum of corrected areas: 10022691

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045116.D
Acq On : 04 Oct 2021 23:44
Operator : SY/MD
Sample : M4023-13 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

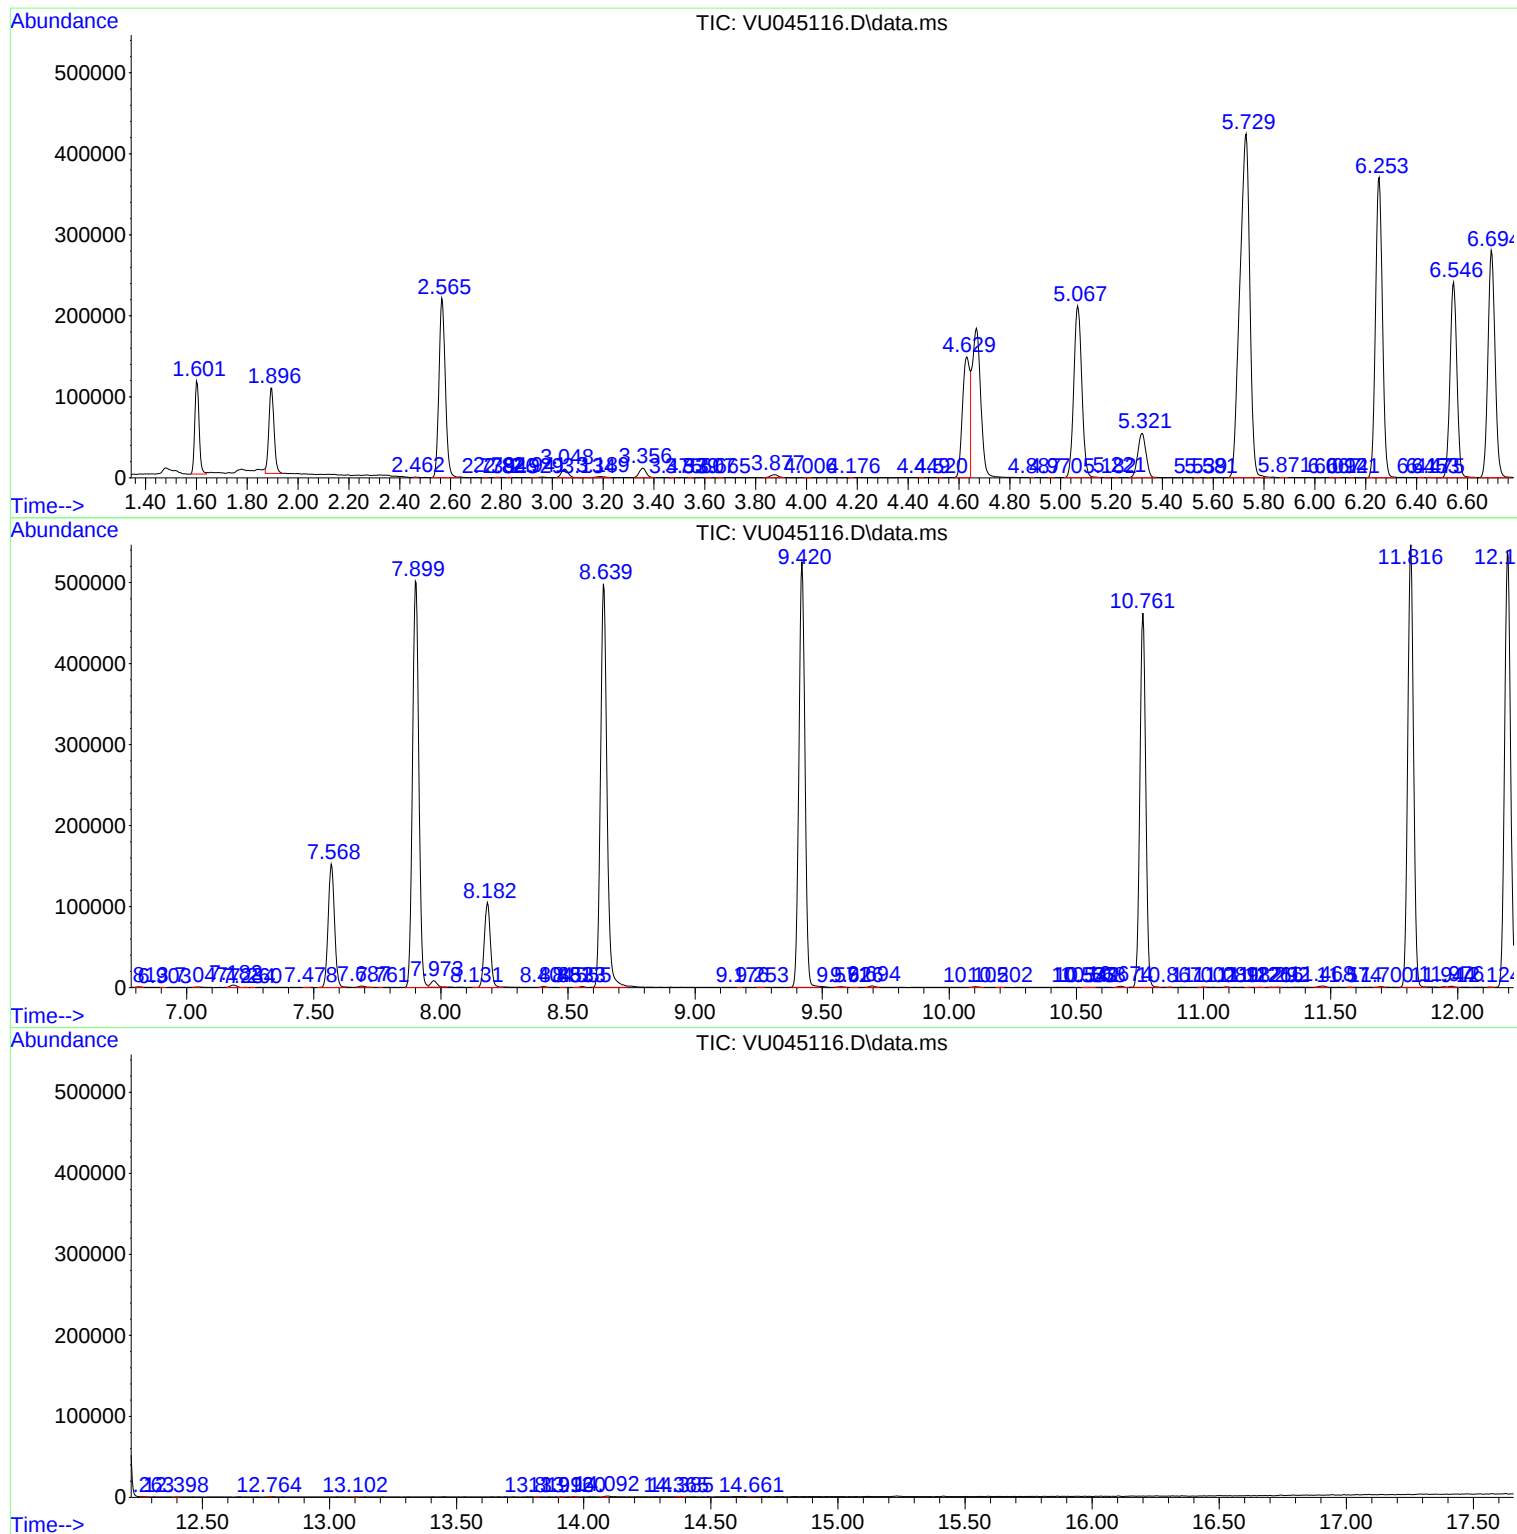

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045116.D
Acq On : 04 Oct 2021 23:44
Operator : SY/MD
Sample : M4023-13 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045116.D
Acq On : 04 Oct 2021 23:44
Operator : SY/MD
Sample : M4023-13 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
