

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045117.D
 Acq On : 05 Oct 2021 00:08
 Operator : SY/MD
 Sample : M4023-14 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	93	rBV	109475	129578	11.50%	1.404%
2	1.896	165	173	187	rVB	105469	147948	13.13%	1.604%
3	2.565	368	381	400	rVV	207267	348692	30.94%	3.779%
4	2.671	412	414	418	rBV	286	211	0.02%	0.002%
5	2.719	428	429	436	rVB	221	227	0.02%	0.002%
6	2.793	448	452	461	rVB2	537	803	0.07%	0.009%
7	2.835	461	465	471	rBV2	365	389	0.03%	0.004%
8	2.864	471	474	479	rVB2	214	179	0.02%	0.002%
9	2.964	496	505	508	rBV2	643	1066	0.09%	0.012%
10	3.047	520	531	541	rBV4	2215	3708	0.33%	0.040%
11	3.189	564	575	585	rBV3	1683	3587	0.32%	0.039%
12	3.282	601	604	607	rBV	287	244	0.02%	0.003%
13	3.324	612	617	623	rVB	185	277	0.02%	0.003%
14	3.350	623	625	631	rBV2	190	190	0.02%	0.002%
15	3.706	733	736	739	rBV2	210	194	0.02%	0.002%
16	3.922	799	803	805	rBV2	177	167	0.01%	0.002%
17	3.938	805	808	815	rVB2	233	289	0.03%	0.003%
18	4.012	826	831	835	rBV2	186	212	0.02%	0.002%
19	4.063	842	847	850	rVB2	185	191	0.02%	0.002%
20	4.099	851	858	860	rBV	276	275	0.02%	0.003%
21	4.173	878	881	885	rBV2	220	169	0.01%	0.002%
22	4.205	885	891	896	rVB2	189	277	0.02%	0.003%
23	4.327	925	929	933	rVB2	311	342	0.03%	0.004%
24	4.369	939	942	945	rBV2	183	192	0.02%	0.002%
25	4.552	994	999	1002	rBV2	196	237	0.02%	0.003%
26	4.629	1008	1023	1060	rBV	145359	381910	33.88%	4.139%
27	4.806	1075	1078	1086	rBV3	254	347	0.03%	0.004%
28	4.931	1110	1117	1122	rVB2	214	346	0.03%	0.004%
29	4.960	1123	1126	1131	rBV2	253	236	0.02%	0.003%
30	5.067	1143	1159	1186	rBV	204925	447479	39.70%	4.850%
31	5.163	1186	1189	1192	rVB3	244	176	0.02%	0.002%
32	5.295	1223	1230	1232	rBV3	492	600	0.05%	0.007%
33	5.378	1251	1256	1261	rVB2	374	491	0.04%	0.005%
34	5.494	1289	1292	1298	rVB2	237	228	0.02%	0.002%
35	5.530	1298	1303	1305	rBV	181	194	0.02%	0.002%
36	5.729	1342	1365	1389	rBV2	413724	1127156	100.00%	12.216%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045117.D
 Acq On : 05 Oct 2021 00:08
 Operator : SY/MD
 Sample : M4023-14 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.835	1395	1398	1401	rVB2	420	250	0.02%	0.003%
38	6.041	1458	1462	1464	rBV	274	219	0.02%	0.002%
39	6.108	1478	1483	1484	rVV2	304	208	0.02%	0.002%
40	6.253	1513	1528	1546	rBV	360994	674991	59.88%	7.316%
41	6.542	1607	1618	1635	rVB6	12018	23748	2.11%	0.257%
42	6.639	1643	1648	1650	rBV	157	185	0.02%	0.002%
43	6.693	1650	1665	1687	rVV	274341	529227	46.95%	5.736%
44	6.803	1696	1699	1700	rBV	439	257	0.02%	0.003%
45	6.857	1712	1716	1720	rBV2	172	184	0.02%	0.002%
46	7.044	1769	1774	1775	rBV3	465	387	0.03%	0.004%
47	7.182	1809	1817	1830	rBV5	2885	5007	0.44%	0.054%
48	7.250	1836	1838	1846	rVB2	219	295	0.03%	0.003%
49	7.568	1924	1937	1955	rBV	146797	252467	22.40%	2.736%
50	7.642	1958	1960	1965	rVV2	361	304	0.03%	0.003%
51	7.687	1967	1974	1987	rVB2	1711	2908	0.26%	0.032%
52	7.902	2026	2041	2055	rVV	490773	841252	74.63%	9.118%
53	7.973	2057	2063	2073	rVB2	8044	12175	1.08%	0.132%
54	8.182	2116	2128	2145	rVV	103236	171254	15.19%	1.856%
55	8.356	2177	2182	2184	rBV2	310	298	0.03%	0.003%
56	8.465	2211	2216	2218	rBV	272	199	0.02%	0.002%
57	8.481	2218	2221	2225	rVB3	295	215	0.02%	0.002%
58	8.520	2226	2233	2235	rBV	234	314	0.03%	0.003%
59	8.552	2239	2243	2254	rVB4	856	1140	0.10%	0.012%
60	8.639	2256	2270	2297	rBV	484846	870010	77.19%	9.429%
61	8.809	2318	2323	2329	rBV3	185	262	0.02%	0.003%
62	8.922	2352	2358	2365	rBV2	278	491	0.04%	0.005%
63	9.041	2391	2395	2403	rBV2	194	342	0.03%	0.004%
64	9.250	2454	2460	2463	rBV2	201	270	0.02%	0.003%
65	9.420	2499	2513	2545	rBV	507967	824664	73.16%	8.938%
66	9.571	2554	2560	2569	rVB3	619	908	0.08%	0.010%
67	9.697	2592	2599	2608	rBV2	1599	2348	0.21%	0.025%
68	10.102	2720	2725	2730	rVB3	414	478	0.04%	0.005%
69	10.150	2735	2740	2744	rBV2	192	258	0.02%	0.003%
70	10.359	2801	2805	2809	rBV2	218	251	0.02%	0.003%
71	10.433	2824	2828	2836	rVB2	174	232	0.02%	0.003%
72	10.526	2854	2857	2860	rBV2	188	170	0.02%	0.002%
73	10.761	2916	2930	2952	rBV	449308	720674	63.94%	7.811%
74	10.870	2961	2964	2968	rBV	358	376	0.03%	0.004%
75	10.951	2986	2989	2994	rBV2	194	198	0.02%	0.002%
76	10.996	2999	3003	3011	rVV3	280	460	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045117.D
 Acq On : 05 Oct 2021 00:08
 Operator : SY/MD
 Sample : M4023-14 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.070	3023	3026	3030	rBV2	231	250	0.02%	0.003%
78	11.298	3093	3097	3101	rVB2	283	246	0.02%	0.003%
79	11.471	3141	3151	3159	rBV6	1543	2806	0.25%	0.030%
80	11.651	3204	3207	3211	rVB	205	184	0.02%	0.002%
81	11.693	3217	3220	3222	rBV4	469	299	0.03%	0.003%
82	11.764	3239	3242	3245	rBV	254	232	0.02%	0.003%
83	11.815	3245	3258	3277	rVV	541512	827142	73.38%	8.965%
84	11.976	3303	3308	3313	rVB3	920	1046	0.09%	0.011%
85	12.105	3343	3348	3351	rBV2	230	263	0.02%	0.003%
86	12.195	3361	3376	3398	rBV	531178	850127	75.42%	9.214%
87	12.741	3542	3546	3552	rBV2	223	338	0.03%	0.004%
88	12.770	3552	3555	3560	rVV2	286	320	0.03%	0.003%
89	12.909	3593	3598	3600	rBV2	264	282	0.03%	0.003%
90	13.587	3807	3809	3812	rBV	203	170	0.02%	0.002%
91	13.642	3823	3826	3829	rBV	274	215	0.02%	0.002%
92	13.803	3870	3876	3880	rBV2	188	221	0.02%	0.002%
93	13.992	3932	3935	3937	rBV	299	234	0.02%	0.003%
94	14.095	3961	3967	3976	rBV2	886	1553	0.14%	0.017%
95	14.204	3997	4001	4002	rBV	250	173	0.02%	0.002%
96	14.404	4060	4063	4070	rBV2	259	405	0.04%	0.004%
97	14.475	4083	4085	4090	rVB2	360	297	0.03%	0.003%
98	14.568	4112	4114	4116	rBV	341	210	0.02%	0.002%
99	14.780	4178	4180	4189	rVB3	298	379	0.03%	0.004%
100	15.227	4315	4319	4320	rBV2	656	436	0.04%	0.005%


Sum of corrected areas: 9226511

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045117.D
Acq On : 05 Oct 2021 00:08
Operator : SY/MD
Sample : M4023-14 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

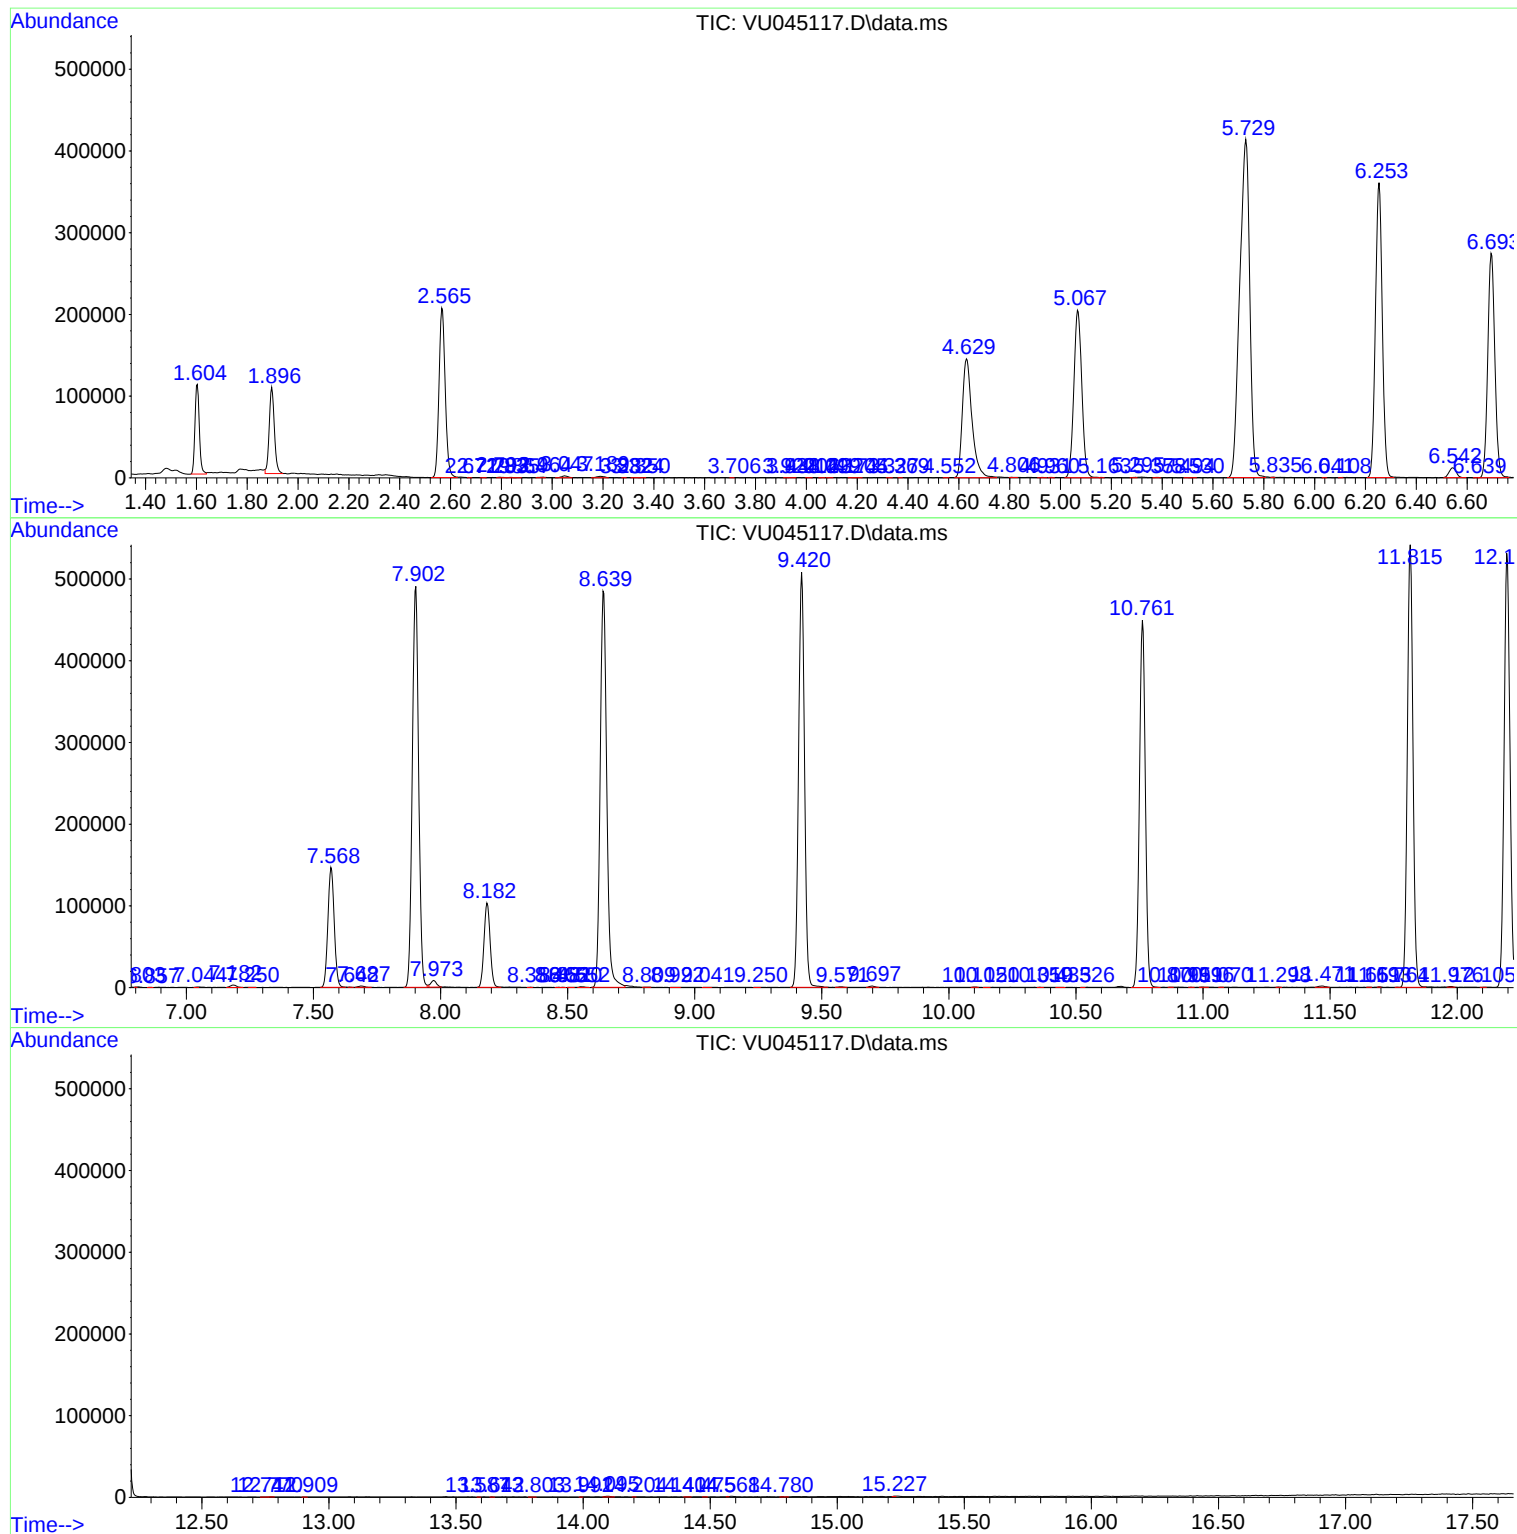

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045117.D
Acq On : 05 Oct 2021 00:08
Operator : SY/MD
Sample : M4023-14 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045117.D
Acq On : 05 Oct 2021 00:08
Operator : SY/MD
Sample : M4023-14 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------