

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045118.D
 Acq On : 05 Oct 2021 00:31
 Operator : SY/MD
 Sample : M4023-15 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	93	rBV	113528	130266	11.19%	1.391%
2	1.903	167	175	187	rVB	87210	114553	9.84%	1.223%
3	2.565	369	381	406	rBV	211819	361237	31.02%	3.856%
4	2.794	445	452	454	rBV	452	536	0.05%	0.006%
5	2.829	459	463	465	rBV	188	137	0.01%	0.001%
6	2.861	470	473	479	rVB3	249	224	0.02%	0.002%
7	2.958	494	503	506	rBV3	625	864	0.07%	0.009%
8	2.993	511	514	520	rVV2	225	199	0.02%	0.002%
9	3.048	522	531	541	rVB2	2694	4627	0.40%	0.049%
10	3.186	561	574	593	rBV5	1896	5177	0.44%	0.055%
11	3.318	613	615	621	rVB2	148	140	0.01%	0.001%
12	3.449	651	656	659	rBV2	250	292	0.03%	0.003%
13	3.495	666	670	676	rVB2	146	142	0.01%	0.002%
14	3.546	682	686	687	rBV	189	151	0.01%	0.002%
15	3.675	725	726	732	rVB2	216	187	0.02%	0.002%
16	3.707	732	736	738	rBV	209	180	0.02%	0.002%
17	3.742	744	747	751	rBV	157	163	0.01%	0.002%
18	3.880	787	790	793	rBV	164	140	0.01%	0.001%
19	3.977	814	820	824	rBV2	176	272	0.02%	0.003%
20	4.067	845	848	851	rBV	223	180	0.02%	0.002%
21	4.141	867	871	878	rVB	243	329	0.03%	0.004%
22	4.170	878	880	883	rBV2	191	153	0.01%	0.002%
23	4.363	936	940	943	rBV2	171	160	0.01%	0.002%
24	4.559	994	1001	1003	rBV	224	309	0.03%	0.003%
25	4.633	1008	1024	1061	rBV	147454	387618	33.29%	4.138%
26	4.916	1109	1112	1116	rVB2	233	201	0.02%	0.002%
27	4.945	1116	1121	1127	rBV3	227	217	0.02%	0.002%
28	4.986	1132	1134	1137	rBV2	251	150	0.01%	0.002%
29	5.067	1142	1159	1189	rVB	210375	464108	39.86%	4.955%
30	5.295	1223	1230	1233	rBV2	664	812	0.07%	0.009%
31	5.372	1250	1254	1255	rBV	311	206	0.02%	0.002%
32	5.629	1330	1334	1337	rBV	198	141	0.01%	0.002%
33	5.729	1343	1365	1393	rBV2	429954	1164454	100.00%	12.431%
34	5.951	1431	1434	1437	rBV3	279	231	0.02%	0.002%
35	5.996	1446	1448	1453	rVB2	267	182	0.02%	0.002%
36	6.080	1471	1474	1477	rBV2	192	184	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045118.D
 Acq On : 05 Oct 2021 00:31
 Operator : SY/MD
 Sample : M4023-15 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.112	1481	1484	1486	rVV2	296	226	0.02%	0.002%
38	6.128	1486	1489	1493	rVB3	377	314	0.03%	0.003%
39	6.253	1513	1528	1551	rBV	374342	704367	60.49%	7.520%
40	6.465	1591	1594	1598	rVB2	164	146	0.01%	0.002%
41	6.543	1605	1618	1630	rBV5	12301	24604	2.11%	0.263%
42	6.694	1647	1665	1683	rBV	279712	545063	46.81%	5.819%
43	6.813	1695	1702	1708	rBV3	634	960	0.08%	0.010%
44	6.893	1723	1727	1730	rBV2	205	216	0.02%	0.002%
45	6.964	1746	1749	1754	rBV2	215	198	0.02%	0.002%
46	7.047	1769	1775	1784	rVB4	842	1301	0.11%	0.014%
47	7.089	1784	1788	1790	rBV2	181	179	0.02%	0.002%
48	7.131	1797	1801	1805	rVB2	176	205	0.02%	0.002%
49	7.154	1805	1808	1810	rBV2	212	146	0.01%	0.002%
50	7.186	1810	1818	1828	rVV3	2941	4712	0.40%	0.050%
51	7.568	1924	1937	1957	rBV	150213	262861	22.57%	2.806%
52	7.690	1968	1975	1984	rVB2	1609	2441	0.21%	0.026%
53	7.748	1989	1993	1996	rBV2	193	211	0.02%	0.002%
54	7.899	2026	2040	2056	rVV	515165	867401	74.49%	9.260%
55	7.973	2056	2063	2077	rVB	7557	13465	1.16%	0.144%
56	8.182	2114	2128	2148	rBV	106833	176897	15.19%	1.889%
57	8.308	2162	2167	2171	rVB	309	269	0.02%	0.003%
58	8.337	2171	2176	2177	rBV2	187	152	0.01%	0.002%
59	8.420	2191	2202	2205	rBV2	168	361	0.03%	0.004%
60	8.478	2216	2220	2223	rBV2	282	267	0.02%	0.003%
61	8.555	2238	2244	2252	rBV4	1313	1677	0.14%	0.018%
62	8.642	2257	2271	2310	rBV	496393	875992	75.23%	9.352%
63	8.899	2347	2351	2353	rBV	197	170	0.01%	0.002%
64	9.054	2391	2399	2402	rBV2	243	380	0.03%	0.004%
65	9.211	2445	2448	2453	rVB2	154	177	0.02%	0.002%
66	9.420	2500	2513	2536	rBV	524577	863585	74.16%	9.219%
67	9.571	2555	2560	2567	rVB3	760	1018	0.09%	0.011%
68	9.623	2573	2576	2583	rVB2	210	255	0.02%	0.003%
69	9.658	2583	2587	2590	rBV	153	139	0.01%	0.001%
70	9.700	2590	2600	2610	rVV3	1360	2093	0.18%	0.022%
71	9.986	2684	2689	2692	rBV	237	264	0.02%	0.003%
72	10.237	2763	2767	2770	rBV	206	226	0.02%	0.002%
73	10.301	2782	2787	2790	rBV2	229	266	0.02%	0.003%
74	10.362	2801	2806	2812	rBV2	324	453	0.04%	0.005%
75	10.433	2826	2828	2834	rVB2	214	207	0.02%	0.002%
76	10.462	2834	2837	2840	rBV2	177	154	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045118.D
 Acq On : 05 Oct 2021 00:31
 Operator : SY/MD
 Sample : M4023-15 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.485	2840	2844	2850	rVB	304	263	0.02%	0.003%
78	10.674	2896	2903	2911	rBV4	1259	1744	0.15%	0.019%
79	10.761	2917	2930	2952	rVB	448004	708141	60.81%	7.560%
80	10.915	2973	2978	2984	rVB3	244	285	0.02%	0.003%
81	11.005	3001	3006	3008	rBV2	300	318	0.03%	0.003%
82	11.089	3029	3032	3034	rBV3	385	332	0.03%	0.004%
83	11.173	3051	3058	3063	rBV2	271	489	0.04%	0.005%
84	11.259	3079	3085	3087	rBV2	213	194	0.02%	0.002%
85	11.349	3111	3113	3117	rBV	169	153	0.01%	0.002%
86	11.407	3126	3131	3138	rBV2	264	357	0.03%	0.004%
87	11.462	3140	3148	3159	rVB4	1664	3257	0.28%	0.035%
88	11.568	3174	3181	3183	rBV	248	272	0.02%	0.003%
89	11.674	3210	3214	3217	rBV2	212	235	0.02%	0.003%
90	11.816	3245	3258	3276	rBV	521955	818329	70.28%	8.736%
91	11.928	3290	3293	3294	rBV2	309	170	0.01%	0.002%
92	11.976	3303	3308	3316	rVB4	1189	1452	0.12%	0.016%
93	12.195	3363	3376	3397	rBV	523743	834331	71.65%	8.907%
94	12.591	3496	3499	3502	rBV	174	170	0.01%	0.002%
95	12.645	3512	3516	3519	rBV2	372	400	0.03%	0.004%
96	13.478	3771	3775	3777	rBV2	276	220	0.02%	0.002%
97	14.089	3956	3965	3966	rBV2	711	814	0.07%	0.009%
98	14.716	4156	4160	4163	rBV2	420	363	0.03%	0.004%
99	15.237	4316	4322	4328	rBV6	713	1119	0.10%	0.012%
100	15.578	4424	4428	4432	rBV3	350	420	0.04%	0.004%



Sum of corrected areas: 9366968

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045118.D
Acq On : 05 Oct 2021 00:31
Operator : SY/MD
Sample : M4023-15 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

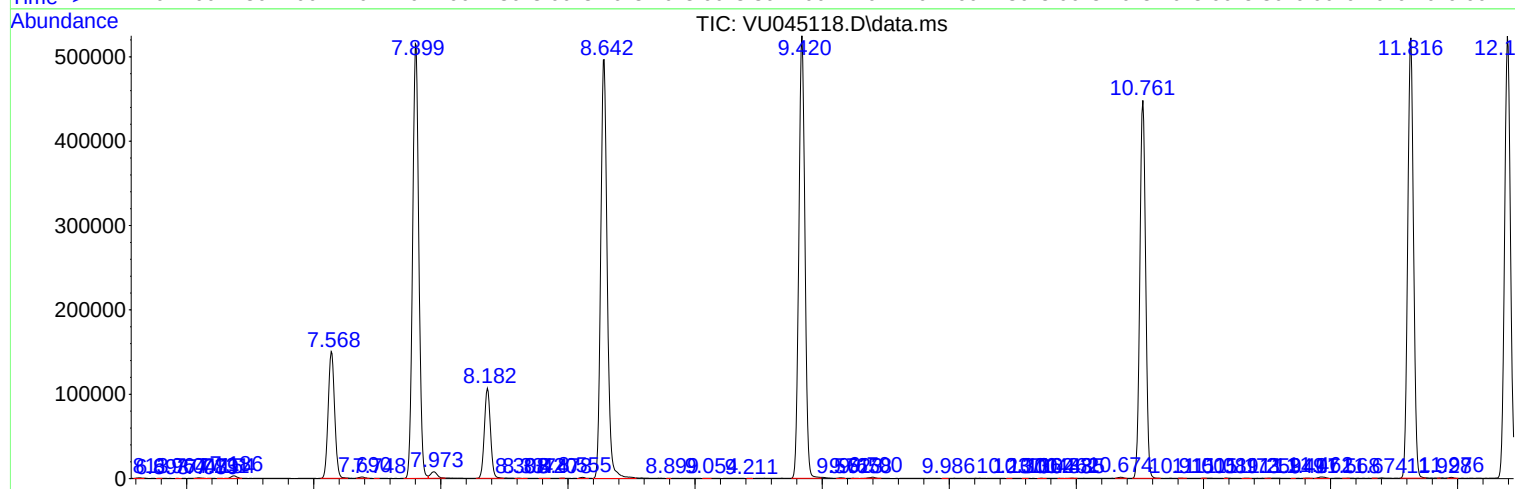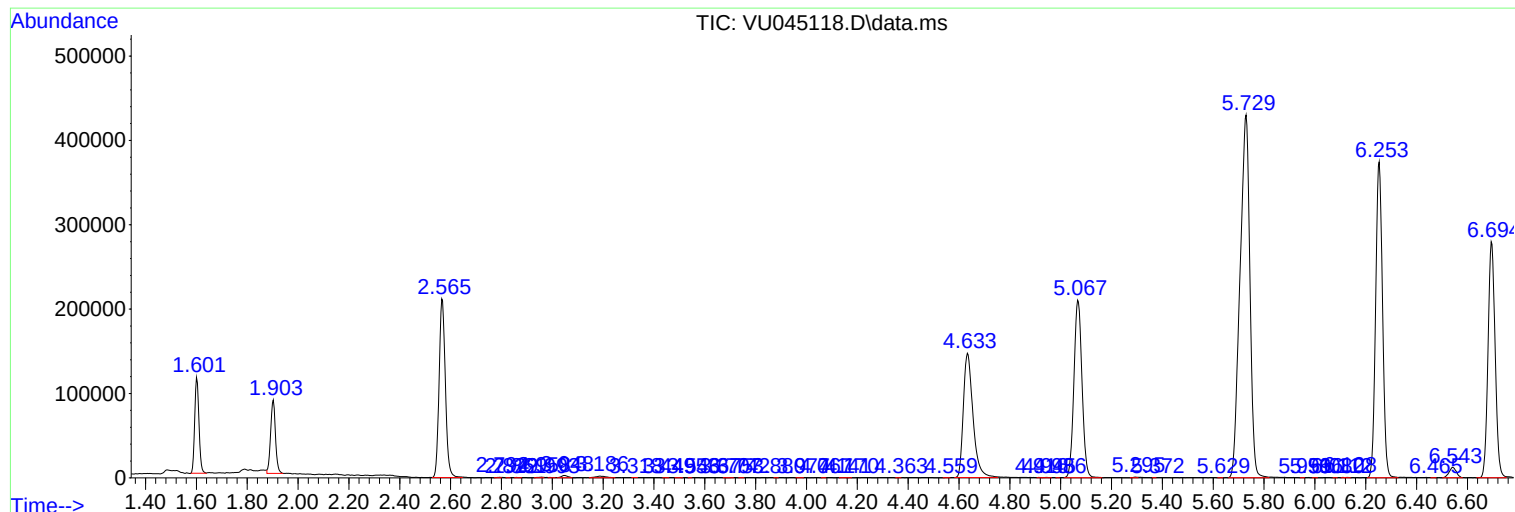

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045118.D
Acq On : 05 Oct 2021 00:31
Operator : SY/MD
Sample : M4023-15 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045118.D
Acq On : 05 Oct 2021 00:31
Operator : SY/MD
Sample : M4023-15 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------