

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045119.D
 Acq On : 05 Oct 2021 00:54
 Operator : SY/MD
 Sample : M4023-16 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045119.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	92	rBV	115713	131329	11.27%	1.401%
2	1.903	168	175	193	rVB	117682	150548	12.92%	1.606%
3	2.462	346	349	351	rBV	224	150	0.01%	0.002%
4	2.568	369	382	409	rBV	210046	359077	30.81%	3.830%
5	2.736	431	434	438	rBV	238	207	0.02%	0.002%
6	2.861	469	473	481	rVB3	206	257	0.02%	0.003%
7	2.919	487	491	496	rVB	163	145	0.01%	0.002%
8	2.961	496	504	505	rBV2	636	842	0.07%	0.009%
9	3.051	522	532	542	rVB4	2177	3880	0.33%	0.041%
10	3.144	556	561	566	rVV2	248	347	0.03%	0.004%
11	3.192	566	576	588	rVV2	1423	3399	0.29%	0.036%
12	3.247	591	593	597	rVV2	243	181	0.02%	0.002%
13	3.279	600	603	607	rVB	235	174	0.01%	0.002%
14	3.308	607	612	614	rBV	175	165	0.01%	0.002%
15	3.646	711	717	721	rBV	198	251	0.02%	0.003%
16	3.765	749	754	758	rBV	198	146	0.01%	0.002%
17	3.919	792	802	805	rBV	227	388	0.03%	0.004%
18	4.099	852	858	861	rBV2	194	167	0.01%	0.002%
19	4.173	879	881	885	rVB	184	148	0.01%	0.002%
20	4.208	888	892	900	rVB	247	305	0.03%	0.003%
21	4.250	900	905	911	rBV2	238	380	0.03%	0.004%
22	4.298	916	920	924	rBV2	221	174	0.01%	0.002%
23	4.334	928	931	939	rVB2	214	352	0.03%	0.004%
24	4.395	946	950	952	rBV	247	183	0.02%	0.002%
25	4.485	975	978	981	rVB	231	161	0.01%	0.002%
26	4.633	1009	1024	1061	rBV	148687	399439	34.27%	4.260%
27	4.800	1074	1076	1084	rVB2	522	414	0.04%	0.004%
28	4.880	1098	1101	1105	rVB3	298	278	0.02%	0.003%
29	4.935	1113	1118	1119	rBV2	207	170	0.01%	0.002%
30	4.996	1135	1137	1142	rVB3	323	256	0.02%	0.003%
31	5.067	1142	1159	1189	rBV	212537	465062	39.91%	4.960%
32	5.215	1202	1205	1208	rBV4	271	145	0.01%	0.002%
33	5.237	1210	1212	1218	rVB	362	245	0.02%	0.003%
34	5.298	1224	1231	1236	rVB3	442	661	0.06%	0.007%
35	5.343	1242	1245	1247	rBV	173	143	0.01%	0.002%
36	5.375	1251	1255	1256	rBV2	325	228	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045119.D
 Acq On : 05 Oct 2021 00:54
 Operator : SY/MD
 Sample : M4023-16 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.385	1256	1258	1260	rVB	316	157	0.01%	0.002%
38	5.459	1278	1281	1285	rVB2	206	154	0.01%	0.002%
39	5.530	1301	1303	1308	rVB	232	185	0.02%	0.002%
40	5.588	1314	1321	1325	rBV	561	797	0.07%	0.009%
41	5.729	1342	1365	1388	rBV2	432759	1165416	100.00%	12.431%
42	5.977	1438	1442	1444	rBV2	327	194	0.02%	0.002%
43	6.035	1457	1460	1466	rBV2	230	221	0.02%	0.002%
44	6.118	1483	1486	1491	rVB2	383	391	0.03%	0.004%
45	6.253	1512	1528	1550	rBV	372519	703178	60.34%	7.500%
46	6.539	1606	1617	1628	rVB7	6974	14474	1.24%	0.154%
47	6.584	1628	1631	1633	rBV	184	151	0.01%	0.002%
48	6.694	1651	1665	1685	rBV	281090	550821	47.26%	5.875%
49	7.028	1762	1769	1770	rBV	247	263	0.02%	0.003%
50	7.051	1770	1776	1785	rVB4	881	1363	0.12%	0.015%
51	7.092	1785	1789	1792	rBV2	252	240	0.02%	0.003%
52	7.186	1807	1818	1828	rBV4	3067	5333	0.46%	0.057%
53	7.269	1839	1844	1845	rBV2	221	202	0.02%	0.002%
54	7.372	1872	1876	1881	rBV2	234	293	0.03%	0.003%
55	7.504	1912	1917	1922	rBV2	209	216	0.02%	0.002%
56	7.568	1922	1937	1956	rBV	151698	263724	22.63%	2.813%
57	7.694	1969	1976	1984	rVB2	1557	2486	0.21%	0.027%
58	7.796	2007	2008	2014	rVB2	378	252	0.02%	0.003%
59	7.903	2026	2041	2056	rBV	505439	871472	74.78%	9.295%
60	7.973	2057	2063	2077	rVB2	7611	12899	1.11%	0.138%
61	8.124	2108	2110	2114	rBV2	195	152	0.01%	0.002%
62	8.182	2116	2128	2148	rVV	106196	178040	15.28%	1.899%
63	8.317	2166	2170	2174	rBV2	210	249	0.02%	0.003%
64	8.555	2236	2244	2250	rBV5	955	1409	0.12%	0.015%
65	8.639	2257	2270	2298	rBV	504896	873964	74.99%	9.322%
66	8.851	2331	2336	2339	rBV2	220	172	0.01%	0.002%
67	8.941	2357	2364	2367	rBV2	192	257	0.02%	0.003%
68	8.976	2372	2375	2378	rBV	279	236	0.02%	0.003%
69	9.009	2382	2385	2392	rVB	272	344	0.03%	0.004%
70	9.044	2392	2396	2401	rBV	233	257	0.02%	0.003%
71	9.301	2473	2476	2483	rBV2	171	228	0.02%	0.002%
72	9.420	2500	2513	2547	rBV	519107	862135	73.98%	9.196%
73	9.571	2554	2560	2568	rBV3	785	1069	0.09%	0.011%
74	9.694	2591	2598	2606	rBV	1320	1775	0.15%	0.019%
75	9.751	2610	2616	2624	rBV2	256	421	0.04%	0.004%
76	9.793	2624	2629	2632	rBV2	171	227	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045119.D
 Acq On : 05 Oct 2021 00:54
 Operator : SY/MD
 Sample : M4023-16 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.105	2714	2726	2729	rBV3	454	803	0.07%	0.009%
78	10.214	2756	2760	2763	rBV	203	180	0.02%	0.002%
79	10.587	2873	2876	2882	rVB	221	216	0.02%	0.002%
80	10.674	2896	2903	2912	rVB3	1324	1677	0.14%	0.018%
81	10.761	2917	2930	2950	rBV	445674	701878	60.23%	7.486%
82	10.867	2959	2963	2968	rVB3	191	182	0.02%	0.002%
83	10.970	2992	2995	2997	rBV2	192	149	0.01%	0.002%
84	11.005	3000	3006	3010	rVV3	304	367	0.03%	0.004%
85	11.462	3140	3148	3159	rBV4	1567	2967	0.25%	0.032%
86	11.693	3217	3220	3226	rBV3	726	802	0.07%	0.009%
87	11.735	3229	3233	3237	rVB	276	266	0.02%	0.003%
88	11.816	3244	3258	3275	rBV	515468	805329	69.10%	8.590%
89	12.054	3328	3332	3334	rBV	218	174	0.01%	0.002%
90	12.082	3336	3341	3344	rVV2	157	176	0.02%	0.002%
91	12.195	3362	3376	3392	rBV	509849	821602	70.50%	8.763%
92	12.417	3441	3445	3454	rVB2	242	375	0.03%	0.004%
93	12.854	3578	3581	3583	rVB2	251	151	0.01%	0.002%
94	13.311	3718	3723	3725	rBV	268	266	0.02%	0.003%
95	14.253	4013	4016	4017	rBV	365	197	0.02%	0.002%
96	14.301	4028	4031	4033	rBV2	225	157	0.01%	0.002%
97	14.500	4090	4093	4095	rBV2	370	317	0.03%	0.003%
98	14.581	4114	4118	4128	rBV3	440	563	0.05%	0.006%
99	14.732	4162	4165	4166	rBV2	286	147	0.01%	0.002%
100	14.925	4222	4225	4227	rBV	384	290	0.02%	0.003%




Sum of corrected areas: 9375445

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045119.D
Acq On : 05 Oct 2021 00:54
Operator : SY/MD
Sample : M4023-16 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

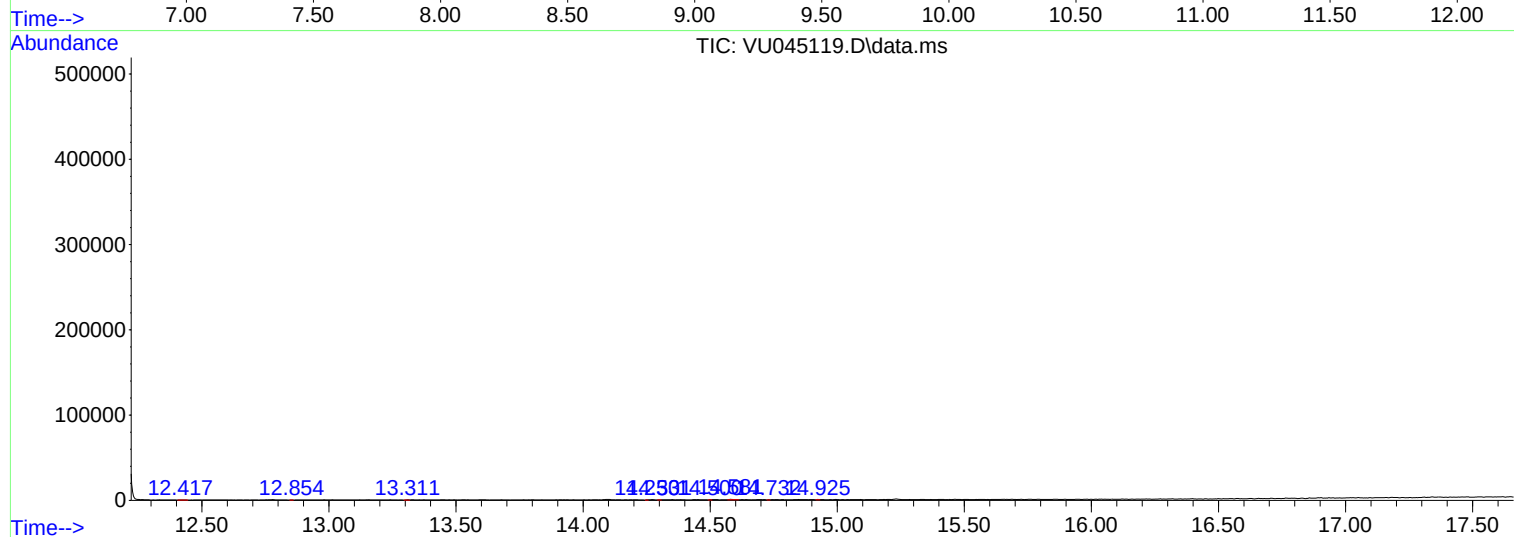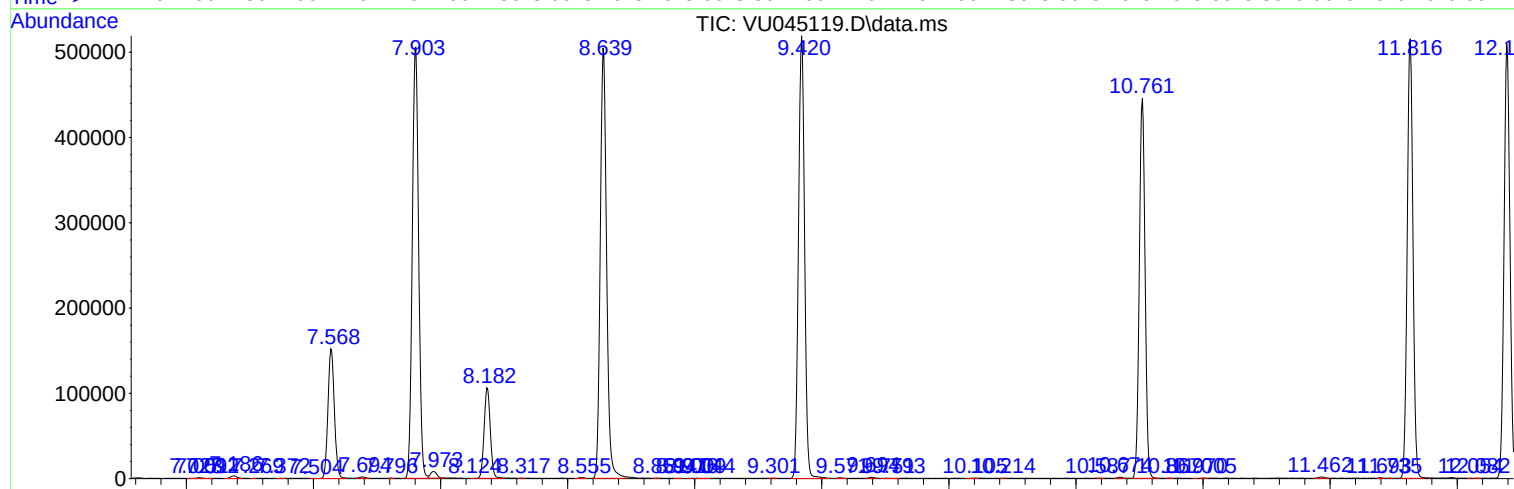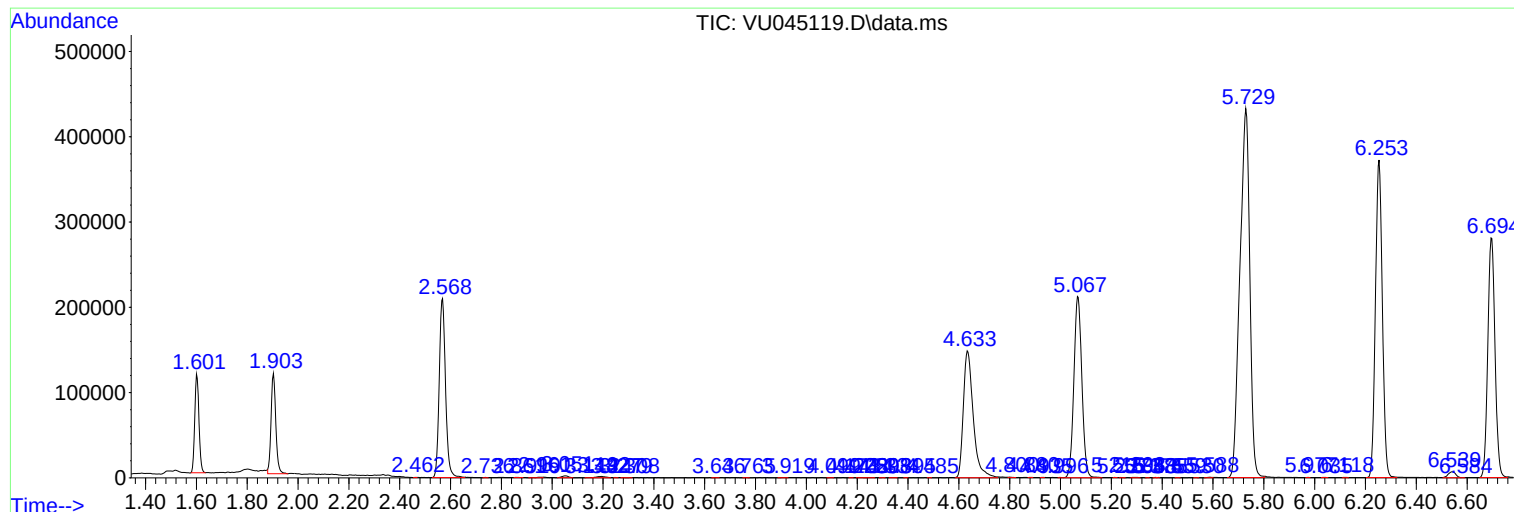

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045119.D
Acq On : 05 Oct 2021 00:54
Operator : SY/MD
Sample : M4023-16 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045119.D
Acq On : 05 Oct 2021 00:54
Operator : SY/MD
Sample : M4023-16 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
