

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045120.D
 Acq On : 05 Oct 2021 01:18
 Operator : SY/MD
 Sample : M4023-17 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	97	rVB	121022	142827	11.81%	1.473%
2	1.906	169	176	192	rVB	83818	105173	8.69%	1.085%
3	2.565	369	381	410	rBV	218914	369162	30.52%	3.808%
4	2.729	430	432	436	rBV2	253	197	0.02%	0.002%
5	2.787	446	450	451	rBV2	271	185	0.02%	0.002%
6	2.797	451	453	457	rVB2	376	271	0.02%	0.003%
7	2.903	483	486	492	rVB2	225	187	0.02%	0.002%
8	2.961	498	504	518	rVB2	765	1442	0.12%	0.015%
9	3.047	523	531	542	rBV2	2104	3646	0.30%	0.038%
10	3.147	559	562	566	rBV2	234	181	0.01%	0.002%
11	3.192	566	576	577	rBV2	1531	1991	0.16%	0.021%
12	3.263	593	598	602	rVB2	237	221	0.02%	0.002%
13	3.475	661	664	667	rBV2	216	146	0.01%	0.002%
14	3.607	700	705	708	rBV2	214	223	0.02%	0.002%
15	3.662	716	722	725	rBV2	198	162	0.01%	0.002%
16	3.768	752	755	759	rVB	200	163	0.01%	0.002%
17	3.813	766	769	772	rBV	150	141	0.01%	0.001%
18	3.941	804	809	814	rBV2	205	178	0.01%	0.002%
19	4.086	850	854	858	rBV2	143	187	0.02%	0.002%
20	4.276	909	913	916	rVB2	218	153	0.01%	0.002%
21	4.298	916	920	922	rBV	223	217	0.02%	0.002%
22	4.414	952	956	964	rVB	273	401	0.03%	0.004%
23	4.462	966	971	973	rBV	191	195	0.02%	0.002%
24	4.501	980	983	986	rBV	196	155	0.01%	0.002%
25	4.562	999	1002	1009	rVB2	212	231	0.02%	0.002%
26	4.642	1009	1027	1077	rBV	135169	419239	34.66%	4.324%
27	5.067	1140	1159	1180	rBV	217247	480242	39.70%	4.954%
28	5.298	1225	1231	1236	rVB3	531	686	0.06%	0.007%
29	5.334	1239	1242	1245	rBV2	185	156	0.01%	0.002%
30	5.388	1256	1259	1264	rBV2	186	184	0.02%	0.002%
31	5.520	1295	1300	1306	rBV2	171	243	0.02%	0.003%
32	5.588	1317	1321	1326	rBV2	233	306	0.03%	0.003%
33	5.642	1334	1338	1340	rBV2	171	161	0.01%	0.002%
34	5.729	1343	1365	1396	rVV2	442008	1209704	100.00%	12.478%
35	6.067	1466	1470	1474	rVB2	184	165	0.01%	0.002%
36	6.112	1478	1484	1487	rBV2	352	456	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045120.D
 Acq On : 05 Oct 2021 01:18
 Operator : SY/MD
 Sample : M4023-17 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.166	1495	1501	1506	rVB2	223	285	0.02%	0.003%
38	6.253	1512	1528	1548	rBV	381692	717748	59.33%	7.404%
39	6.424	1577	1581	1586	rVB3	323	343	0.03%	0.004%
40	6.449	1586	1589	1593	rVB2	366	295	0.02%	0.003%
41	6.485	1593	1600	1604	rBV2	181	276	0.02%	0.003%
42	6.533	1604	1615	1627	rBV7	4748	9829	0.81%	0.101%
43	6.694	1651	1665	1689	rBV	292351	570804	47.19%	5.888%
44	6.787	1692	1694	1695	rVV	519	206	0.02%	0.002%
45	6.813	1695	1702	1708	rVV4	823	1123	0.09%	0.012%
46	6.864	1712	1718	1720	rBV	216	241	0.02%	0.002%
47	6.906	1727	1731	1737	rBV2	230	273	0.02%	0.003%
48	6.951	1741	1745	1751	rBV2	234	298	0.02%	0.003%
49	7.054	1769	1777	1784	rBV4	590	1002	0.08%	0.010%
50	7.147	1804	1806	1810	rBV2	183	174	0.01%	0.002%
51	7.189	1810	1819	1833	rVV7	3035	6078	0.50%	0.063%
52	7.568	1924	1937	1959	rBV	152869	269258	22.26%	2.777%
53	7.687	1968	1974	1985	rVB4	1763	2944	0.24%	0.030%
54	7.903	2026	2041	2057	rBV	523378	903050	74.65%	9.315%
55	7.970	2057	2062	2074	rVB	7588	12412	1.03%	0.128%
56	8.182	2115	2128	2151	rBV	108755	185182	15.31%	1.910%
57	8.459	2210	2214	2216	rBV	256	209	0.02%	0.002%
58	8.552	2239	2243	2245	rBV3	765	602	0.05%	0.006%
59	8.587	2250	2254	2257	rBV	160	175	0.01%	0.002%
60	8.645	2258	2272	2301	rBV	516296	922530	76.26%	9.516%
61	8.867	2338	2341	2346	rVB2	283	232	0.02%	0.002%
62	8.899	2346	2351	2352	rBV	167	163	0.01%	0.002%
63	9.005	2381	2384	2386	rBV2	196	164	0.01%	0.002%
64	9.420	2500	2513	2549	rVV	541415	885084	73.17%	9.130%
65	9.571	2556	2560	2570	rVB3	629	681	0.06%	0.007%
66	9.697	2592	2599	2609	rBV3	1583	2223	0.18%	0.023%
67	9.793	2626	2629	2634	rVB2	213	206	0.02%	0.002%
68	9.819	2634	2637	2639	rBV	174	155	0.01%	0.002%
69	9.857	2645	2649	2651	rBV	262	212	0.02%	0.002%
70	9.967	2679	2683	2685	rBV	220	169	0.01%	0.002%
71	10.079	2714	2718	2720	rBV2	208	174	0.01%	0.002%
72	10.102	2722	2725	2730	rVB3	478	479	0.04%	0.005%
73	10.488	2842	2845	2849	rVB3	303	243	0.02%	0.003%
74	10.677	2895	2904	2910	rBV4	1579	2178	0.18%	0.022%
75	10.761	2917	2930	2947	rVV	469816	745711	61.64%	7.692%
76	10.835	2950	2953	2956	rVB	354	253	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045120.D
 Acq On : 05 Oct 2021 01:18
 Operator : SY/MD
 Sample : M4023-17 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.002	2999	3005	3012	rVB3	308	413	0.03%	0.004%
78	11.063	3021	3024	3029	rBV	189	207	0.02%	0.002%
79	11.095	3029	3034	3039	rVB3	469	528	0.04%	0.005%
80	11.124	3039	3043	3044	rBV	295	172	0.01%	0.002%
81	11.304	3093	3099	3104	rBV2	321	380	0.03%	0.004%
82	11.330	3104	3107	3112	rVV	163	152	0.01%	0.002%
83	11.468	3141	3150	3162	rBV6	1361	2602	0.22%	0.027%
84	11.674	3209	3214	3216	rBV2	173	177	0.01%	0.002%
85	11.693	3216	3220	3227	rVB2	630	700	0.06%	0.007%
86	11.816	3242	3258	3277	rBV	533052	834460	68.98%	8.607%
87	12.195	3362	3376	3392	rBV	537947	867967	71.75%	8.953%
88	12.359	3424	3427	3430	rVB2	178	141	0.01%	0.001%
89	12.504	3468	3472	3477	rBV2	201	263	0.02%	0.003%
90	12.716	3535	3538	3542	rBV2	214	246	0.02%	0.003%
91	12.832	3567	3574	3577	rBV2	279	419	0.03%	0.004%
92	12.941	3605	3608	3610	rBV	188	153	0.01%	0.002%
93	13.005	3625	3628	3631	rBV	185	151	0.01%	0.002%
94	13.076	3647	3650	3654	rVB2	209	140	0.01%	0.001%
95	13.819	3878	3881	3883	rBV	201	167	0.01%	0.002%
96	14.089	3960	3965	3972	rBV	554	822	0.07%	0.008%
97	14.510	4094	4096	4102	rVB2	252	189	0.02%	0.002%
98	14.574	4112	4116	4117	rBV2	331	231	0.02%	0.002%
99	15.060	4264	4267	4269	rBV	312	228	0.02%	0.002%
100	15.227	4315	4319	4320	rBV3	601	481	0.04%	0.005%


Sum of corrected areas: 9694630

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045120.D
Acq On : 05 Oct 2021 01:18
Operator : SY/MD
Sample : M4023-17 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

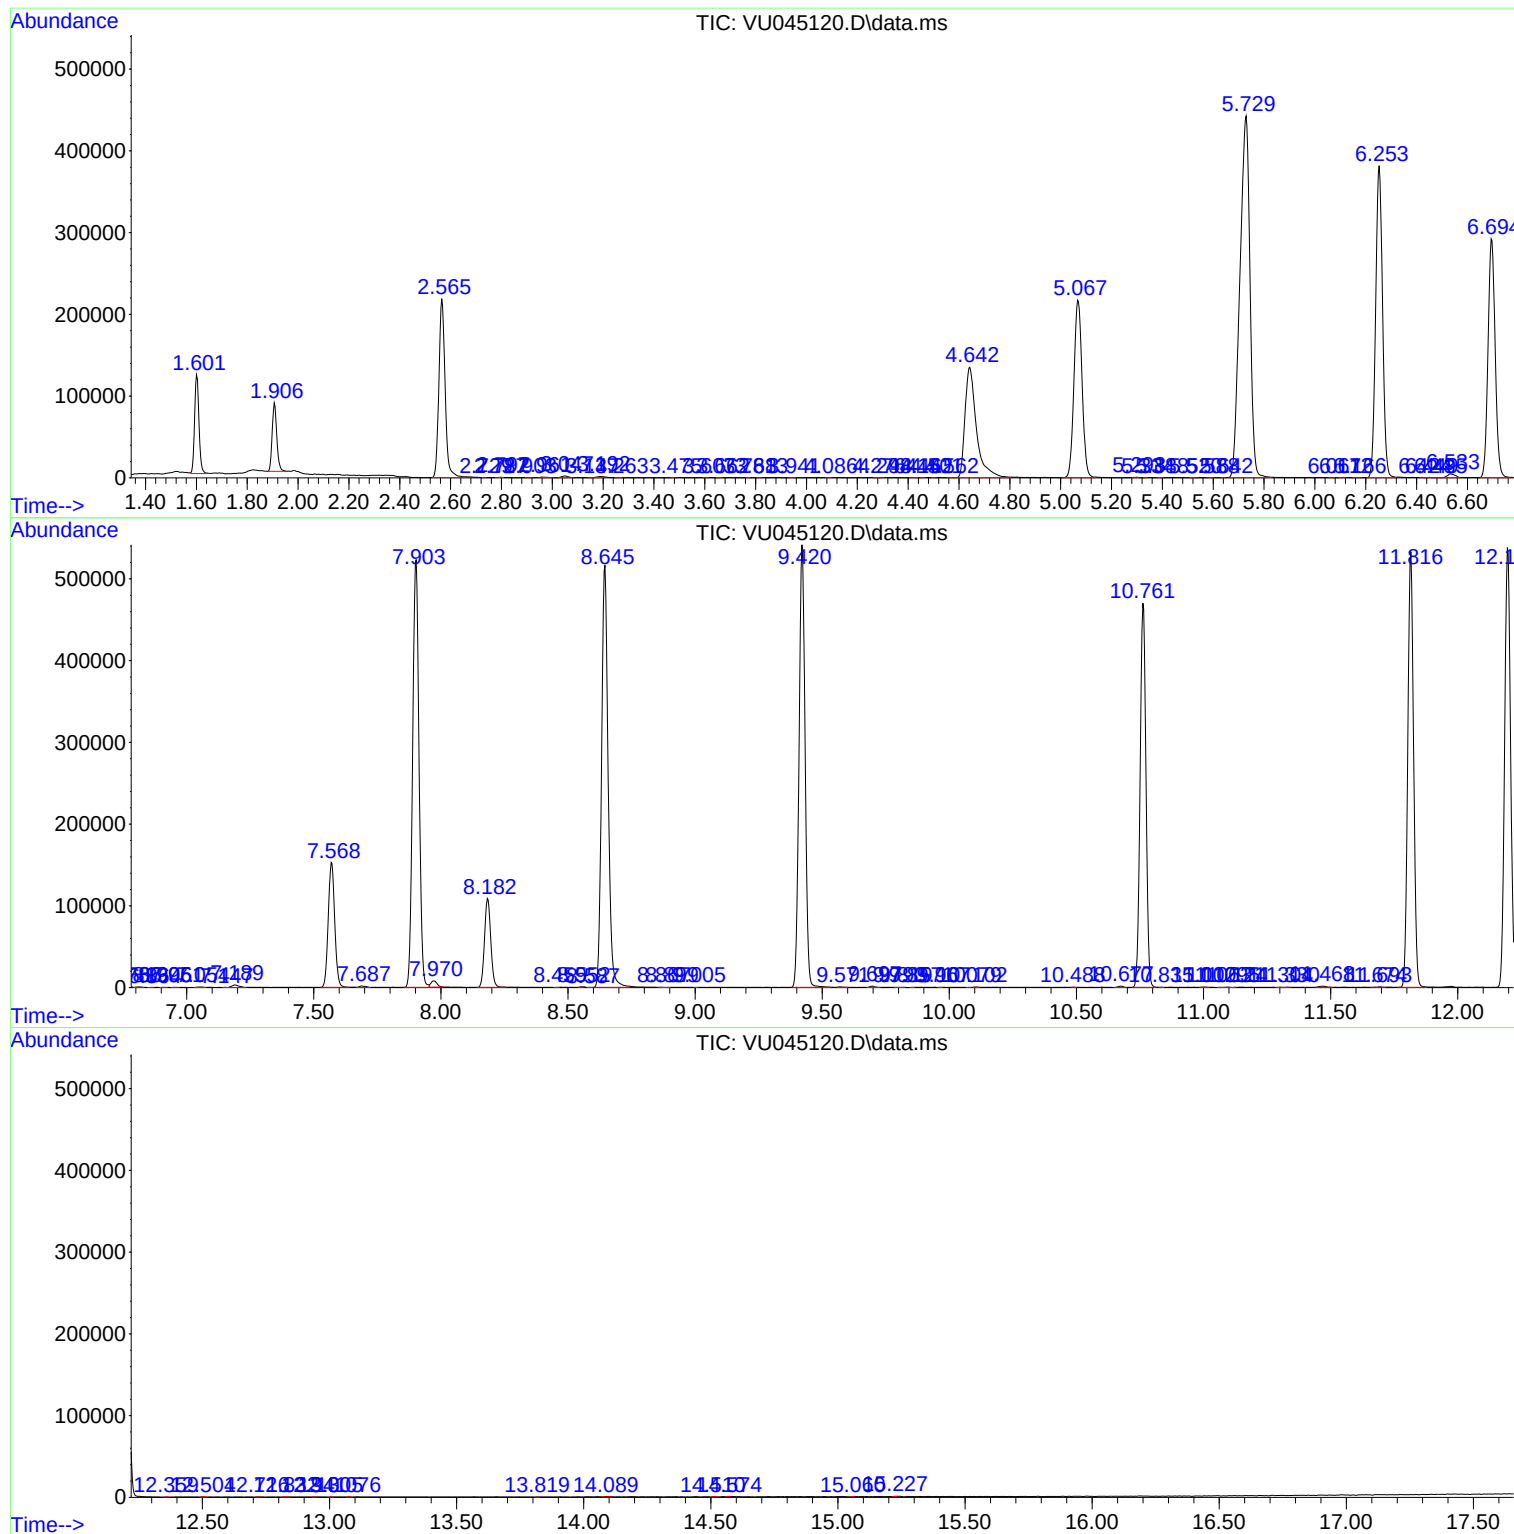

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045120.D
Acq On : 05 Oct 2021 01:18
Operator : SY/MD
Sample : M4023-17 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045120.D
Acq On : 05 Oct 2021 01:18
Operator : SY/MD
Sample : M4023-17 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------