

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045121.D
 Acq On : 05 Oct 2021 01:41
 Operator : SY/MD
 Sample : M4023-14 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045121.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	100	rVB	115448	133645	11.50%	1.426%
2	1.906	169	176	193	rVB	78580	102115	8.79%	1.089%
3	2.565	369	381	413	rVV	210288	356141	30.65%	3.799%
4	2.697	420	422	427	rVB2	435	292	0.03%	0.003%
5	2.719	427	429	435	rVB3	334	265	0.02%	0.003%
6	2.748	435	438	441	rVB2	240	170	0.01%	0.002%
7	2.867	470	475	477	rBV2	201	212	0.02%	0.002%
8	3.051	523	532	543	rVB3	2288	3983	0.34%	0.042%
9	3.189	565	575	590	rVV2	1831	4389	0.38%	0.047%
10	3.314	610	614	618	rBV2	169	175	0.02%	0.002%
11	3.382	631	635	638	rBV	191	174	0.01%	0.002%
12	3.443	652	654	659	rVB2	220	205	0.02%	0.002%
13	3.475	659	664	668	rBV	205	204	0.02%	0.002%
14	3.543	682	685	688	rBV	185	175	0.02%	0.002%
15	3.559	688	690	696	rVB	175	174	0.01%	0.002%
16	3.948	808	811	815	rBV	194	179	0.02%	0.002%
17	3.993	818	825	829	rVB2	273	330	0.03%	0.004%
18	4.256	902	907	909	rBV2	223	268	0.02%	0.003%
19	4.485	975	978	981	rBV2	224	205	0.02%	0.002%
20	4.642	1010	1027	1074	rBV	126558	408107	35.13%	4.354%
21	4.944	1118	1121	1123	rBV	238	172	0.01%	0.002%
22	4.999	1135	1138	1141	rBV2	269	237	0.02%	0.003%
23	5.067	1143	1159	1186	rVV	209539	462480	39.81%	4.934%
24	5.565	1308	1314	1318	rBV2	224	320	0.03%	0.003%
25	5.729	1343	1365	1394	rBV2	427030	1161864	100.00%	12.394%
26	5.928	1425	1427	1430	rVB3	288	176	0.02%	0.002%
27	5.986	1443	1445	1450	rVB	364	262	0.02%	0.003%
28	6.115	1481	1485	1487	rBV2	329	300	0.03%	0.003%
29	6.169	1498	1502	1506	rVB2	192	188	0.02%	0.002%
30	6.202	1506	1512	1513	rBV2	262	249	0.02%	0.003%
31	6.253	1513	1528	1555	rVV	371512	695946	59.90%	7.424%
32	6.539	1602	1617	1626	rBV7	4605	9039	0.78%	0.096%
33	6.645	1644	1650	1651	rBV	244	194	0.02%	0.002%
34	6.694	1651	1665	1693	rVV	281175	549483	47.29%	5.862%
35	6.813	1696	1702	1707	rVB3	624	688	0.06%	0.007%
36	6.980	1750	1754	1755	rBV	227	176	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045121.D
 Acq On : 05 Oct 2021 01:41
 Operator : SY/MD
 Sample : M4023-14 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.050	1770	1776	1785	rVB2	493	787	0.07%	0.008%
38	7.189	1811	1819	1831	rVB3	3103	5457	0.47%	0.058%
39	7.243	1831	1836	1841	rVB2	327	303	0.03%	0.003%
40	7.568	1925	1937	1958	rBV	146324	260354	22.41%	2.777%
41	7.690	1968	1975	1983	rBV3	1776	2961	0.25%	0.032%
42	7.784	2001	2004	2008	rBV3	286	264	0.02%	0.003%
43	7.841	2018	2022	2026	rBV2	189	229	0.02%	0.002%
44	7.903	2026	2041	2056	rBV	502950	869027	74.80%	9.270%
45	7.970	2057	2062	2074	rVB	7245	11629	1.00%	0.124%
46	8.112	2103	2106	2109	rBV	184	166	0.01%	0.002%
47	8.182	2116	2128	2149	rVV	104816	176221	15.17%	1.880%
48	8.407	2195	2198	2202	rVV	237	201	0.02%	0.002%
49	8.478	2209	2220	2223	rBV3	386	633	0.05%	0.007%
50	8.552	2241	2243	2245	rBV2	523	346	0.03%	0.004%
51	8.645	2259	2272	2302	rVV	491293	889329	76.54%	9.487%
52	8.880	2342	2345	2347	rBV	255	209	0.02%	0.002%
53	9.034	2388	2393	2396	rVV2	232	219	0.02%	0.002%
54	9.057	2396	2400	2405	rBV2	144	183	0.02%	0.002%
55	9.128	2419	2422	2425	rBV	168	157	0.01%	0.002%
56	9.250	2457	2460	2463	rBV	218	178	0.02%	0.002%
57	9.420	2494	2513	2534	rBV	528155	868093	74.72%	9.260%
58	9.697	2592	2599	2608	rVB3	1262	1798	0.15%	0.019%
59	9.777	2620	2624	2629	rBV	248	200	0.02%	0.002%
60	9.957	2677	2680	2683	rBV	203	191	0.02%	0.002%
61	10.002	2688	2694	2697	rVB2	268	297	0.03%	0.003%
62	10.025	2697	2701	2706	rBV2	168	236	0.02%	0.003%
63	10.076	2712	2717	2721	rBV2	209	225	0.02%	0.002%
64	10.102	2721	2725	2732	rVB3	599	732	0.06%	0.008%
65	10.140	2732	2737	2739	rBV	272	253	0.02%	0.003%
66	10.201	2753	2756	2760	rBV2	177	187	0.02%	0.002%
67	10.275	2776	2779	2781	rBV2	229	187	0.02%	0.002%
68	10.359	2801	2805	2806	rBV2	198	175	0.02%	0.002%
69	10.677	2896	2904	2910	rBV2	1371	1841	0.16%	0.020%
70	10.761	2917	2930	2953	rBV	440959	719634	61.94%	7.677%
71	10.873	2962	2965	2973	rVB3	290	339	0.03%	0.004%
72	10.915	2973	2978	2984	rVB3	367	509	0.04%	0.005%
73	10.967	2984	2994	3001	rBV2	256	579	0.05%	0.006%
74	11.002	3001	3005	3010	rBV3	322	398	0.03%	0.004%
75	11.182	3058	3061	3065	rBV2	258	271	0.02%	0.003%
76	11.465	3140	3149	3158	rVB4	1454	2098	0.18%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045121.D
 Acq On : 05 Oct 2021 01:41
 Operator : SY/MD
 Sample : M4023-14 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.578	3181	3184	3189	rVB3	233	221	0.02%	0.002%
78	11.697	3214	3221	3223	rBV4	535	529	0.05%	0.006%
79	11.816	3245	3258	3278	rVV	524836	817684	70.38%	8.723%
80	11.922	3288	3291	3293	rBV2	288	160	0.01%	0.002%
81	11.944	3295	3298	3302	rVV4	334	336	0.03%	0.004%
82	11.973	3304	3307	3312	rVB2	676	567	0.05%	0.006%
83	12.195	3363	3376	3397	rVV	510745	838301	72.15%	8.943%
84	12.488	3461	3467	3470	rBV2	209	259	0.02%	0.003%
85	12.619	3505	3508	3513	rBV	210	235	0.02%	0.003%
86	12.645	3513	3516	3519	rVB2	256	170	0.01%	0.002%
87	12.931	3600	3605	3608	rBV2	229	237	0.02%	0.003%
88	13.147	3669	3672	3675	rBV2	304	242	0.02%	0.003%
89	13.250	3698	3704	3711	rBV2	309	460	0.04%	0.005%
90	13.304	3717	3721	3723	rBV2	217	178	0.02%	0.002%
91	13.854	3890	3892	3895	rBV	245	170	0.01%	0.002%
92	14.050	3949	3953	3955	rBV	275	258	0.02%	0.003%
93	14.092	3963	3966	3979	rVB3	681	1134	0.10%	0.012%
94	14.143	3979	3982	3988	rBV2	395	346	0.03%	0.004%
95	14.172	3988	3991	3998	rBV2	266	275	0.02%	0.003%
96	14.205	3998	4001	4003	rVB	350	207	0.02%	0.002%
97	14.455	4071	4079	4087	rBV2	399	658	0.06%	0.007%
98	14.491	4087	4090	4098	rVV2	293	344	0.03%	0.004%
99	15.227	4316	4319	4323	rBV	470	555	0.05%	0.006%
100	15.529	4409	4413	4415	rBV2	397	389	0.03%	0.004%




Sum of corrected areas: 9374193

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045121.D
Acq On : 05 Oct 2021 01:41
Operator : SY/MD
Sample : M4023-14 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

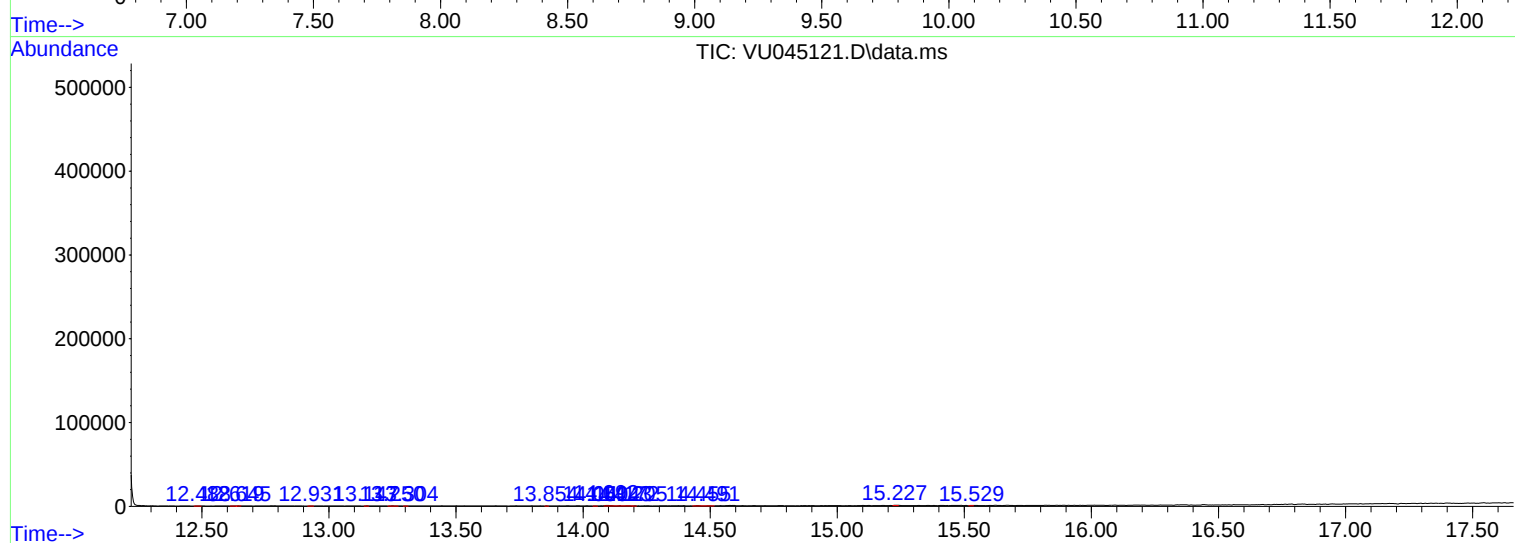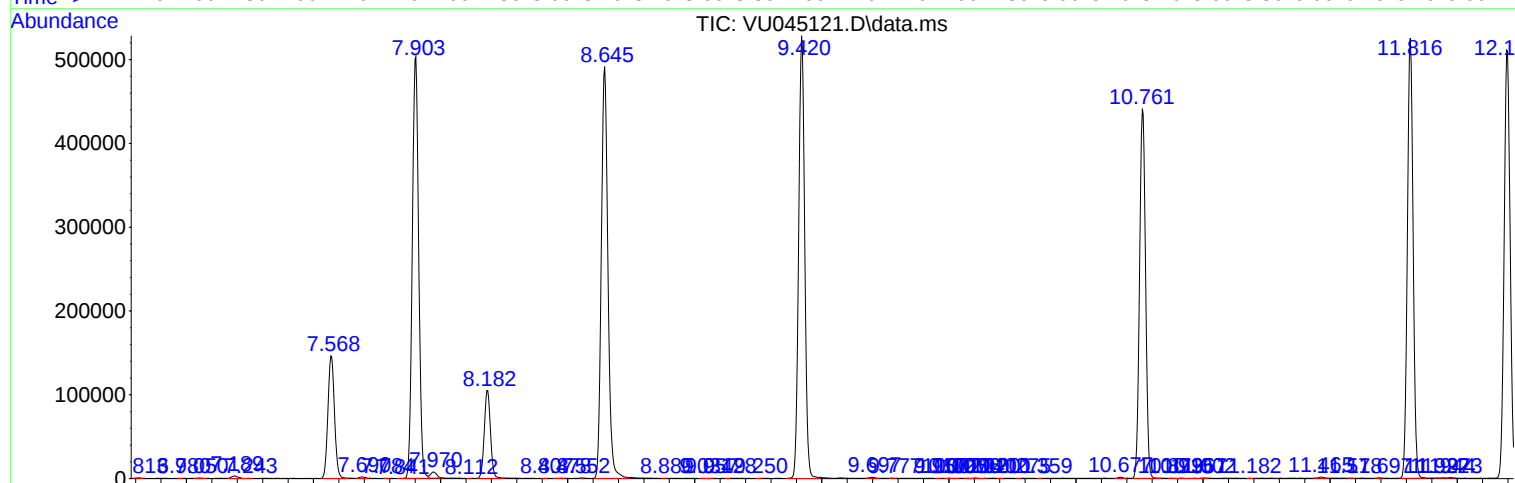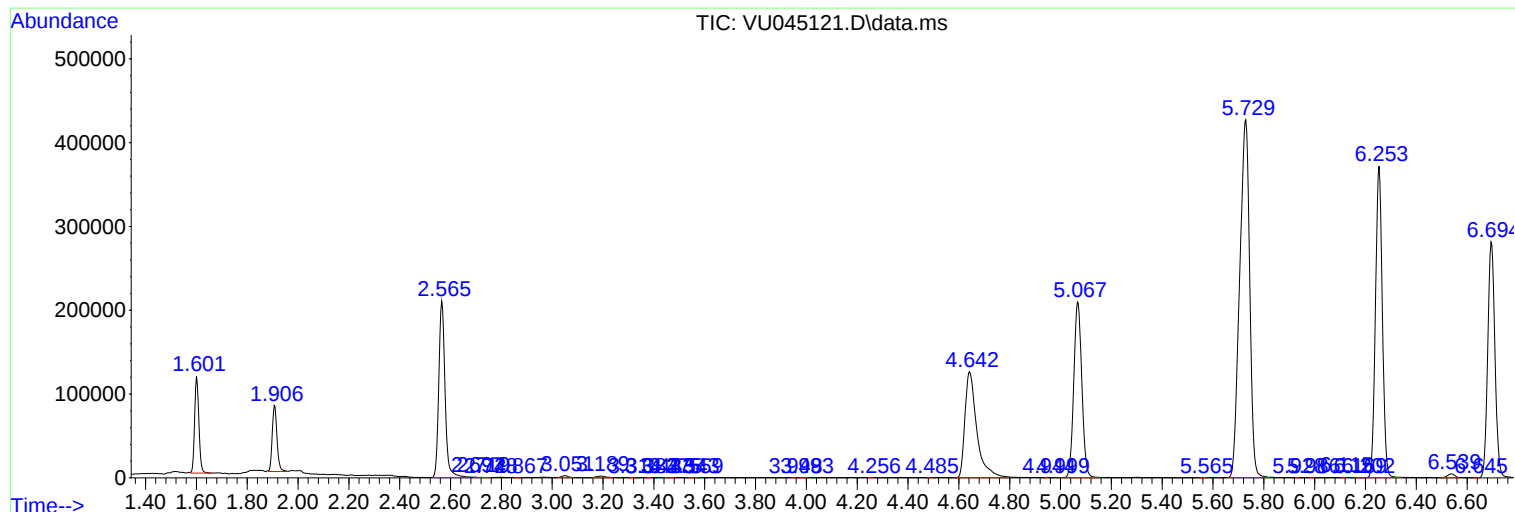

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045121.D
Acq On : 05 Oct 2021 01:41
Operator : SY/MD
Sample : M4023-14 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045121.D
Acq On : 05 Oct 2021 01:41
Operator : SY/MD
Sample : M4023-14 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
