

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045123.D
 Acq On : 05 Oct 2021 02:27
 Operator : SY/MD
 Sample : M4023-20 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	93	rBV	114885	131310	11.28%	1.421%
2	1.906	170	176	188	rVB	83812	105606	9.07%	1.143%
3	2.565	369	381	403	rBV	205201	349274	30.01%	3.781%
4	2.793	449	452	457	rBV2	337	359	0.03%	0.004%
5	2.848	464	469	471	rBV	223	230	0.02%	0.002%
6	2.880	475	479	481	rBV2	196	177	0.02%	0.002%
7	3.047	523	531	541	rVV3	1976	3453	0.30%	0.037%
8	3.308	609	612	615	rVV	213	160	0.01%	0.002%
9	3.433	647	651	654	rBV2	210	187	0.02%	0.002%
10	3.478	662	665	666	rBV2	156	106	0.01%	0.001%
11	3.507	672	674	677	rBV2	151	125	0.01%	0.001%
12	3.600	693	703	705	rBV2	161	261	0.02%	0.003%
13	3.700	727	734	737	rBV	186	278	0.02%	0.003%
14	3.777	755	758	763	rVB	173	138	0.01%	0.001%
15	3.803	763	766	771	rVB2	184	160	0.01%	0.002%
16	3.838	771	777	778	rBV2	214	202	0.02%	0.002%
17	3.948	808	811	815	rBV	143	126	0.01%	0.001%
18	4.005	826	829	831	rBV	154	109	0.01%	0.001%
19	4.063	843	847	849	rBV2	182	137	0.01%	0.001%
20	4.086	849	854	858	rBV2	173	219	0.02%	0.002%
21	4.166	876	879	881	rBV	198	120	0.01%	0.001%
22	4.276	910	913	916	rBV2	214	184	0.02%	0.002%
23	4.304	920	922	927	rVB	180	184	0.02%	0.002%
24	4.327	927	929	934	rVB	143	142	0.01%	0.002%
25	4.349	934	936	941	rBV2	188	213	0.02%	0.002%
26	4.587	1005	1010	1011	rBV	193	171	0.01%	0.002%
27	4.639	1011	1026	1074	rVV	129486	397037	34.11%	4.298%
28	4.909	1108	1110	1112	rBV	198	138	0.01%	0.001%
29	5.067	1140	1159	1192	rBV	211050	463000	39.78%	5.012%
30	5.253	1213	1217	1220	rBV2	173	199	0.02%	0.002%
31	5.324	1236	1239	1246	rVB2	230	300	0.03%	0.003%
32	5.356	1246	1249	1252	rBV	253	225	0.02%	0.002%
33	5.372	1252	1254	1258	rVV	157	108	0.01%	0.001%
34	5.414	1264	1267	1273	rVB	217	203	0.02%	0.002%
35	5.449	1273	1278	1284	rBV2	179	228	0.02%	0.002%
36	5.626	1328	1333	1335	rBV2	172	182	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045123.D
 Acq On : 05 Oct 2021 02:27
 Operator : SY/MD
 Sample : M4023-20 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.729	1340	1365	1396	rBV2	427176	1163857	100.00%	12.599%
38	5.957	1433	1436	1440	rVB3	262	181	0.02%	0.002%
39	6.031	1457	1459	1462	rBV	158	111	0.01%	0.001%
40	6.050	1462	1465	1470	rVB	287	252	0.02%	0.003%
41	6.166	1498	1501	1504	rBV2	150	115	0.01%	0.001%
42	6.253	1513	1528	1551	rBV	367224	691070	59.38%	7.481%
43	6.536	1606	1616	1627	rVB9	5240	10886	0.94%	0.118%
44	6.597	1631	1635	1638	rVB3	273	217	0.02%	0.002%
45	6.616	1638	1641	1642	rBV	196	109	0.01%	0.001%
46	6.693	1650	1665	1687	rBV	280240	546517	46.96%	5.916%
47	6.806	1695	1700	1701	rBV2	549	449	0.04%	0.005%
48	6.989	1752	1757	1760	rBV2	213	231	0.02%	0.003%
49	7.009	1760	1763	1766	rBV2	140	119	0.01%	0.001%
50	7.047	1770	1775	1776	rBV	481	382	0.03%	0.004%
51	7.189	1808	1819	1830	rBV5	2588	4949	0.43%	0.054%
52	7.356	1865	1871	1874	rVB2	176	203	0.02%	0.002%
53	7.436	1893	1896	1898	rBV2	161	131	0.01%	0.001%
54	7.504	1914	1917	1919	rBV	161	131	0.01%	0.001%
55	7.568	1923	1937	1961	rBV	147655	257295	22.11%	2.785%
56	7.774	1998	2001	2003	rBV	178	119	0.01%	0.001%
57	7.793	2004	2007	2010	rVV2	370	250	0.02%	0.003%
58	7.902	2026	2041	2056	rBV	502303	863536	74.20%	9.348%
59	8.182	2116	2128	2149	rBV	103656	175024	15.04%	1.895%
60	8.401	2195	2196	2200	rVB	174	110	0.01%	0.001%
61	8.430	2200	2205	2208	rBV2	252	279	0.02%	0.003%
62	8.555	2240	2244	2250	rBV3	666	772	0.07%	0.008%
63	8.642	2258	2271	2302	rBV	488555	872464	74.96%	9.445%
64	9.002	2378	2383	2385	rBV	163	176	0.02%	0.002%
65	9.031	2389	2392	2394	rBV2	221	157	0.01%	0.002%
66	9.121	2415	2420	2422	rBV	90	105	0.01%	0.001%
67	9.308	2475	2478	2482	rBV2	179	152	0.01%	0.002%
68	9.346	2487	2490	2496	rVB2	214	213	0.02%	0.002%
69	9.372	2496	2498	2500	rBV	200	132	0.01%	0.001%
70	9.420	2500	2513	2547	rVV	517814	854485	73.42%	9.250%
71	9.574	2555	2561	2567	rVB3	522	662	0.06%	0.007%
72	9.700	2592	2600	2606	rVB4	1177	1778	0.15%	0.019%
73	9.745	2611	2614	2617	rBV	259	219	0.02%	0.002%
74	9.838	2640	2643	2645	rBV	193	107	0.01%	0.001%
75	9.854	2645	2648	2651	rBV2	183	151	0.01%	0.002%
76	9.912	2663	2666	2671	rVB	208	137	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045123.D
 Acq On : 05 Oct 2021 02:27
 Operator : SY/MD
 Sample : M4023-20 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	9.960	2678	2681	2683	rBV2	179	111	0.01%	0.001%
78	10.098	2719	2724	2726	rBV	382	247	0.02%	0.003%
79	10.214	2757	2760	2763	rBV2	149	124	0.01%	0.001%
80	10.282	2779	2781	2784	rBV2	187	136	0.01%	0.001%
81	10.336	2795	2798	2803	rBV	98	104	0.01%	0.001%
82	10.381	2808	2812	2817	rVB2	236	274	0.02%	0.003%
83	10.423	2822	2825	2827	rBV	202	129	0.01%	0.001%
84	10.516	2850	2854	2855	rBV	159	113	0.01%	0.001%
85	10.574	2869	2872	2876	rBV	214	158	0.01%	0.002%
86	10.671	2896	2902	2911	rVB4	1167	1697	0.15%	0.018%
87	10.716	2911	2916	2917	rBV	189	176	0.02%	0.002%
88	10.761	2918	2930	2950	rVB	441237	707477	60.79%	7.659%
89	10.873	2961	2965	2966	rBV	273	179	0.02%	0.002%
90	10.915	2975	2978	2979	rBV	238	138	0.01%	0.001%
91	11.050	3017	3020	3022	rBV	179	142	0.01%	0.002%
92	11.102	3033	3036	3037	rBV	235	134	0.01%	0.001%
93	11.291	3092	3095	3100	rBV	200	229	0.02%	0.002%
94	11.462	3140	3148	3160	rVB5	1467	2569	0.22%	0.028%
95	11.587	3181	3187	3189	rBV2	258	337	0.03%	0.004%
96	11.700	3216	3222	3223	rBV3	457	403	0.03%	0.004%
97	11.815	3245	3258	3277	rBV	507374	799095	68.66%	8.651%
98	11.973	3303	3307	3314	rVB4	980	1158	0.10%	0.013%
99	12.195	3361	3376	3396	rBV	509947	818594	70.33%	8.862%
100	12.478	3459	3464	3469	rBV2	205	300	0.03%	0.003%




Sum of corrected areas: 9237508

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045123.D
Acq On : 05 Oct 2021 02:27
Operator : SY/MD
Sample : M4023-20 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

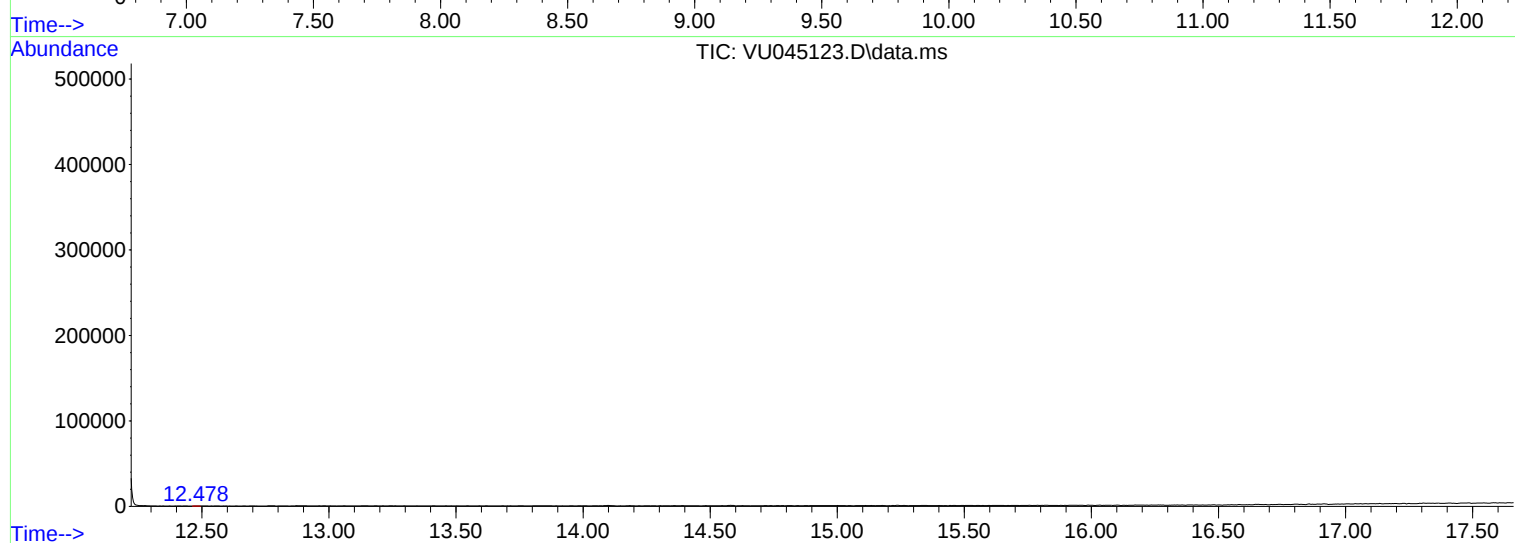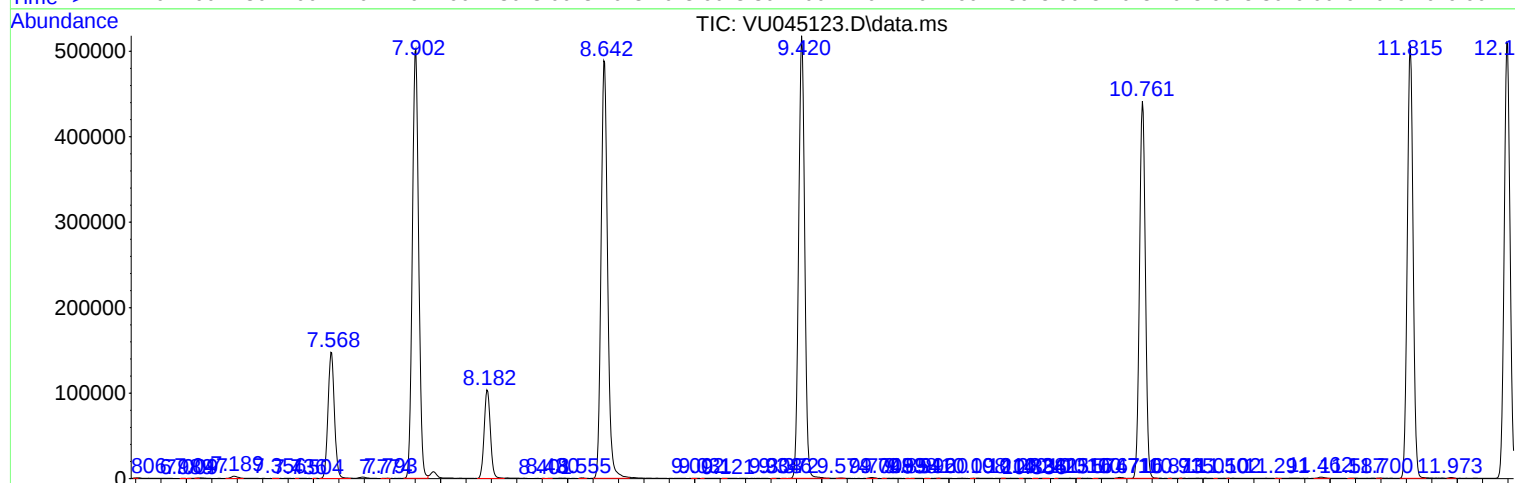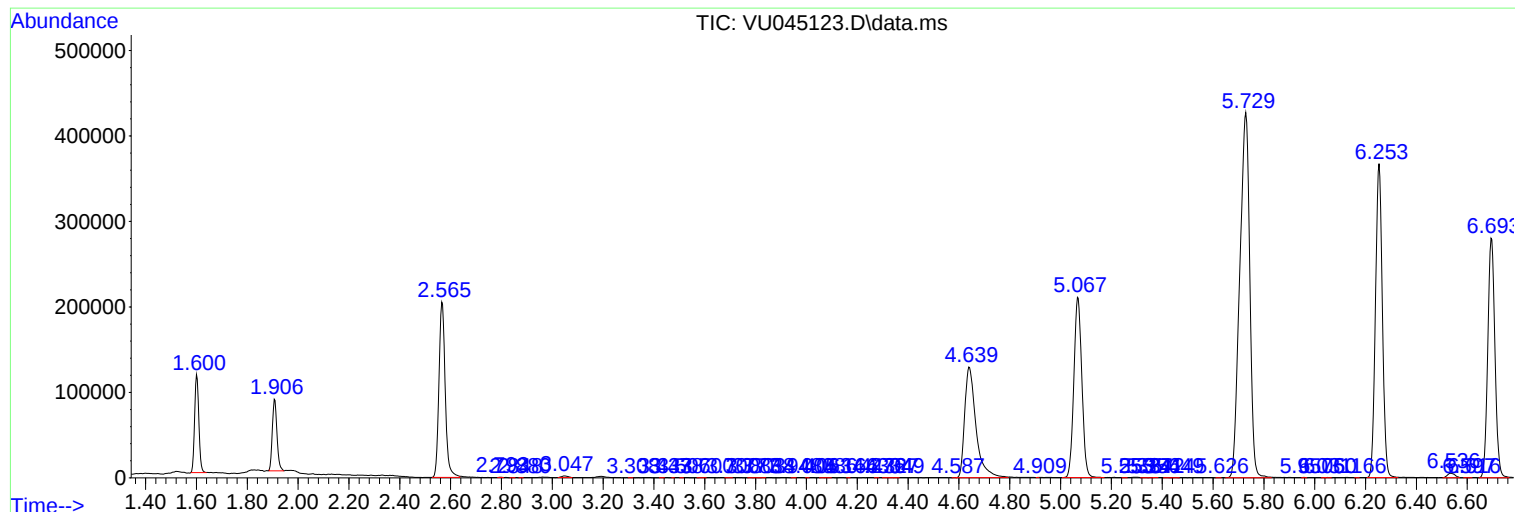

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045123.D
Acq On : 05 Oct 2021 02:27
Operator : SY/MD
Sample : M4023-20 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045123.D
Acq On : 05 Oct 2021 02:27
Operator : SY/MD
Sample : M4023-20 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
