

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045124.D
 Acq On : 05 Oct 2021 02:51
 Operator : SY/MD
 Sample : M4025-01 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	75	81	96	rVB	112210	128306	11.26%	1.401%
2	1.906	170	176	194	rVB	76845	95724	8.40%	1.045%
3	2.565	369	381	416	rBV	203049	341982	30.01%	3.734%
4	2.864	471	474	475	rBV	202	138	0.01%	0.002%
5	3.179	567	572	574	rBV2	492	386	0.03%	0.004%
6	3.260	591	597	600	rBV	198	265	0.02%	0.003%
7	3.324	613	617	620	rBV	194	184	0.02%	0.002%
8	3.375	632	633	639	rVB	162	153	0.01%	0.002%
9	3.469	658	662	663	rBV	192	96	0.01%	0.001%
10	3.591	695	700	704	rBV2	166	168	0.01%	0.002%
11	3.613	704	707	711	rBV2	186	176	0.02%	0.002%
12	3.748	747	749	751	rBV2	179	105	0.01%	0.001%
13	3.761	751	753	756	rVV	114	83	0.01%	0.001%
14	3.883	786	791	797	rBV2	199	282	0.02%	0.003%
15	3.938	805	808	811	rVV	143	136	0.01%	0.001%
16	3.973	815	819	822	rBV2	205	180	0.02%	0.002%
17	3.999	824	827	831	rVB	244	200	0.02%	0.002%
18	4.054	839	844	846	rBV2	169	177	0.02%	0.002%
19	4.070	846	849	853	rVB2	160	148	0.01%	0.002%
20	4.089	853	855	858	rBV	120	104	0.01%	0.001%
21	4.141	868	871	874	rBV	193	125	0.01%	0.001%
22	4.157	874	876	878	rBV2	144	82	0.01%	0.001%
23	4.224	893	897	900	rBV	187	213	0.02%	0.002%
24	4.394	947	950	953	rVB	224	161	0.01%	0.002%
25	4.420	953	958	962	rBV2	195	218	0.02%	0.002%
26	4.446	963	966	972	rVV2	158	199	0.02%	0.002%
27	4.513	984	987	988	rBV	121	88	0.01%	0.001%
28	4.642	1011	1027	1076	rBV	122720	392854	34.48%	4.289%
29	5.067	1143	1159	1188	rBV	205998	452820	39.74%	4.944%
30	5.224	1206	1208	1210	rVB	337	116	0.01%	0.001%
31	5.301	1222	1232	1238	rVB3	483	838	0.07%	0.009%
32	5.340	1241	1244	1246	rBV	147	125	0.01%	0.001%
33	5.430	1269	1272	1274	rBV	197	152	0.01%	0.002%
34	5.549	1306	1309	1312	rBV2	165	145	0.01%	0.002%
35	5.581	1316	1319	1322	rBV2	144	143	0.01%	0.002%
36	5.729	1343	1365	1393	rBV2	420931	1139388	100.00%	12.440%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045124.D
 Acq On : 05 Oct 2021 02:51
 Operator : SY/MD
 Sample : M4025-01 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.909	1418	1421	1425	rBV3	269	271	0.02%	0.003%
38	5.970	1435	1440	1446	rVB2	324	393	0.03%	0.004%
39	5.999	1446	1449	1452	rBV	235	161	0.01%	0.002%
40	6.076	1471	1473	1479	rVB	209	208	0.02%	0.002%
41	6.108	1479	1483	1487	rBV3	335	380	0.03%	0.004%
42	6.253	1513	1528	1558	rBV	374191	703752	61.77%	7.684%
43	6.443	1584	1587	1589	rBV	276	177	0.02%	0.002%
44	6.536	1606	1616	1631	rVB7	5305	10931	0.96%	0.119%
45	6.591	1631	1633	1635	rBV2	160	107	0.01%	0.001%
46	6.632	1642	1646	1649	rBV	185	154	0.01%	0.002%
47	6.693	1650	1665	1688	rBV	275263	538414	47.25%	5.879%
48	6.915	1732	1734	1736	rBV	156	106	0.01%	0.001%
49	7.047	1770	1775	1786	rBV3	705	1165	0.10%	0.013%
50	7.137	1795	1803	1806	rBV2	211	264	0.02%	0.003%
51	7.156	1806	1809	1811	rVV	160	138	0.01%	0.002%
52	7.189	1811	1819	1834	rVB4	2792	5522	0.48%	0.060%
53	7.246	1834	1837	1842	rVB	206	221	0.02%	0.002%
54	7.272	1842	1845	1849	rBV2	121	121	0.01%	0.001%
55	7.433	1890	1895	1900	rBV2	255	386	0.03%	0.004%
56	7.507	1914	1918	1924	rBV2	192	212	0.02%	0.002%
57	7.568	1924	1937	1958	rBV	142085	251907	22.11%	2.750%
58	7.761	1992	1997	2000	rBV	226	211	0.02%	0.002%
59	7.796	2004	2008	2011	rBV	208	188	0.02%	0.002%
60	7.902	2026	2041	2057	rBV	489698	848660	74.48%	9.266%
61	8.105	2101	2104	2107	rBV2	175	170	0.01%	0.002%
62	8.131	2109	2112	2115	rBV	202	163	0.01%	0.002%
63	8.182	2116	2128	2148	rVV	99721	170934	15.00%	1.866%
64	8.349	2175	2180	2183	rBV	251	266	0.02%	0.003%
65	8.552	2240	2243	2248	rBV3	566	497	0.04%	0.005%
66	8.645	2258	2272	2298	rBV	482623	865742	75.98%	9.453%
67	8.857	2334	2338	2339	rBV	249	196	0.02%	0.002%
68	9.156	2426	2431	2432	rBV2	152	164	0.01%	0.002%
69	9.189	2438	2441	2443	rBV2	161	97	0.01%	0.001%
70	9.285	2469	2471	2474	rBV2	153	107	0.01%	0.001%
71	9.420	2499	2513	2539	rBV	527451	861355	75.60%	9.405%
72	9.629	2575	2578	2580	rBV	213	171	0.02%	0.002%
73	9.703	2594	2601	2610	rVB2	1110	1662	0.15%	0.018%
74	9.889	2655	2659	2663	rBV	266	229	0.02%	0.003%
75	9.918	2663	2668	2670	rBV2	204	239	0.02%	0.003%
76	10.063	2709	2713	2716	rBV	223	214	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045124.D
 Acq On : 05 Oct 2021 02:51
 Operator : SY/MD
 Sample : M4025-01 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.092	2719	2722	2725	rBV2	320	257	0.02%	0.003%
78	10.143	2736	2738	2740	rBV	189	98	0.01%	0.001%
79	10.185	2749	2751	2753	rBV	163	100	0.01%	0.001%
80	10.240	2765	2768	2770	rBV	141	100	0.01%	0.001%
81	10.304	2785	2788	2789	rBV	199	113	0.01%	0.001%
82	10.336	2794	2798	2805	rBV2	282	363	0.03%	0.004%
83	10.423	2820	2825	2828	rBV	212	169	0.01%	0.002%
84	10.674	2895	2903	2913	rVB5	1303	1949	0.17%	0.021%
85	10.761	2917	2930	2948	rBV	438947	705212	61.89%	7.700%
86	10.857	2957	2960	2967	rBV2	203	218	0.02%	0.002%
87	10.899	2970	2973	2979	rVB2	401	305	0.03%	0.003%
88	11.066	3022	3025	3029	rVB2	144	89	0.01%	0.001%
89	11.143	3046	3049	3051	rBV	202	114	0.01%	0.001%
90	11.211	3062	3070	3074	rBV2	243	368	0.03%	0.004%
91	11.275	3087	3090	3093	rVB2	229	137	0.01%	0.001%
92	11.298	3093	3097	3101	rBV2	227	194	0.02%	0.002%
93	11.442	3140	3142	3144	rBV2	247	113	0.01%	0.001%
94	11.815	3245	3258	3277	rBV	524410	813316	71.38%	8.880%
95	12.041	3325	3328	3335	rBV	211	251	0.02%	0.003%
96	12.195	3364	3376	3395	rBV	496253	811778	71.25%	8.863%
97	12.426	3446	3448	3450	rBV2	171	93	0.01%	0.001%
98	12.610	3502	3505	3507	rBV	224	150	0.01%	0.002%
99	12.854	3578	3581	3583	rBV	241	162	0.01%	0.002%
100	12.950	3608	3611	3614	rBV2	337	277	0.02%	0.003%




Sum of corrected areas: 9158841

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045124.D
Acq On : 05 Oct 2021 02:51
Operator : SY/MD
Sample : M4025-01 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COAL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

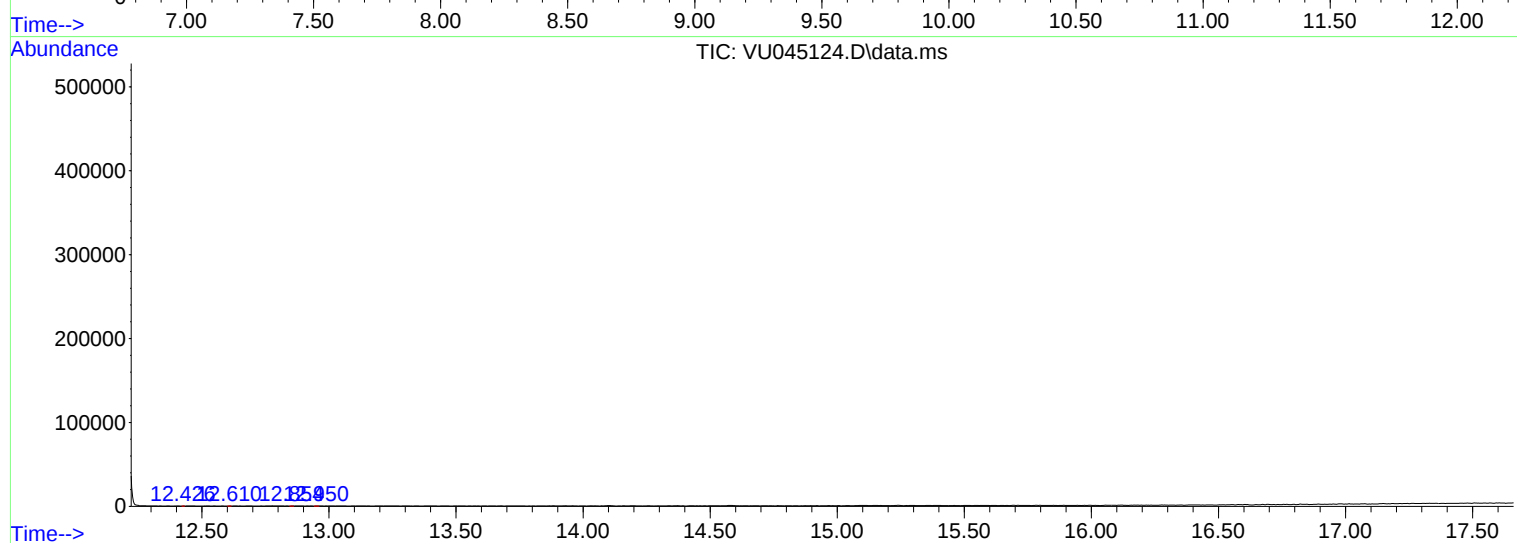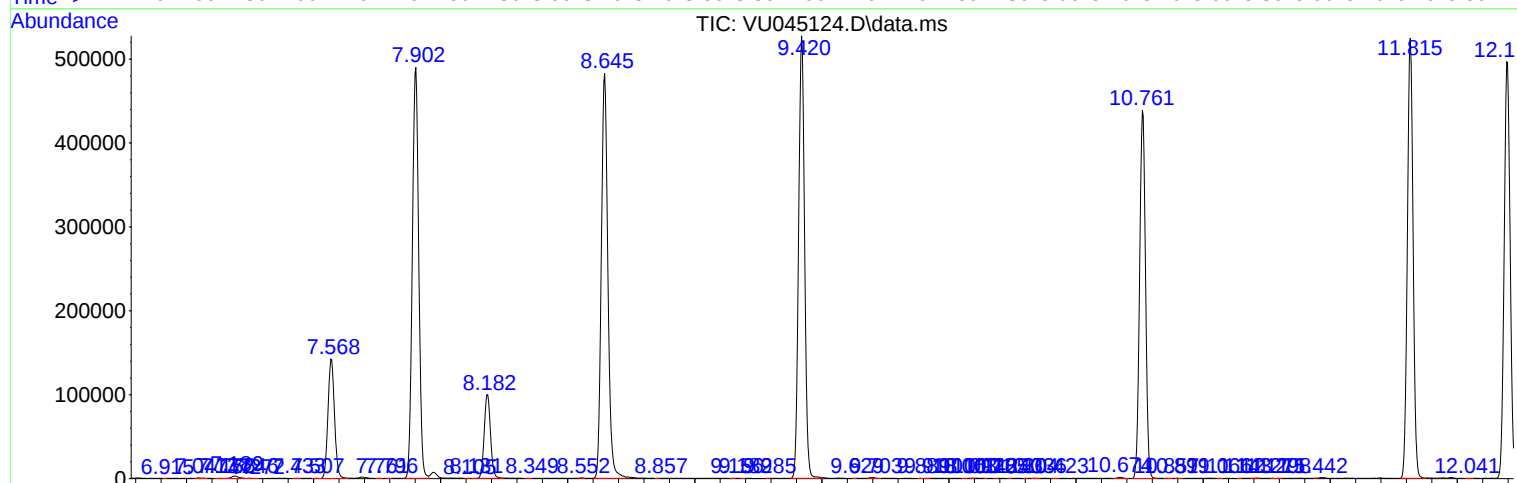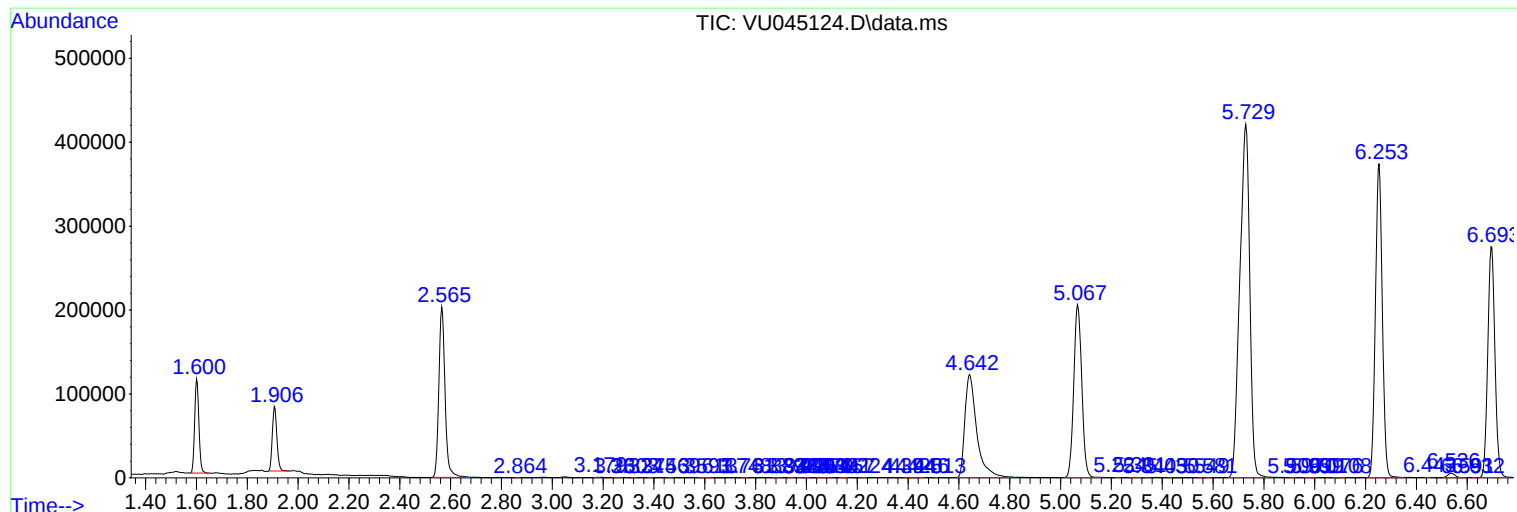

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045124.D
Acq On : 05 Oct 2021 02:51
Operator : SY/MD
Sample : M4025-01 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045124.D
Acq On : 05 Oct 2021 02:51
Operator : SY/MD
Sample : M4025-01 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
