

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045125.D
 Acq On : 05 Oct 2021 03:14
 Operator : SY/MD
 Sample : M4025-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045125.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	75	81	96	rVB	113907	129450	11.26%	1.409%
2	1.906	170	176	189	rVB	85431	107103	9.31%	1.166%
3	2.565	369	381	415	rBV	203219	348580	30.31%	3.795%
4	2.748	434	438	442	rBV2	240	234	0.02%	0.003%
5	2.935	494	496	498	rBV	154	107	0.01%	0.001%
6	2.954	499	502	506	rBV2	466	368	0.03%	0.004%
7	2.996	512	515	519	rBV	353	319	0.03%	0.003%
8	3.105	547	549	551	rBV	154	106	0.01%	0.001%
9	3.192	568	576	580	rBV2	641	853	0.07%	0.009%
10	3.288	596	606	610	rVB2	216	426	0.04%	0.005%
11	3.321	610	616	622	rBV2	221	226	0.02%	0.002%
12	3.356	624	627	630	rVB2	210	154	0.01%	0.002%
13	3.375	630	633	635	rBV	188	146	0.01%	0.002%
14	3.446	652	655	658	rBV2	190	151	0.01%	0.002%
15	3.475	661	664	665	rBV	150	89	0.01%	0.001%
16	3.507	672	674	676	rBV2	159	92	0.01%	0.001%
17	3.636	709	714	718	rBV	263	274	0.02%	0.003%
18	3.687	728	730	734	rVB	213	154	0.01%	0.002%
19	3.716	734	739	744	rBV2	253	309	0.03%	0.003%
20	3.771	754	756	761	rBV	119	131	0.01%	0.001%
21	3.796	761	764	769	rVV2	188	153	0.01%	0.002%
22	3.825	771	773	776	rVV2	157	102	0.01%	0.001%
23	3.841	776	778	781	rVV2	215	158	0.01%	0.002%
24	3.858	781	783	786	rVB	162	103	0.01%	0.001%
25	3.964	813	816	817	rBV	153	100	0.01%	0.001%
26	4.144	869	872	874	rBV	120	100	0.01%	0.001%
27	4.192	883	887	888	rBV2	160	104	0.01%	0.001%
28	4.205	888	891	892	rBV	162	102	0.01%	0.001%
29	4.243	899	903	908	rBV2	203	249	0.02%	0.003%
30	4.359	935	939	941	rBV2	160	143	0.01%	0.002%
31	4.401	950	952	955	rBV	157	111	0.01%	0.001%
32	4.446	962	966	969	rVB2	201	150	0.01%	0.002%
33	4.465	969	972	975	rBV	278	234	0.02%	0.003%
34	4.513	983	987	988	rBV2	159	130	0.01%	0.001%
35	4.639	1009	1026	1068	rVV	136602	406288	35.33%	4.423%
36	4.941	1117	1120	1127	rBV2	232	289	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045125.D
 Acq On : 05 Oct 2021 03:14
 Operator : SY/MD
 Sample : M4025-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.067	1143	1159	1180	rBV	207795	457852	39.81%	4.985%
38	5.205	1198	1202	1204	rBV2	254	178	0.02%	0.002%
39	5.221	1204	1207	1212	rVB3	267	262	0.02%	0.003%
40	5.298	1225	1231	1236	rBV4	548	876	0.08%	0.010%
41	5.356	1246	1249	1251	rBV2	163	118	0.01%	0.001%
42	5.378	1254	1256	1259	rVB2	353	180	0.02%	0.002%
43	5.398	1259	1262	1265	rBV2	174	114	0.01%	0.001%
44	5.546	1306	1308	1313	rVB2	204	176	0.02%	0.002%
45	5.575	1313	1317	1320	rBV2	293	306	0.03%	0.003%
46	5.729	1341	1365	1393	rBV2	418612	1150090	100.00%	12.521%
47	5.928	1425	1427	1429	rBV	328	226	0.02%	0.002%
48	6.160	1496	1499	1502	rBV2	181	166	0.01%	0.002%
49	6.253	1514	1528	1549	rVV	364167	687262	59.76%	7.482%
50	6.536	1607	1616	1630	rVB6	3886	7370	0.64%	0.080%
51	6.623	1637	1643	1646	rBV2	211	220	0.02%	0.002%
52	6.693	1650	1665	1693	rBV	273309	540349	46.98%	5.883%
53	6.964	1744	1749	1751	rBV	160	153	0.01%	0.002%
54	7.099	1785	1791	1795	rBV2	217	259	0.02%	0.003%
55	7.140	1801	1804	1807	rBV2	166	157	0.01%	0.002%
56	7.185	1811	1818	1831	rVB5	2712	4553	0.40%	0.050%
57	7.256	1837	1840	1842	rBV2	197	132	0.01%	0.001%
58	7.275	1842	1846	1850	rVB2	206	201	0.02%	0.002%
59	7.362	1870	1873	1877	rBV2	178	174	0.02%	0.002%
60	7.468	1902	1906	1909	rVB	213	172	0.01%	0.002%
61	7.488	1909	1912	1915	rBV	166	141	0.01%	0.002%
62	7.568	1925	1937	1956	rBV	145498	253162	22.01%	2.756%
63	7.690	1968	1975	1984	rVV2	1907	3038	0.26%	0.033%
64	7.729	1984	1987	1992	rVB2	181	170	0.01%	0.002%
65	7.809	2009	2012	2015	rBV	223	176	0.02%	0.002%
66	7.902	2022	2041	2056	rBV	496949	854824	74.33%	9.306%
67	8.118	2104	2108	2111	rBV2	212	182	0.02%	0.002%
68	8.137	2111	2114	2116	rBV	169	138	0.01%	0.002%
69	8.182	2116	2128	2147	rBV	100659	171300	14.89%	1.865%
70	8.475	2215	2219	2223	rBV2	343	387	0.03%	0.004%
71	8.539	2236	2239	2240	rBV	190	107	0.01%	0.001%
72	8.558	2241	2245	2250	rVB4	617	587	0.05%	0.006%
73	8.642	2257	2271	2308	rBV	502301	889256	77.32%	9.681%
74	8.909	2350	2354	2357	rBV2	160	181	0.02%	0.002%
75	8.938	2361	2363	2367	rBV	251	197	0.02%	0.002%
76	9.275	2465	2468	2473	rBV2	129	173	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045125.D
 Acq On : 05 Oct 2021 03:14
 Operator : SY/MD
 Sample : M4025-02 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	9.317	2478	2481	2483	rBV	215	163	0.01%	0.002%
78	9.420	2500	2513	2547	rBV	509348	847169	73.66%	9.223%
79	9.565	2555	2558	2561	rBV	432	377	0.03%	0.004%
80	9.693	2591	2598	2608	rBV3	1011	1556	0.14%	0.017%
81	9.819	2634	2637	2641	rBV2	215	189	0.02%	0.002%
82	10.002	2690	2694	2699	rVB2	226	226	0.02%	0.002%
83	10.028	2699	2702	2703	rBV2	197	134	0.01%	0.001%
84	10.169	2743	2746	2748	rBV	168	120	0.01%	0.001%
85	10.230	2762	2765	2768	rBV	204	189	0.02%	0.002%
86	10.504	2847	2850	2852	rBV	263	189	0.02%	0.002%
87	10.571	2867	2871	2872	rBV	186	126	0.01%	0.001%
88	10.616	2881	2885	2886	rBV	148	110	0.01%	0.001%
89	10.761	2918	2930	2950	rVB	443470	704689	61.27%	7.672%
90	10.938	2982	2985	2990	rVB2	228	206	0.02%	0.002%
91	10.999	3002	3004	3007	rBV	267	169	0.01%	0.002%
92	11.208	3066	3069	3072	rBV2	192	181	0.02%	0.002%
93	11.397	3124	3128	3131	rBV2	218	205	0.02%	0.002%
94	11.433	3135	3139	3141	rBV	188	166	0.01%	0.002%
95	11.815	3246	3258	3279	rBV	507491	792141	68.88%	8.624%
96	11.944	3294	3298	3301	rBV3	604	442	0.04%	0.005%
97	12.195	3363	3376	3395	rBV	509674	811880	70.59%	8.839%
98	12.671	3520	3524	3531	rVB	330	346	0.03%	0.004%
99	12.770	3552	3555	3559	rBV2	344	353	0.03%	0.004%
100	14.262	4013	4019	4024	rBV2	453	651	0.06%	0.007%




Sum of corrected areas: 9185330

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045125.D
Acq On : 05 Oct 2021 03:14
Operator : SY/MD
Sample : M4025-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

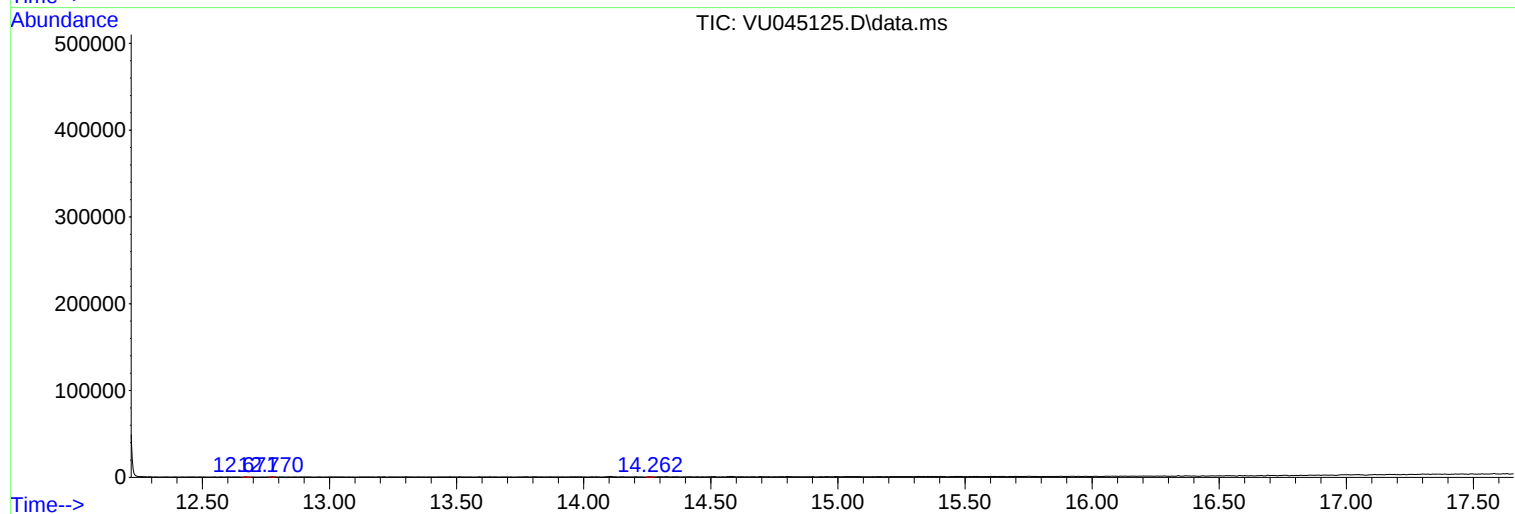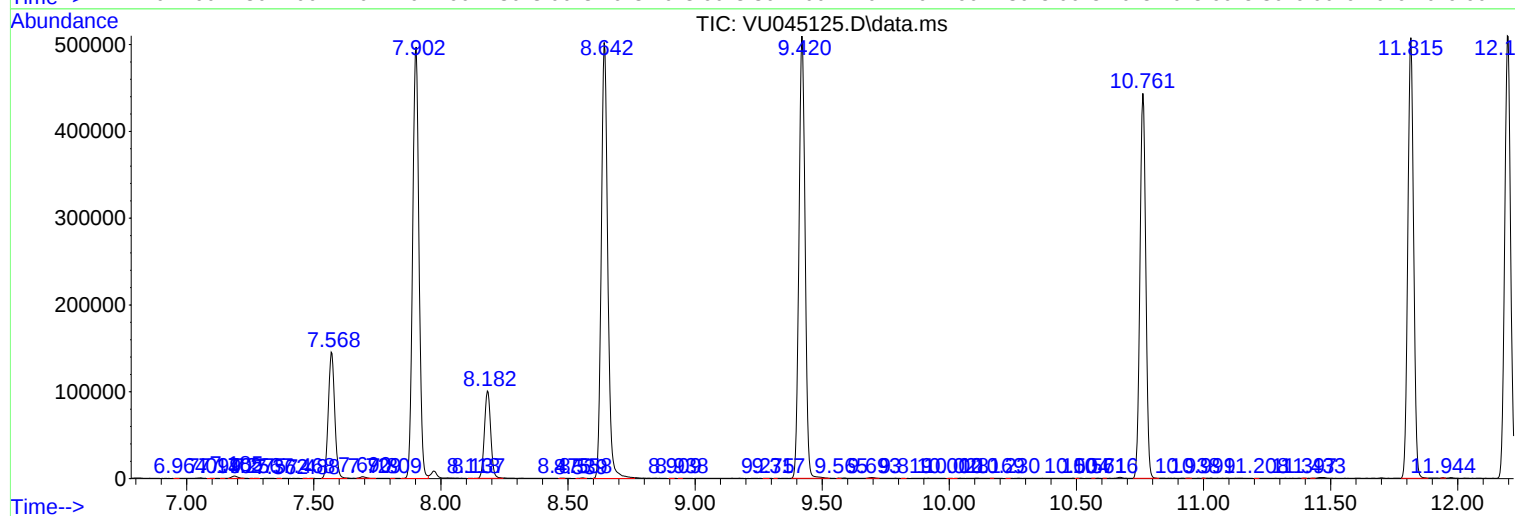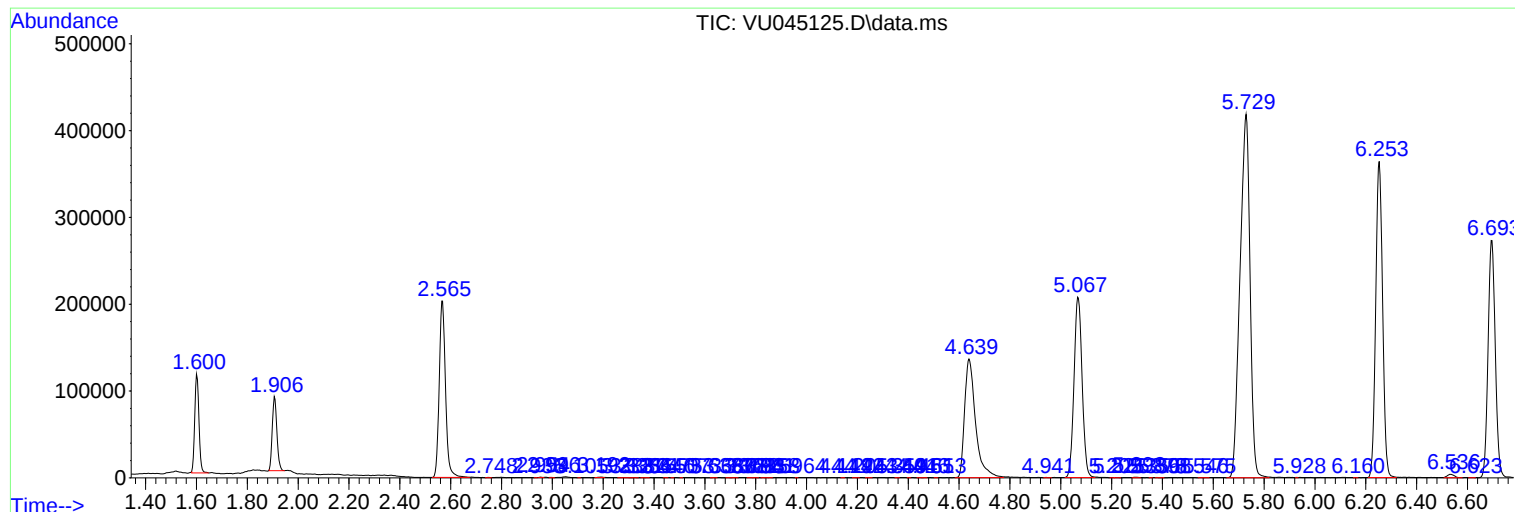

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045125.D
Acq On : 05 Oct 2021 03:14
Operator : SY/MD
Sample : M4025-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045125.D
Acq On : 05 Oct 2021 03:14
Operator : SY/MD
Sample : M4025-02 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------