

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045127.D
 Acq On : 05 Oct 2021 04:01
 Operator : SY/MD
 Sample : M4025-04 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rVB	185074	214671	14.71%	1.997%
2	1.909	169	177	192	rVB	133110	166981	11.44%	1.553%
3	2.565	369	381	413	rBV	302317	510384	34.97%	4.748%
4	2.691	418	420	426	rVB3	371	269	0.02%	0.003%
5	2.790	448	451	454	rVV2	472	413	0.03%	0.004%
6	2.819	458	460	465	rVB2	271	222	0.02%	0.002%
7	3.051	526	532	540	rBV3	784	1207	0.08%	0.011%
8	3.128	553	556	561	rBV	227	194	0.01%	0.002%
9	3.173	566	570	571	rBV	322	236	0.02%	0.002%
10	3.186	571	574	575	rBV2	374	243	0.02%	0.002%
11	3.520	673	678	683	rBV2	237	349	0.02%	0.003%
12	3.620	706	709	716	rBV2	181	256	0.02%	0.002%
13	3.674	723	726	729	rBV	199	190	0.01%	0.002%
14	3.983	819	822	827	rVB2	246	251	0.02%	0.002%
15	4.012	827	831	833	rBV2	220	187	0.01%	0.002%
16	4.379	943	945	953	rVB	238	291	0.02%	0.003%
17	4.642	1009	1027	1075	rBV	130415	420549	28.81%	3.912%
18	5.067	1141	1159	1191	rBV	252367	554363	37.98%	5.157%
19	5.202	1199	1201	1204	rVB2	409	215	0.01%	0.002%
20	5.237	1209	1212	1217	rVV2	272	209	0.01%	0.002%
21	5.292	1223	1229	1237	rBV2	505	771	0.05%	0.007%
22	5.372	1250	1254	1255	rBV2	402	237	0.02%	0.002%
23	5.488	1288	1290	1297	rVB	180	171	0.01%	0.002%
24	5.729	1343	1365	1397	rBV2	546483	1459677	100.00%	13.579%
25	5.896	1415	1417	1425	rVB4	277	236	0.02%	0.002%
26	6.253	1512	1528	1549	rBV	366194	686328	47.02%	6.385%
27	6.436	1582	1585	1587	rBV	254	204	0.01%	0.002%
28	6.449	1587	1589	1591	rVV	261	171	0.01%	0.002%
29	6.468	1592	1595	1597	rVV	297	214	0.01%	0.002%
30	6.533	1605	1615	1625	rVB5	3576	7041	0.48%	0.065%
31	6.694	1651	1665	1693	rVV	336522	658480	45.11%	6.126%
32	6.793	1694	1696	1698	rVV2	553	327	0.02%	0.003%
33	6.813	1698	1702	1710	rVB2	889	1107	0.08%	0.010%
34	6.845	1710	1712	1715	rBV2	348	186	0.01%	0.002%
35	6.951	1740	1745	1747	rBV2	180	213	0.01%	0.002%
36	7.050	1770	1776	1780	rBV3	699	747	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045127.D
 Acq On : 05 Oct 2021 04:01
 Operator : SY/MD
 Sample : M4025-04 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.144	1802	1805	1809	rVB	248	221	0.02%	0.002%
38	7.189	1812	1819	1832	rVV6	2049	3819	0.26%	0.036%
39	7.407	1883	1887	1890	rVB2	240	189	0.01%	0.002%
40	7.440	1894	1897	1904	rVB2	252	339	0.02%	0.003%
41	7.472	1904	1907	1911	rBV	178	169	0.01%	0.002%
42	7.568	1924	1937	1964	rBV2	181294	317824	21.77%	2.957%
43	7.697	1969	1977	1986	rVB2	1363	2206	0.15%	0.021%
44	7.903	2023	2041	2055	rBV	660339	1137164	77.91%	10.579%
45	7.970	2057	2062	2080	rVB	9614	16715	1.15%	0.155%
46	8.121	2105	2109	2115	rBV2	210	284	0.02%	0.003%
47	8.182	2115	2128	2148	rBV	126499	215791	14.78%	2.007%
48	8.314	2164	2169	2172	rBV2	175	182	0.01%	0.002%
49	8.501	2223	2227	2229	rBV	254	228	0.02%	0.002%
50	8.555	2240	2244	2248	rVB3	612	506	0.03%	0.005%
51	8.591	2248	2255	2258	rBV2	172	213	0.01%	0.002%
52	8.645	2258	2272	2303	rBV	495012	886920	60.76%	8.251%
53	8.841	2328	2333	2338	rBV3	226	305	0.02%	0.003%
54	9.054	2395	2399	2402	rBV2	198	237	0.02%	0.002%
55	9.420	2499	2513	2548	rBV	513566	847364	58.05%	7.883%
56	9.571	2554	2560	2565	rBV2	391	446	0.03%	0.004%
57	9.697	2592	2599	2608	rVB4	1294	1997	0.14%	0.019%
58	9.880	2651	2656	2660	rVB2	195	239	0.02%	0.002%
59	9.957	2677	2680	2682	rBV	225	181	0.01%	0.002%
60	10.063	2710	2713	2721	rVB2	269	384	0.03%	0.004%
61	10.105	2721	2726	2732	rBV3	514	783	0.05%	0.007%
62	10.224	2760	2763	2769	rVB2	230	232	0.02%	0.002%
63	10.340	2797	2799	2805	rVB2	168	182	0.01%	0.002%
64	10.539	2857	2861	2863	rBV	243	225	0.02%	0.002%
65	10.671	2895	2902	2911	rBV2	3353	4524	0.31%	0.042%
66	10.761	2917	2930	2949	rBV	494633	787708	53.96%	7.328%
67	10.867	2957	2963	2964	rBV	752	620	0.04%	0.006%
68	10.928	2979	2982	2988	rVB2	466	388	0.03%	0.004%
69	11.095	3031	3034	3037	rBV2	389	267	0.02%	0.002%
70	11.127	3037	3044	3050	rVV5	758	1123	0.08%	0.010%
71	11.156	3051	3053	3056	rVV2	357	201	0.01%	0.002%
72	11.208	3065	3069	3073	rVB3	219	183	0.01%	0.002%
73	11.314	3099	3102	3106	rBV	171	189	0.01%	0.002%
74	11.353	3110	3114	3118	rBV	249	216	0.01%	0.002%
75	11.381	3118	3123	3128	rBV3	253	348	0.02%	0.003%
76	11.462	3139	3148	3158	rBV5	2831	4706	0.32%	0.044%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045127.D
 Acq On : 05 Oct 2021 04:01
 Operator : SY/MD
 Sample : M4025-04 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

77	11.581	3179	3185	3190	rVB2	725	712	0.05%	0.007%
78	11.616	3190	3196	3202	rBV2	315	456	0.03%	0.004%
79	11.703	3214	3223	3229	rBV3	1684	2512	0.17%	0.023%
80	11.816	3244	3258	3273	rBV	511476	800776	54.86%	7.449%
81	11.922	3288	3291	3293	rBV	333	270	0.02%	0.003%
82	11.944	3293	3298	3302	rVV3	1354	1837	0.13%	0.017%
83	11.976	3304	3308	3316	rVB2	2559	3175	0.22%	0.030%
84	12.028	3320	3324	3329	rBV2	409	332	0.02%	0.003%
85	12.195	3359	3376	3398	rBV	628455	1010577	69.23%	9.401%
86	12.275	3398	3401	3406	rVV3	496	488	0.03%	0.005%
87	12.336	3414	3420	3425	rVB4	823	881	0.06%	0.008%
88	12.594	3496	3500	3502	rBV	291	203	0.01%	0.002%
89	12.642	3509	3515	3518	rBV3	646	653	0.04%	0.006%
90	12.767	3548	3554	3556	rBV3	294	314	0.02%	0.003%
91	12.864	3580	3584	3587	rBV	210	176	0.01%	0.002%
92	12.922	3598	3602	3606	rBV	303	349	0.02%	0.003%
93	12.976	3614	3619	3623	rBV2	281	355	0.02%	0.003%
94	13.677	3832	3837	3840	rBV2	320	351	0.02%	0.003%
95	14.250	4012	4015	4018	rBV2	281	199	0.01%	0.002%
96	14.449	4075	4077	4081	rBV	218	173	0.01%	0.002%
97	14.577	4114	4117	4121	rBV2	308	220	0.02%	0.002%
98	14.938	4226	4229	4232	rBV2	285	240	0.02%	0.002%
99	15.487	4397	4400	4404	rBV2	421	403	0.03%	0.004%
100	16.638	4756	4758	4762	rBV3	544	394	0.03%	0.004%




Sum of corrected areas: 10749654

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045127.D
Acq On : 05 Oct 2021 04:01
Operator : SY/MD
Sample : M4025-04 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

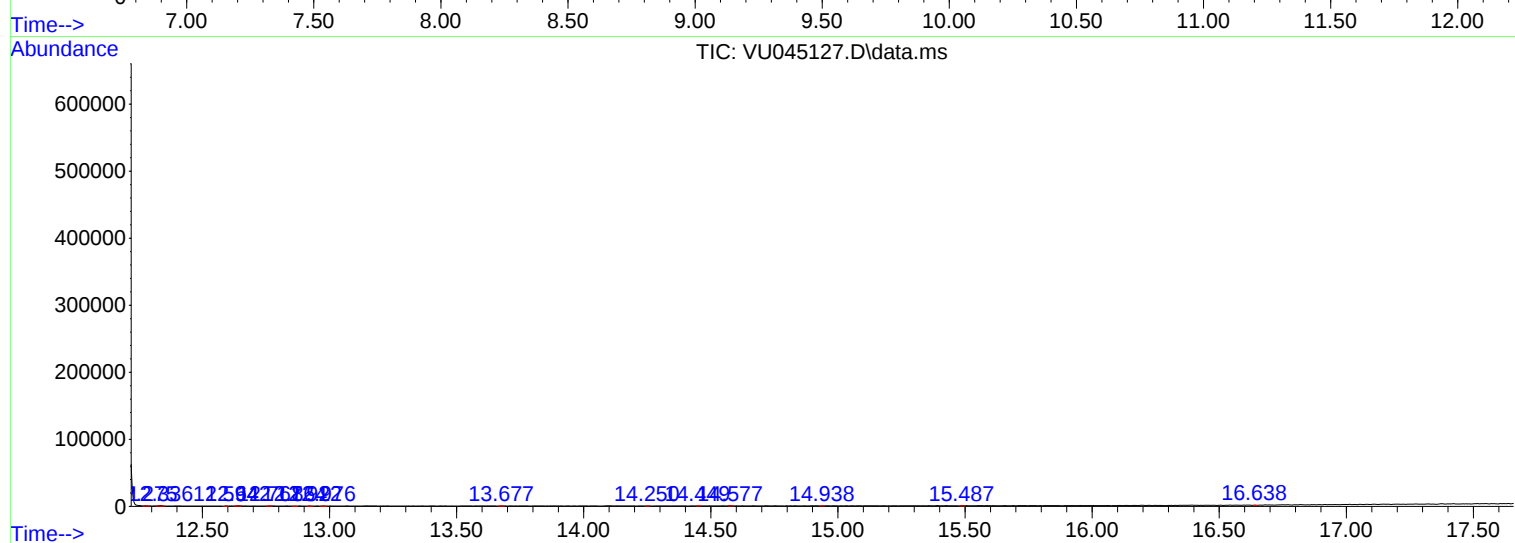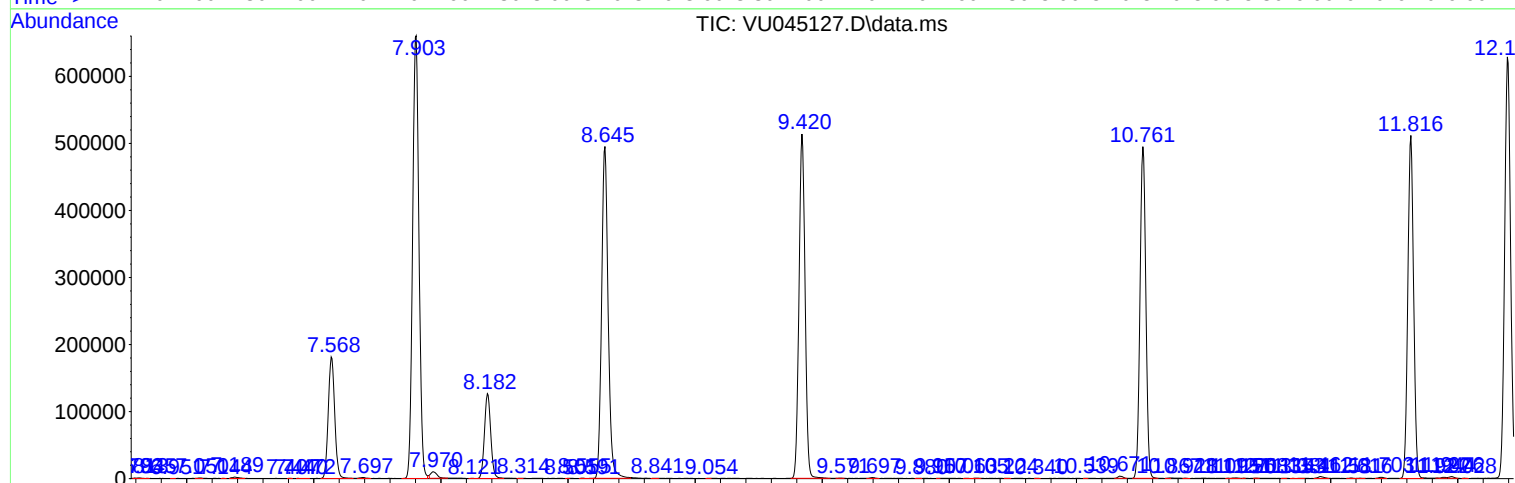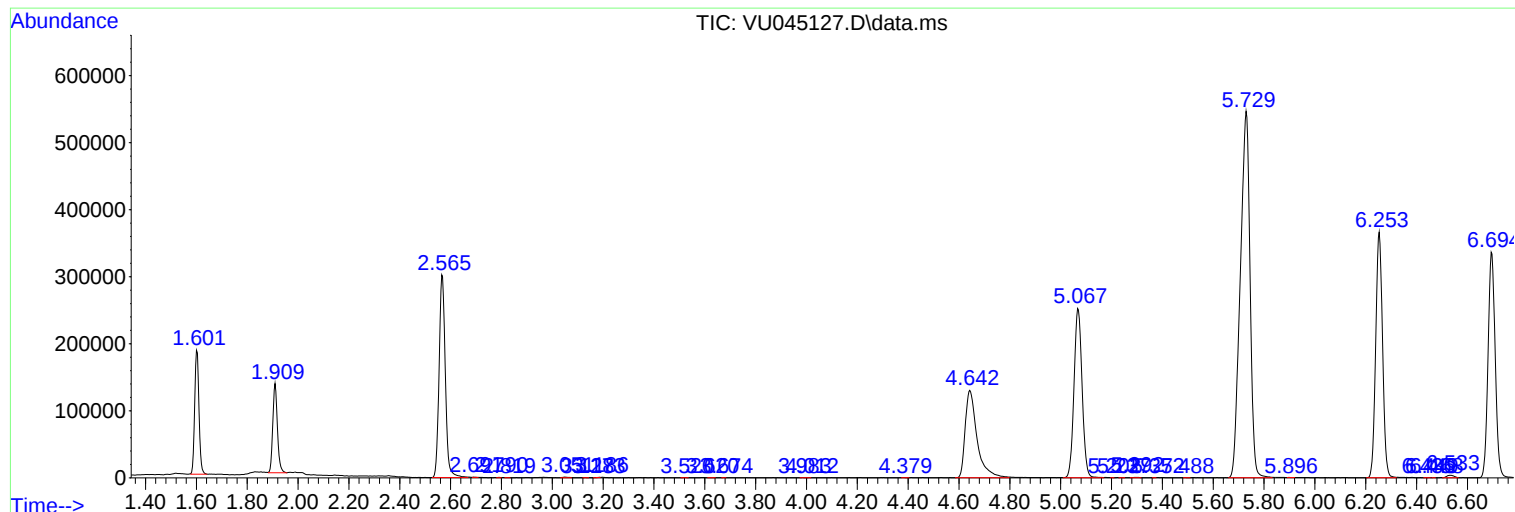

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045127.D
Acq On : 05 Oct 2021 04:01
Operator : SY/MD
Sample : M4025-04 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045127.D
Acq On : 05 Oct 2021 04:01
Operator : SY/MD
Sample : M4025-04 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------