

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045129.D
 Acq On : 05 Oct 2021 04:47
 Operator : SY/MD
 Sample : M4025-06 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045129.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	97	rVB	178068	205707	14.39%	1.948%
2	1.909	169	177	195	rVB	150846	195109	13.65%	1.847%
3	2.568	369	382	412	rBV	296864	499966	34.98%	4.734%
4	2.806	449	456	460	rBV3	235	308	0.02%	0.003%
5	2.961	497	504	507	rBV2	336	451	0.03%	0.004%
6	3.051	524	532	540	rVB5	790	1446	0.10%	0.014%
7	3.173	566	570	571	rBV	259	167	0.01%	0.002%
8	3.195	571	577	583	rVB3	520	721	0.05%	0.007%
9	3.382	632	635	638	rVB	229	162	0.01%	0.002%
10	3.414	638	645	648	rBV2	202	288	0.02%	0.003%
11	3.446	651	655	658	rBV2	235	186	0.01%	0.002%
12	3.504	668	673	678	rBV2	236	236	0.02%	0.002%
13	3.636	710	714	716	rBV	197	159	0.01%	0.002%
14	3.729	740	743	746	rBV	222	175	0.01%	0.002%
15	3.864	782	785	788	rBV2	214	169	0.01%	0.002%
16	3.941	802	809	811	rBV2	151	212	0.01%	0.002%
17	4.124	860	866	870	rVB2	156	179	0.01%	0.002%
18	4.205	887	891	894	rBV2	232	199	0.01%	0.002%
19	4.276	911	913	918	rBV2	140	159	0.01%	0.002%
20	4.340	930	933	936	rVB	221	167	0.01%	0.002%
21	4.362	936	940	942	rBV2	233	230	0.02%	0.002%
22	4.536	991	994	999	rBV	155	162	0.01%	0.002%
23	4.639	1007	1026	1069	rBV	140472	420746	29.44%	3.984%
24	5.067	1143	1159	1179	rBV	247101	543380	38.02%	5.145%
25	5.295	1223	1230	1237	rVB4	568	1020	0.07%	0.010%
26	5.337	1237	1243	1244	rBV	206	165	0.01%	0.002%
27	5.417	1261	1268	1271	rBV2	222	287	0.02%	0.003%
28	5.729	1341	1365	1390	rBV2	530059	1429288	100.00%	13.533%
29	6.079	1472	1474	1478	rVB2	323	230	0.02%	0.002%
30	6.112	1480	1484	1486	rBV	362	258	0.02%	0.002%
31	6.124	1486	1488	1492	rVB2	246	158	0.01%	0.001%
32	6.150	1494	1496	1501	rVB	307	189	0.01%	0.002%
33	6.253	1509	1528	1553	rBV	362005	681186	47.66%	6.450%
34	6.423	1577	1581	1584	rBV2	205	187	0.01%	0.002%
35	6.536	1606	1616	1624	rVV5	3764	6323	0.44%	0.060%
36	6.578	1624	1629	1632	rVB2	296	261	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045129.D
 Acq On : 05 Oct 2021 04:47
 Operator : SY/MD
 Sample : M4025-06 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.693	1651	1665	1695	rBV	331191	646603	45.24%	6.122%
38	6.803	1695	1699	1701	rBV3	523	439	0.03%	0.004%
39	6.996	1756	1759	1764	rVV2	162	179	0.01%	0.002%
40	7.054	1767	1777	1787	rVB3	689	1427	0.10%	0.014%
41	7.105	1787	1793	1798	rVB2	220	328	0.02%	0.003%
42	7.147	1798	1806	1809	rBV2	250	270	0.02%	0.003%
43	7.189	1809	1819	1831	rBV5	2032	3492	0.24%	0.033%
44	7.324	1858	1861	1865	rBV	208	208	0.01%	0.002%
45	7.394	1880	1883	1887	rBV	228	184	0.01%	0.002%
46	7.520	1916	1922	1924	rBV	296	329	0.02%	0.003%
47	7.568	1924	1937	1961	rVV	174118	309470	21.65%	2.930%
48	7.693	1969	1976	1986	rVB5	1353	2069	0.14%	0.020%
49	7.758	1993	1996	2000	rVB2	206	174	0.01%	0.002%
50	7.803	2006	2010	2015	rVB2	198	208	0.01%	0.002%
51	7.902	2027	2041	2056	rBV	657720	1120092	78.37%	10.605%
52	7.970	2056	2062	2081	rVB	9987	18487	1.29%	0.175%
53	8.182	2115	2128	2147	rBV	123420	210295	14.71%	1.991%
54	8.420	2197	2202	2204	rBV2	173	155	0.01%	0.001%
55	8.552	2240	2243	2248	rVB3	531	453	0.03%	0.004%
56	8.578	2248	2251	2253	rBV2	186	157	0.01%	0.001%
57	8.642	2258	2271	2299	rBV	497167	875816	61.28%	8.292%
58	9.012	2380	2386	2388	rBV2	226	293	0.02%	0.003%
59	9.099	2410	2413	2417	rBV2	184	173	0.01%	0.002%
60	9.127	2417	2422	2425	rBV2	196	191	0.01%	0.002%
61	9.189	2437	2441	2444	rBV2	208	197	0.01%	0.002%
62	9.346	2485	2490	2497	rVB2	242	322	0.02%	0.003%
63	9.420	2497	2513	2542	rBV	517954	841041	58.84%	7.963%
64	9.578	2555	2562	2565	rBV2	355	504	0.04%	0.005%
65	9.655	2581	2586	2592	rBV	254	333	0.02%	0.003%
66	9.693	2592	2598	2607	rVV3	1055	1789	0.13%	0.017%
67	10.105	2721	2726	2728	rBV3	423	328	0.02%	0.003%
68	10.295	2782	2785	2789	rVB2	301	239	0.02%	0.002%
69	10.346	2796	2801	2806	rBV2	226	330	0.02%	0.003%
70	10.674	2895	2903	2911	rBV2	2998	4083	0.29%	0.039%
71	10.761	2916	2930	2952	rVB	471528	759443	53.13%	7.191%
72	10.867	2958	2963	2965	rBV2	831	866	0.06%	0.008%
73	10.979	2994	2998	3001	rBV2	231	214	0.01%	0.002%
74	11.005	3001	3006	3008	rBV3	225	247	0.02%	0.002%
75	11.098	3030	3035	3037	rBV2	219	185	0.01%	0.002%
76	11.115	3037	3040	3048	rVV3	498	781	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045129.D
 Acq On : 05 Oct 2021 04:47
 Operator : SY/MD
 Sample : M4025-06 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.459	3139	3147	3157	rBV5	2945	5286	0.37%	0.050%
78	11.558	3174	3178	3181	rBV2	191	214	0.01%	0.002%
79	11.584	3181	3186	3192	rVB3	621	801	0.06%	0.008%
80	11.639	3198	3203	3206	rBV2	223	263	0.02%	0.002%
81	11.700	3212	3222	3229	rBV3	1461	2379	0.17%	0.023%
82	11.815	3244	3258	3275	rBV	502445	779504	54.54%	7.381%
83	11.976	3302	3308	3316	rVB4	2393	3504	0.25%	0.033%
84	12.195	3361	3376	3396	rBV	604750	970814	67.92%	9.192%
85	12.336	3413	3420	3424	rBV2	867	857	0.06%	0.008%
86	12.410	3439	3443	3445	rBV3	505	389	0.03%	0.004%
87	12.558	3485	3489	3494	rBV	243	255	0.02%	0.002%
88	12.642	3511	3515	3521	rVB3	492	454	0.03%	0.004%
89	12.719	3534	3539	3544	rBV2	278	336	0.02%	0.003%
90	13.491	3776	3779	3783	rBV2	247	211	0.01%	0.002%
91	13.819	3878	3881	3885	rBV	272	278	0.02%	0.003%
92	14.066	3952	3958	3961	rBV2	252	341	0.02%	0.003%
93	14.092	3961	3966	3968	rBV3	325	343	0.02%	0.003%
94	14.259	4016	4018	4022	rBV2	319	236	0.02%	0.002%
95	14.385	4050	4057	4061	rBV2	375	565	0.04%	0.005%
96	14.478	4081	4086	4091	rBV2	446	512	0.04%	0.005%
97	14.626	4129	4132	4135	rBV	254	196	0.01%	0.002%
98	14.918	4220	4223	4226	rBV2	279	227	0.02%	0.002%
99	16.063	4577	4579	4583	rBV2	316	208	0.01%	0.002%
100	16.510	4714	4718	4724	rBV4	849	801	0.06%	0.008%




Sum of corrected areas: 10561604

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045129.D
Acq On : 05 Oct 2021 04:47
Operator : SY/MD
Sample : M4025-06 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

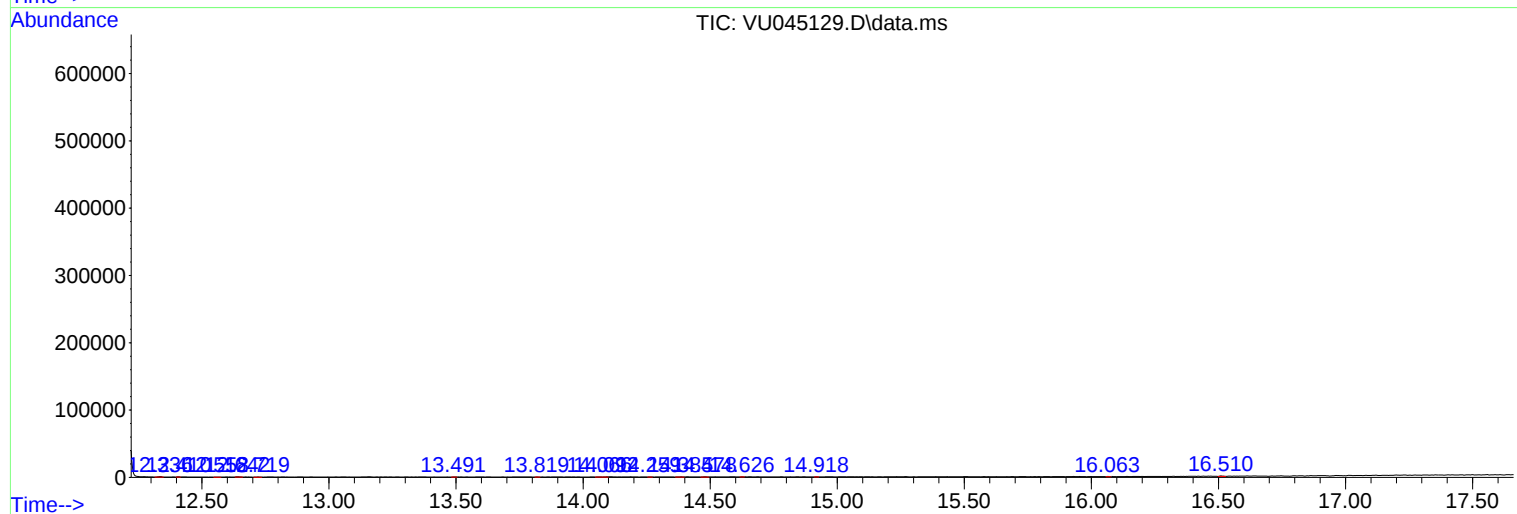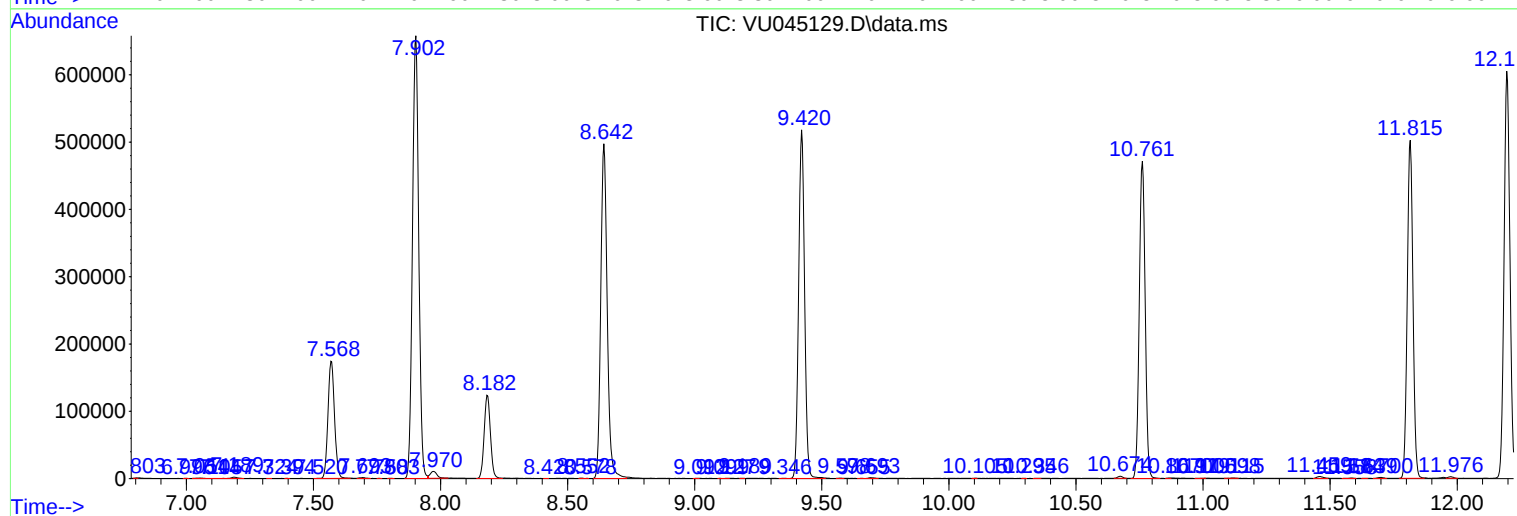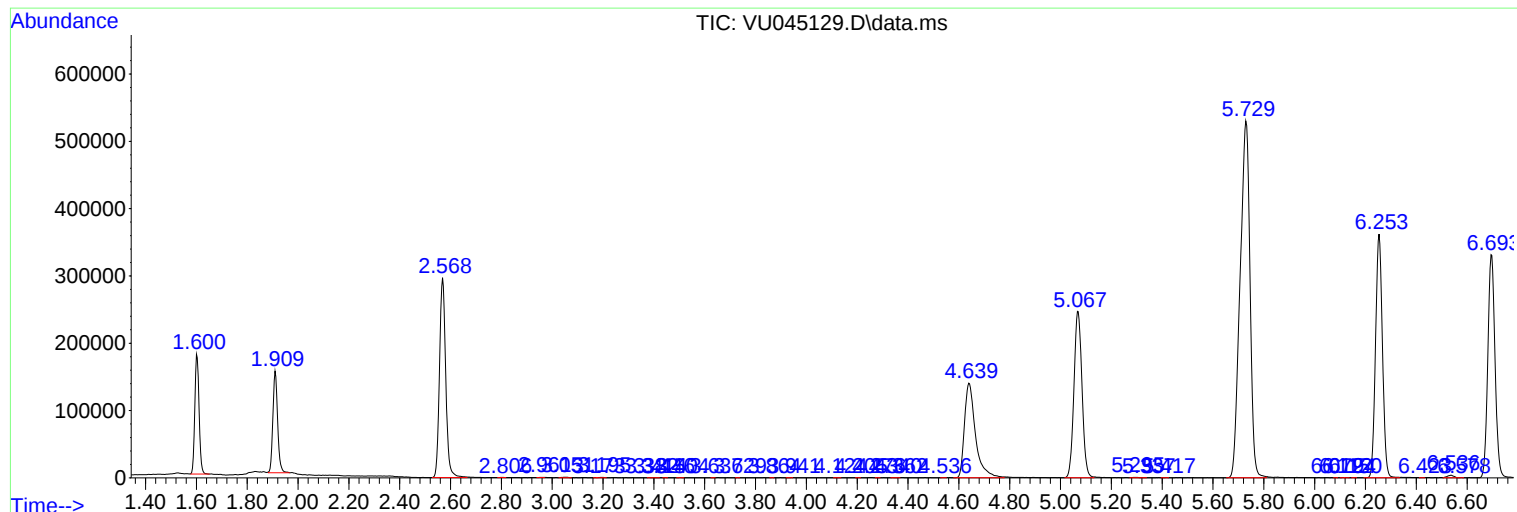

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045129.D
Acq On : 05 Oct 2021 04:47
Operator : SY/MD
Sample : M4025-06 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045129.D
Acq On : 05 Oct 2021 04:47
Operator : SY/MD
Sample : M4025-06 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
