

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045130.D
 Acq On : 05 Oct 2021 05:10
 Operator : SY/MD
 Sample : M4025-07 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045130.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	93	rVB	183081	208938	14.56%	1.965%
2	1.909	169	177	191	rVB	146601	190428	13.27%	1.791%
3	2.569	369	382	409	rBV	296084	496418	34.60%	4.668%
4	2.787	447	450	453	rBV	254	232	0.02%	0.002%
5	2.964	502	505	509	rVV2	464	484	0.03%	0.005%
6	2.996	513	515	518	rVB	312	174	0.01%	0.002%
7	3.041	525	529	530	rBV	583	424	0.03%	0.004%
8	3.054	530	533	538	rVB4	872	889	0.06%	0.008%
9	3.192	573	576	578	rBV3	278	185	0.01%	0.002%
10	3.417	641	646	650	rBV2	263	304	0.02%	0.003%
11	3.794	759	763	767	rBV2	212	214	0.01%	0.002%
12	3.819	767	771	774	rBV2	425	425	0.03%	0.004%
13	4.035	834	838	841	rBV2	177	172	0.01%	0.002%
14	4.179	879	883	885	rBV	226	221	0.02%	0.002%
15	4.562	997	1002	1005	rBV2	144	174	0.01%	0.002%
16	4.642	1011	1027	1088	rVV	128670	421443	29.38%	3.963%
17	4.993	1134	1136	1143	rVB2	245	255	0.02%	0.002%
18	5.067	1143	1159	1186	rBV	247128	546153	38.07%	5.136%
19	5.221	1201	1207	1210	rBV3	318	307	0.02%	0.003%
20	5.298	1225	1231	1238	rBV3	462	718	0.05%	0.007%
21	5.379	1253	1256	1260	rBV2	197	181	0.01%	0.002%
22	5.729	1343	1365	1404	rVV2	534640	1434688	100.00%	13.492%
23	6.121	1482	1487	1493	rBV2	381	329	0.02%	0.003%
24	6.253	1513	1528	1548	rBV	373388	698088	48.66%	6.565%
25	6.485	1596	1600	1603	rBV	213	182	0.01%	0.002%
26	6.533	1605	1615	1624	rVV6	3842	6822	0.48%	0.064%
27	6.620	1639	1642	1647	rVB2	184	167	0.01%	0.002%
28	6.694	1651	1665	1690	rBV	333196	651329	45.40%	6.125%
29	6.806	1696	1700	1705	rBV4	597	719	0.05%	0.007%
30	6.858	1713	1716	1718	rVB2	335	167	0.01%	0.002%
31	6.883	1719	1724	1727	rBV2	206	237	0.02%	0.002%
32	6.957	1742	1747	1750	rBV	165	162	0.01%	0.002%
33	6.996	1754	1759	1764	rVB2	169	221	0.02%	0.002%
34	7.054	1769	1777	1778	rBV3	484	599	0.04%	0.006%
35	7.128	1796	1800	1802	rBV2	179	172	0.01%	0.002%
36	7.192	1811	1820	1832	rBV5	1667	3058	0.21%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045130.D
 Acq On : 05 Oct 2021 05:10
 Operator : SY/MD
 Sample : M4025-07 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.334	1861	1864	1869	rVB	172	190	0.01%	0.002%
38	7.504	1913	1917	1924	rBV2	174	282	0.02%	0.003%
39	7.568	1924	1937	1962	rBV	174524	310383	21.63%	2.919%
40	7.694	1971	1976	1984	rVB3	1041	1762	0.12%	0.017%
41	7.797	2001	2008	2011	rBV	182	232	0.02%	0.002%
42	7.903	2027	2041	2056	rBV	646850	1122704	78.25%	10.558%
43	8.131	2108	2112	2115	rBV	157	152	0.01%	0.001%
44	8.182	2115	2128	2154	rVV	122356	210530	14.67%	1.980%
45	8.301	2163	2165	2170	rVB2	392	273	0.02%	0.003%
46	8.375	2184	2188	2192	rBV	175	188	0.01%	0.002%
47	8.539	2234	2239	2241	rBV	219	215	0.01%	0.002%
48	8.555	2241	2244	2249	rVV2	447	403	0.03%	0.004%
49	8.642	2258	2271	2309	rBV	492431	877467	61.16%	8.252%
50	9.035	2390	2393	2398	rVB2	186	157	0.01%	0.001%
51	9.063	2398	2402	2404	rBV	167	164	0.01%	0.002%
52	9.356	2489	2493	2496	rBV	208	176	0.01%	0.002%
53	9.420	2500	2513	2534	rBV	520613	856649	59.71%	8.056%
54	9.575	2555	2561	2566	rVB	397	498	0.03%	0.005%
55	9.697	2592	2599	2606	rVB	1175	1583	0.11%	0.015%
56	9.874	2651	2654	2656	rBV	198	168	0.01%	0.002%
57	9.957	2678	2680	2686	rBV2	195	239	0.02%	0.002%
58	10.108	2721	2727	2731	rVB3	420	422	0.03%	0.004%
59	10.221	2759	2762	2766	rVB2	205	169	0.01%	0.002%
60	10.263	2768	2775	2782	rVB2	257	404	0.03%	0.004%
61	10.343	2796	2800	2805	rBV2	193	150	0.01%	0.001%
62	10.379	2805	2811	2812	rBV	174	203	0.01%	0.002%
63	10.449	2829	2833	2836	rBV2	155	171	0.01%	0.002%
64	10.674	2894	2903	2914	rVB3	3192	4992	0.35%	0.047%
65	10.761	2914	2930	2952	rBV	473310	768806	53.59%	7.230%
66	10.874	2958	2965	2972	rBV5	626	1088	0.08%	0.010%
67	10.970	2992	2995	2999	rBV2	157	148	0.01%	0.001%
68	10.999	3000	3004	3007	rBV3	285	269	0.02%	0.003%
69	11.115	3037	3040	3041	rBV	420	249	0.02%	0.002%
70	11.382	3120	3123	3127	rVB	384	254	0.02%	0.002%
71	11.407	3127	3131	3136	rBV2	240	306	0.02%	0.003%
72	11.462	3139	3148	3158	rVB3	2857	4930	0.34%	0.046%
73	11.581	3180	3185	3187	rBV2	562	479	0.03%	0.005%
74	11.697	3215	3221	3229	rVB3	1397	2006	0.14%	0.019%
75	11.816	3245	3258	3277	rBV	516287	802629	55.94%	7.548%
76	11.912	3285	3288	3291	rBV4	568	420	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045130.D
 Acq On : 05 Oct 2021 05:10
 Operator : SY/MD
 Sample : M4025-07 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

77	11.944	3295	3298	3302	rVV2	1251	1385	0.10%	0.013%
78	11.977	3303	3308	3318	rVB4	2567	3274	0.23%	0.031%
79	12.054	3326	3332	3335	rBV	254	249	0.02%	0.002%
80	12.121	3349	3353	3356	rBV2	197	168	0.01%	0.002%
81	12.195	3359	3376	3393	rBV	611172	984217	68.60%	9.256%
82	12.330	3414	3418	3424	rVB5	703	738	0.05%	0.007%
83	12.571	3491	3493	3498	rBV2	191	188	0.01%	0.002%
84	12.700	3530	3533	3535	rBV2	199	155	0.01%	0.001%
85	12.861	3579	3583	3586	rBV2	182	183	0.01%	0.002%
86	12.989	3621	3623	3626	rBV	195	158	0.01%	0.001%
87	13.054	3638	3643	3646	rBV2	224	262	0.02%	0.002%
88	13.150	3670	3673	3674	rBV	378	221	0.02%	0.002%
89	13.288	3713	3716	3719	rBV2	179	181	0.01%	0.002%
90	13.385	3741	3746	3749	rBV	285	337	0.02%	0.003%
91	13.732	3850	3854	3859	rBV2	207	251	0.02%	0.002%
92	13.948	3914	3921	3926	rBV	264	444	0.03%	0.004%
93	14.176	3989	3992	3997	rVB3	375	305	0.02%	0.003%
94	14.198	3997	3999	4006	rVB2	289	234	0.02%	0.002%
95	14.230	4006	4009	4012	rBV2	349	248	0.02%	0.002%
96	14.542	4097	4106	4112	rBV3	418	845	0.06%	0.008%
97	14.587	4113	4120	4123	rVV2	397	607	0.04%	0.006%
98	14.655	4138	4141	4142	rBV	307	198	0.01%	0.002%
99	14.732	4163	4165	4169	rBV2	339	235	0.02%	0.002%
100	15.131	4285	4289	4294	rBV2	398	464	0.03%	0.004%




Sum of corrected areas: 10633736

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045130.D
Acq On : 05 Oct 2021 05:10
Operator : SY/MD
Sample : M4025-07 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

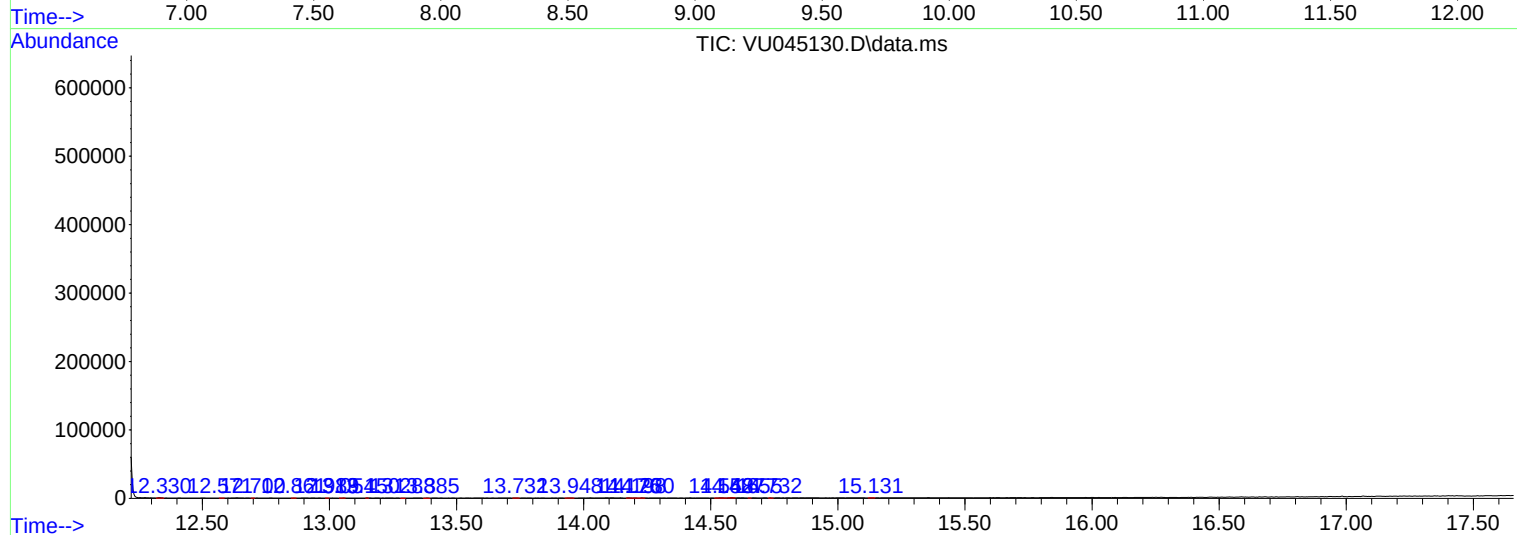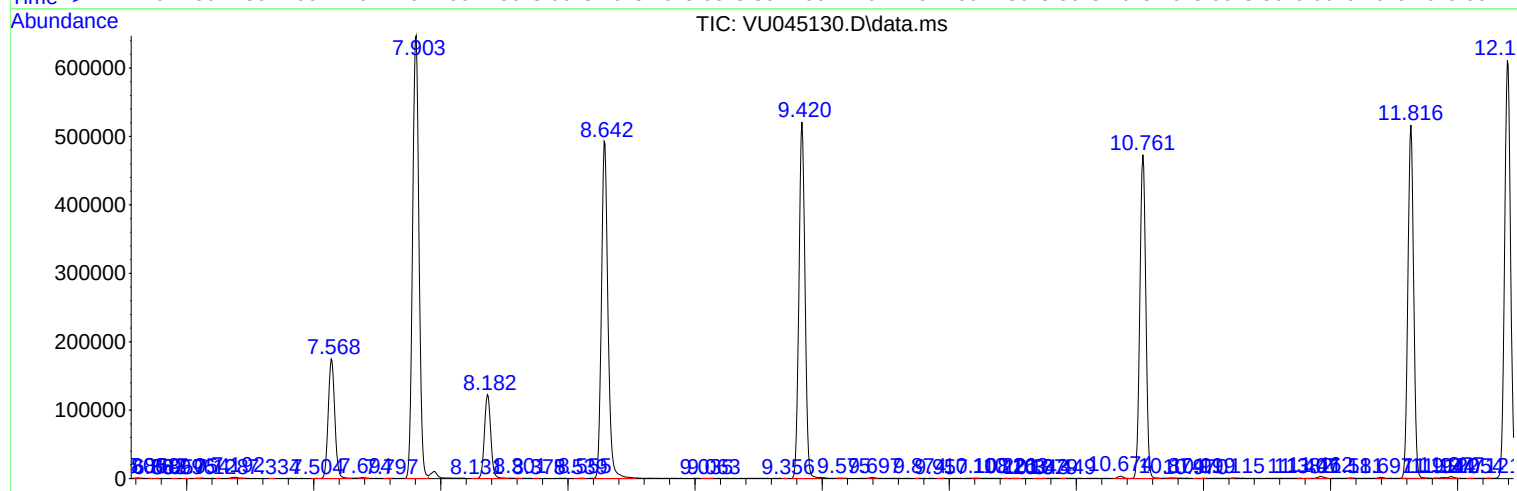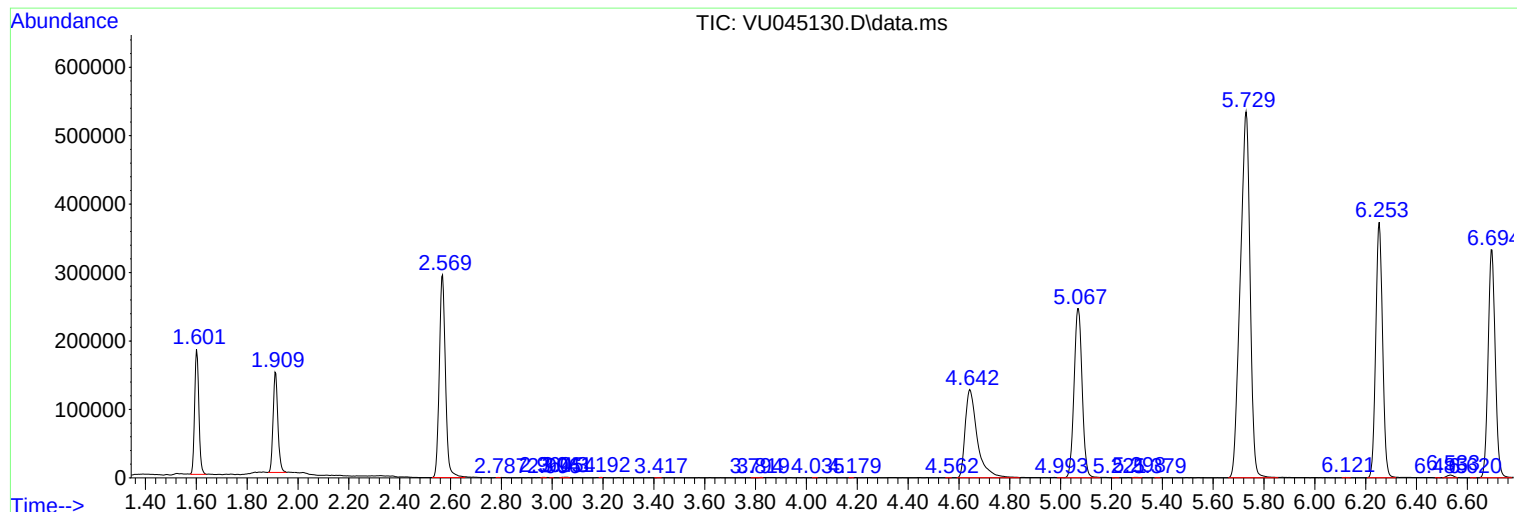

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045130.D
Acq On : 05 Oct 2021 05:10
Operator : SY/MD
Sample : M4025-07 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045130.D
Acq On : 05 Oct 2021 05:10
Operator : SY/MD
Sample : M4025-07 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
