

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045131.D
 Acq On : 05 Oct 2021 05:34
 Operator : SY/MD
 Sample : M4025-08 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045131.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	98	rVB	177132	206273	14.74%	2.005%
2	1.903	168	175	196	rVB	100362	130285	9.31%	1.266%
3	2.565	369	381	415	rVV	290625	489003	34.95%	4.753%
4	2.793	447	452	458	rBV2	458	515	0.04%	0.005%
5	2.819	458	460	466	rVB	220	209	0.01%	0.002%
6	2.861	470	473	475	rBV	239	173	0.01%	0.002%
7	2.954	495	502	507	rBV3	521	816	0.06%	0.008%
8	2.977	507	509	513	rVB	317	182	0.01%	0.002%
9	3.044	525	530	531	rBV2	580	424	0.03%	0.004%
10	3.182	569	573	576	rBV	536	451	0.03%	0.004%
11	3.211	581	582	587	rVB2	403	234	0.02%	0.002%
12	3.263	594	598	602	rVB	194	186	0.01%	0.002%
13	3.501	667	672	676	rBV2	196	171	0.01%	0.002%
14	3.925	798	804	808	rBV2	176	208	0.01%	0.002%
15	4.478	973	976	980	rBV2	190	169	0.01%	0.002%
16	4.555	996	1000	1004	rVB	263	242	0.02%	0.002%
17	4.636	1004	1025	1063	rBV	142347	400104	28.59%	3.889%
18	4.861	1092	1095	1101	rVB2	245	260	0.02%	0.003%
19	5.067	1143	1159	1181	rBV	245611	535469	38.27%	5.205%
20	5.231	1204	1210	1215	rBV2	230	247	0.02%	0.002%
21	5.282	1222	1226	1228	rBV	301	250	0.02%	0.002%
22	5.729	1343	1365	1388	rBV2	517509	1399290	100.00%	13.601%
23	6.076	1468	1473	1479	rVB2	127	174	0.01%	0.002%
24	6.118	1483	1486	1489	rBV2	321	265	0.02%	0.003%
25	6.134	1489	1491	1497	rVB2	246	210	0.02%	0.002%
26	6.179	1498	1505	1508	rVB	286	286	0.02%	0.003%
27	6.253	1513	1528	1552	rBV	350472	656541	46.92%	6.382%
28	6.481	1595	1599	1601	rBV	293	173	0.01%	0.002%
29	6.533	1605	1615	1627	rVB3	3756	6435	0.46%	0.063%
30	6.697	1650	1666	1694	rBV	324425	638574	45.64%	6.207%
31	6.947	1740	1744	1747	rBV	243	210	0.02%	0.002%
32	6.967	1747	1750	1755	rVB	222	189	0.01%	0.002%
33	7.044	1770	1774	1776	rBV	559	505	0.04%	0.005%
34	7.118	1792	1797	1799	rBV2	222	202	0.01%	0.002%
35	7.185	1810	1818	1829	rVB5	2223	3905	0.28%	0.038%
36	7.568	1925	1937	1959	rBV	172414	303645	21.70%	2.951%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045131.D
 Acq On : 05 Oct 2021 05:34
 Operator : SY/MD
 Sample : M4025-08 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.690	1966	1975	1985	rVB3	1101	2020	0.14%	0.020%
38	7.902	2025	2041	2056	rBV	646782	1096697	78.38%	10.660%
39	7.970	2056	2062	2074	rVB	9576	16308	1.17%	0.159%
40	8.076	2090	2095	2097	rBV2	355	365	0.03%	0.004%
41	8.182	2115	2128	2147	rBV2	120110	204195	14.59%	1.985%
42	8.349	2177	2180	2184	rVB	202	176	0.01%	0.002%
43	8.375	2184	2188	2191	rBV2	248	223	0.02%	0.002%
44	8.410	2194	2199	2206	rBV2	163	254	0.02%	0.002%
45	8.459	2210	2214	2218	rBV2	193	249	0.02%	0.002%
46	8.555	2242	2244	2247	rVB2	331	222	0.02%	0.002%
47	8.642	2257	2271	2303	rBV	484779	852811	60.95%	8.289%
48	8.890	2343	2348	2351	rVB2	391	339	0.02%	0.003%
49	8.906	2351	2353	2359	rVB2	222	225	0.02%	0.002%
50	8.996	2375	2381	2382	rBV2	209	246	0.02%	0.002%
51	9.420	2499	2513	2533	rBV	497659	811196	57.97%	7.885%
52	9.574	2555	2561	2568	rVV3	439	537	0.04%	0.005%
53	9.693	2593	2598	2606	rBV2	940	1378	0.10%	0.013%
54	9.777	2620	2624	2628	rBV	215	255	0.02%	0.002%
55	10.018	2697	2699	2706	rVB2	310	262	0.02%	0.003%
56	10.102	2720	2725	2732	rVB3	426	577	0.04%	0.006%
57	10.282	2777	2781	2784	rBV2	211	271	0.02%	0.003%
58	10.346	2799	2801	2807	rBV2	171	206	0.01%	0.002%
59	10.391	2811	2815	2819	rBV	180	238	0.02%	0.002%
60	10.674	2895	2903	2912	rBV2	3248	4502	0.32%	0.044%
61	10.761	2917	2930	2948	rVB	469913	759248	54.26%	7.380%
62	10.851	2955	2958	2960	rBV2	280	186	0.01%	0.002%
63	10.870	2960	2964	2969	rVB3	454	385	0.03%	0.004%
64	10.902	2970	2974	2978	rVB3	316	312	0.02%	0.003%
65	10.934	2978	2984	2985	rBV	197	214	0.02%	0.002%
66	10.979	2994	2998	3001	rBV2	225	237	0.02%	0.002%
67	11.002	3001	3005	3008	rVV2	311	253	0.02%	0.002%
68	11.092	3026	3033	3036	rBV	365	417	0.03%	0.004%
69	11.121	3037	3042	3046	rBV4	544	594	0.04%	0.006%
70	11.211	3067	3070	3076	rVB2	439	328	0.02%	0.003%
71	11.250	3076	3082	3084	rBV	244	262	0.02%	0.003%
72	11.298	3093	3097	3100	rVB2	277	174	0.01%	0.002%
73	11.391	3123	3126	3130	rBV2	332	295	0.02%	0.003%
74	11.462	3140	3148	3158	rVB4	2658	4543	0.32%	0.044%
75	11.581	3179	3185	3193	rBV2	506	645	0.05%	0.006%
76	11.700	3216	3222	3230	rVB	1339	1645	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
 Data File : VU045131.D
 Acq On : 05 Oct 2021 05:34
 Operator : SY/MD
 Sample : M4025-08 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

77	11.815	3245	3258	3282	rBV	490652	764370	54.63%	7.430%
78	11.922	3288	3291	3294	rBV3	367	364	0.03%	0.004%
79	11.944	3295	3298	3302	rVV2	1368	1357	0.10%	0.013%
80	11.976	3303	3308	3316	rVB3	2559	3202	0.23%	0.031%
81	12.089	3340	3343	3348	rVB2	219	251	0.02%	0.002%
82	12.121	3348	3353	3358	rBV3	323	413	0.03%	0.004%
83	12.195	3358	3376	3395	rBV	602617	972978	69.53%	9.457%
84	12.330	3416	3418	3423	rBV3	602	540	0.04%	0.005%
85	12.635	3509	3513	3515	rBV3	490	387	0.03%	0.004%
86	12.719	3537	3539	3542	rBV	217	176	0.01%	0.002%
87	12.767	3550	3554	3557	rBV3	414	358	0.03%	0.003%
88	12.979	3617	3620	3624	rBV2	203	186	0.01%	0.002%
89	13.147	3666	3672	3676	rBV4	520	629	0.04%	0.006%
90	13.568	3798	3803	3807	rBV2	196	244	0.02%	0.002%
91	13.822	3878	3882	3883	rBV2	288	210	0.02%	0.002%
92	13.963	3920	3926	3928	rBV2	266	292	0.02%	0.003%
93	14.002	3935	3938	3941	rBV	240	197	0.01%	0.002%
94	14.179	3990	3993	3997	rBV	279	184	0.01%	0.002%
95	14.346	4041	4045	4047	rBV2	305	221	0.02%	0.002%
96	14.359	4047	4049	4052	rVB2	289	192	0.01%	0.002%
97	14.529	4100	4102	4105	rBV3	249	179	0.01%	0.002%
98	14.577	4112	4117	4119	rBV2	371	402	0.03%	0.004%
99	14.700	4152	4155	4158	rBV3	324	301	0.02%	0.003%
100	14.854	4197	4203	4208	rBV2	415	545	0.04%	0.005%




Sum of corrected areas: 10288143

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045131.D
Acq On : 05 Oct 2021 05:34
Operator : SY/MD
Sample : M4025-08 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

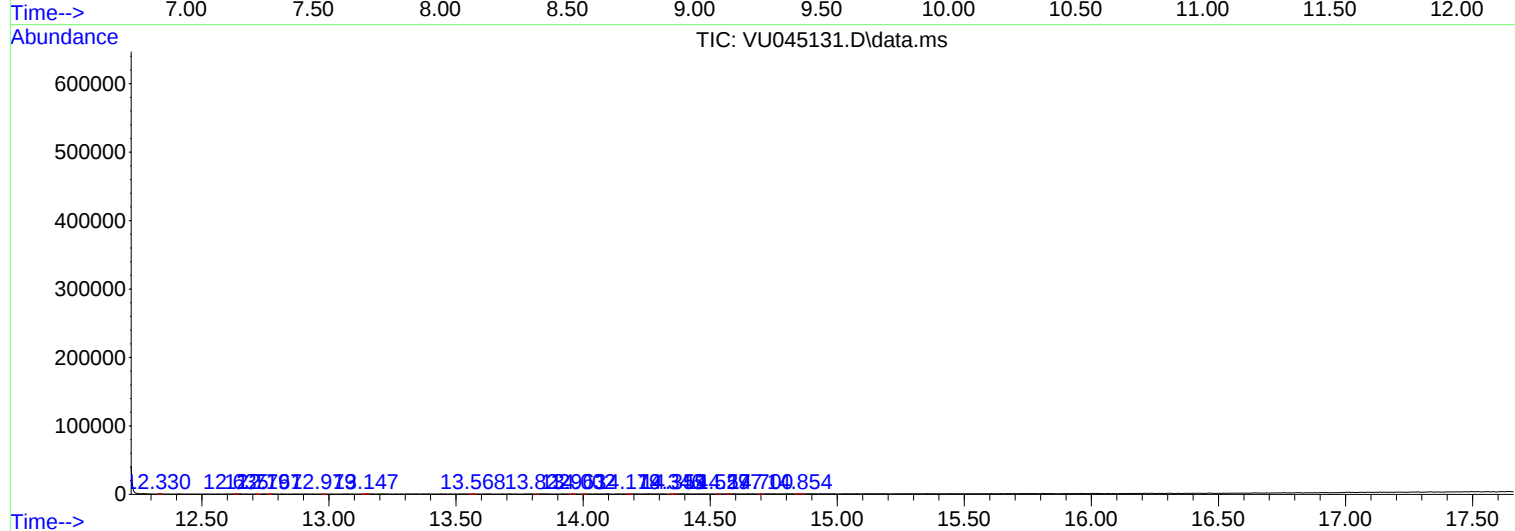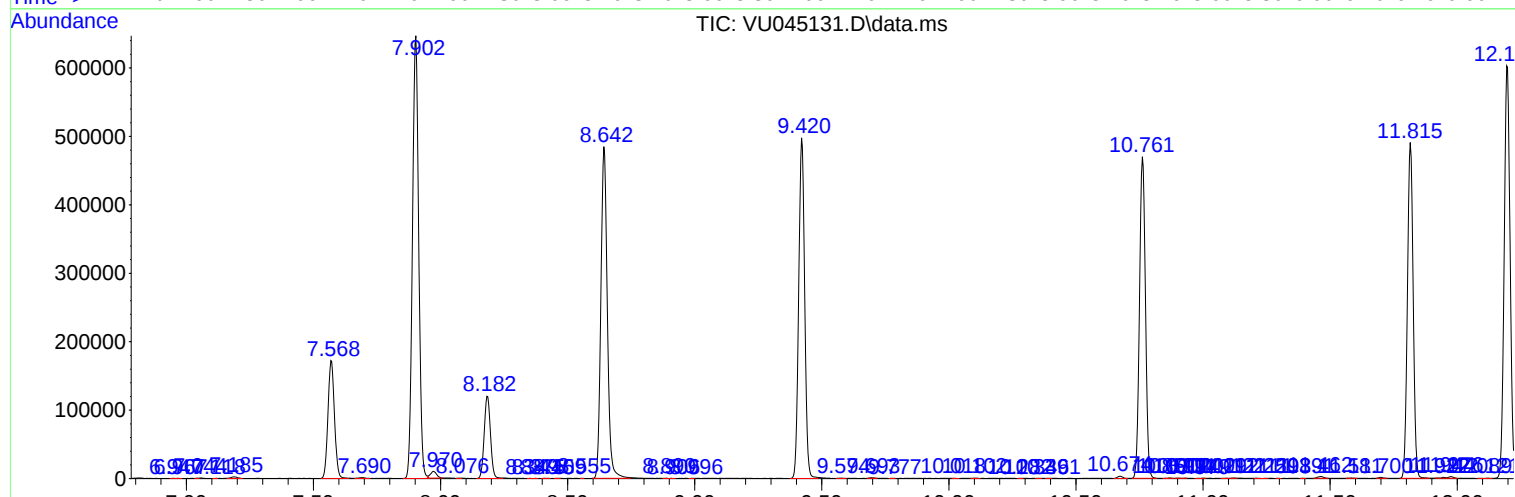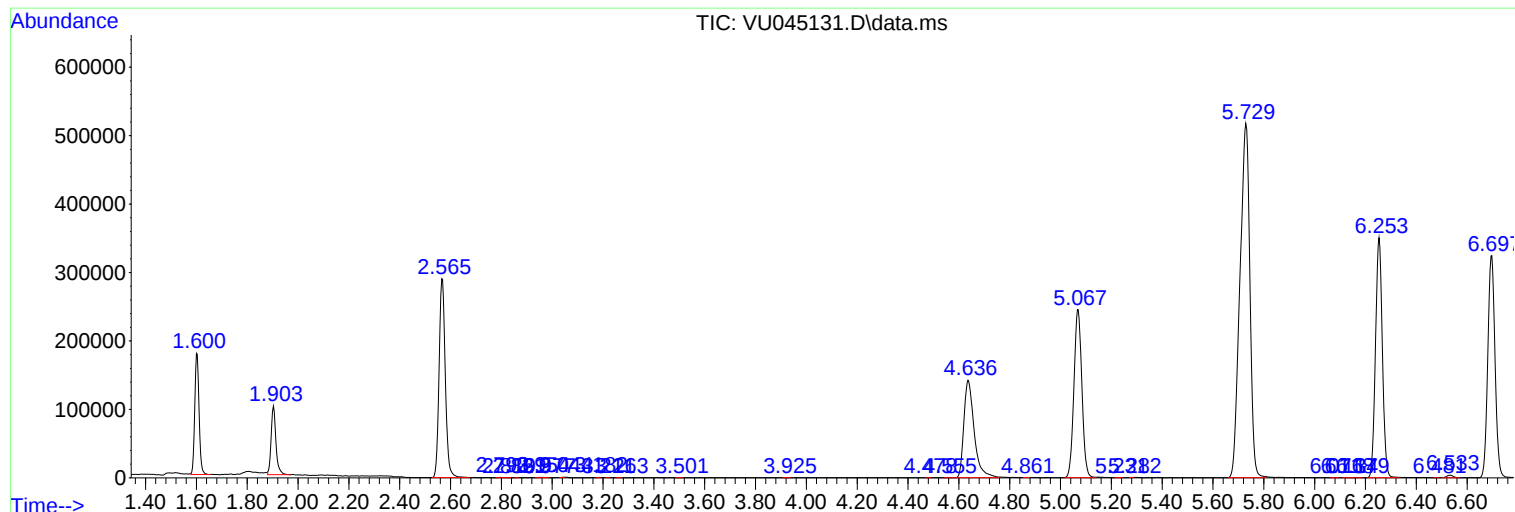

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045131.D
Acq On : 05 Oct 2021 05:34
Operator : SY/MD
Sample : M4025-08 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045131.D
Acq On : 05 Oct 2021 05:34
Operator : SY/MD
Sample : M4025-08 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
