


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100421\
Data File : VU045085.D
Acq On : 04 Oct 2021 09:21
Operator : SY/MD
Sample : BFB005
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB005

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Title : VOC Analysis
Last Update : Mon Oct 11 01:47:08 2021

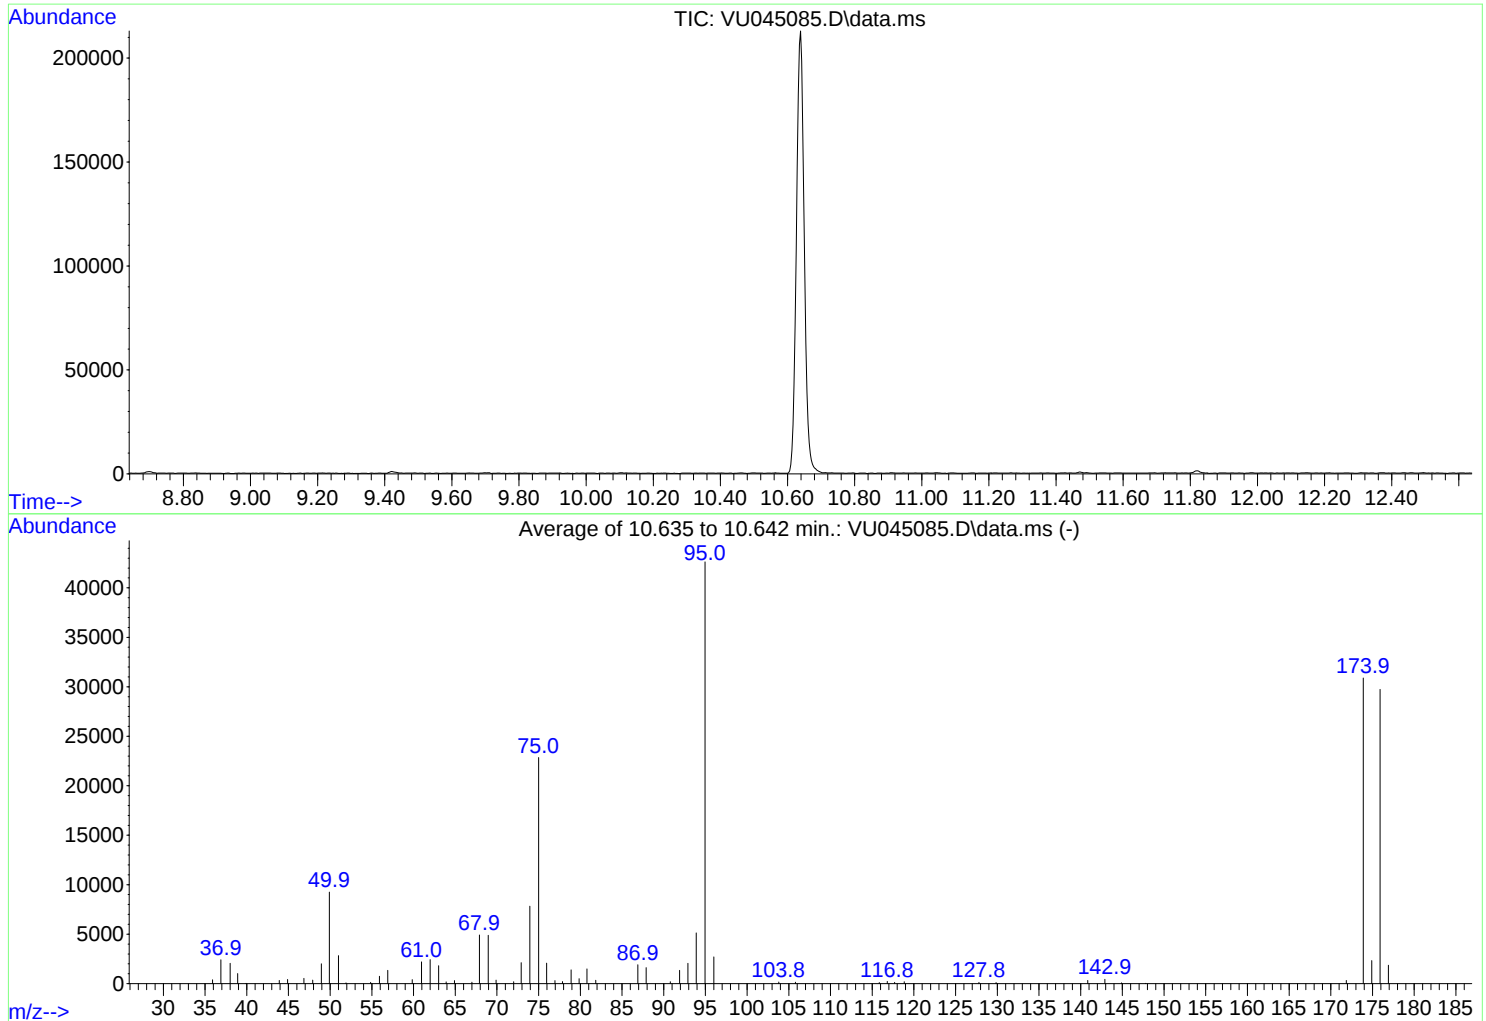

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.7	9244	PASS
75	95	30	80	53.6	22843	PASS
95	95	100	100	100.0	42627	PASS
96	95	5	9	6.3	2703	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.5	30893	PASS
175	174	5	9	7.6	2335	PASS
176	174	95	101	96.3	29744	PASS
177	176	5	9	6.2	1852	PASS

Scan 2879 (10.597 min): VU045085.D\data.ms
BFB005

m/z	Abundance
39.90	119.0
43.90	222.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
35.90	381.0
36.90	2461.0
38.00	2158.0
38.90	1062.0
39.90	127.0
43.90	559.0
44.90	408.0
46.90	548.0
47.90	326.0
48.90	2074.0
49.90	9411.0
51.00	2951.0
51.90	122.0
54.80	148.0
55.90	808.0
56.90	1382.0
59.80	385.0
61.00	2224.0
62.00	2406.0
63.00	1760.0
63.90	181.0
64.90	298.0
67.00	149.0
67.90	5026.0
68.90	5087.0
69.90	337.0
71.90	200.0
72.90	2147.0
74.00	7849.0
75.00	22808.0
75.90	2186.0
77.00	354.0
77.90	230.0
78.90	1376.0
79.80	536.0
80.80	1600.0
81.90	357.0
86.90	1934.0
87.90	1677.0
90.80	194.0
91.90	1300.0
92.90	2098.0
93.90	5184.0
95.00	42856.0
96.00	2801.0
103.80	174.0
105.80	151.0
115.80	107.0
116.80	223.0
117.70	141.0
118.90	211.0
127.80	142.0
129.80	109.0
140.80	315.0
142.90	472.0
144.90	113.0
147.80	101.0
171.90	285.0
173.90	29864.0
174.90	2219.0
175.90	29488.0
176.90	1912.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
35.90	398.0
36.90	2518.0
38.00	2125.0
38.90	1075.0
39.90	140.0
43.90	565.0
44.90	445.0
46.90	558.0
47.90	378.0
48.90	2054.0
49.90	9524.0
51.00	2918.0
51.90	110.0
54.90	135.0
55.90	762.0
56.90	1382.0
59.90	431.0
60.90	2242.0
62.00	2531.0
63.00	1885.0
63.90	179.0
64.90	303.0
67.00	151.0
67.90	5068.0
68.90	5024.0
69.90	368.0
72.00	195.0
72.90	2195.0
73.90	8099.0
75.00	23688.0
76.00	2131.0
76.90	303.0
77.80	205.0
78.90	1422.0
79.80	531.0
80.80	1525.0
81.90	353.0
86.90	1987.0
87.90	1654.0
90.80	214.0
91.90	1389.0
92.90	2144.0
93.90	5353.0
94.90	44128.0
96.00	2796.0
103.80	167.0
105.80	149.0
115.90	116.0
116.80	232.0
117.70	134.0
118.80	197.0
127.80	135.0
129.90	107.0
140.90	335.0
142.90	460.0
144.90	114.0
171.90	327.0
173.90	31912.0
174.90	2423.0
175.90	30712.0
176.90	1901.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
35.90	382.0
36.90	2234.0
38.00	1869.0
38.90	921.0
39.90	183.0
43.90	535.0
44.90	416.0
46.80	511.0
47.90	352.0
49.00	1881.0
49.90	8796.0
51.00	2613.0
54.90	110.0
55.90	667.0
56.90	1273.0
59.90	408.0
60.90	2153.0
62.00	2362.0
63.00	1788.0
63.90	192.0
64.90	310.0
67.00	138.0
67.90	4661.0
69.00	4521.0
69.90	371.0
72.10	168.0
72.90	2037.0
73.90	7551.0
75.00	22032.0
76.00	1905.0
76.90	273.0
77.80	205.0
78.90	1355.0
79.90	455.0
80.80	1340.0
81.80	319.0
86.90	1788.0
87.90	1529.0
90.80	197.0
91.90	1328.0
92.90	1915.0
93.90	4858.0
95.00	40896.0
96.00	2512.0
103.80	138.0
105.80	128.0
115.90	122.0
116.80	223.0
117.70	130.0
118.80	191.0
127.80	113.0
129.90	124.0
140.90	337.0
142.90	396.0
171.80	351.0
173.90	30904.0
174.90	2364.0
175.90	29032.0
176.90	1744.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005