
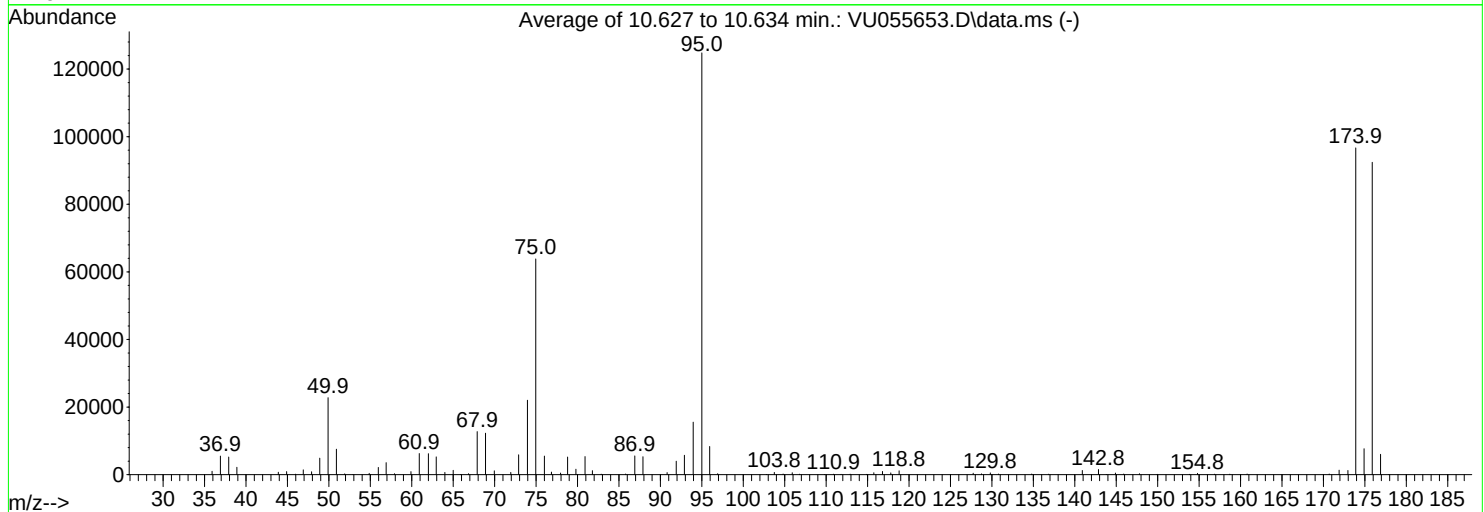


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100423\
Data File : VU055653.D
Acq On : 04 Oct 2023 08:44
Operator : MD/SY
Sample : BFB057
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB057

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR091923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Oct 04 23:00:34 2023

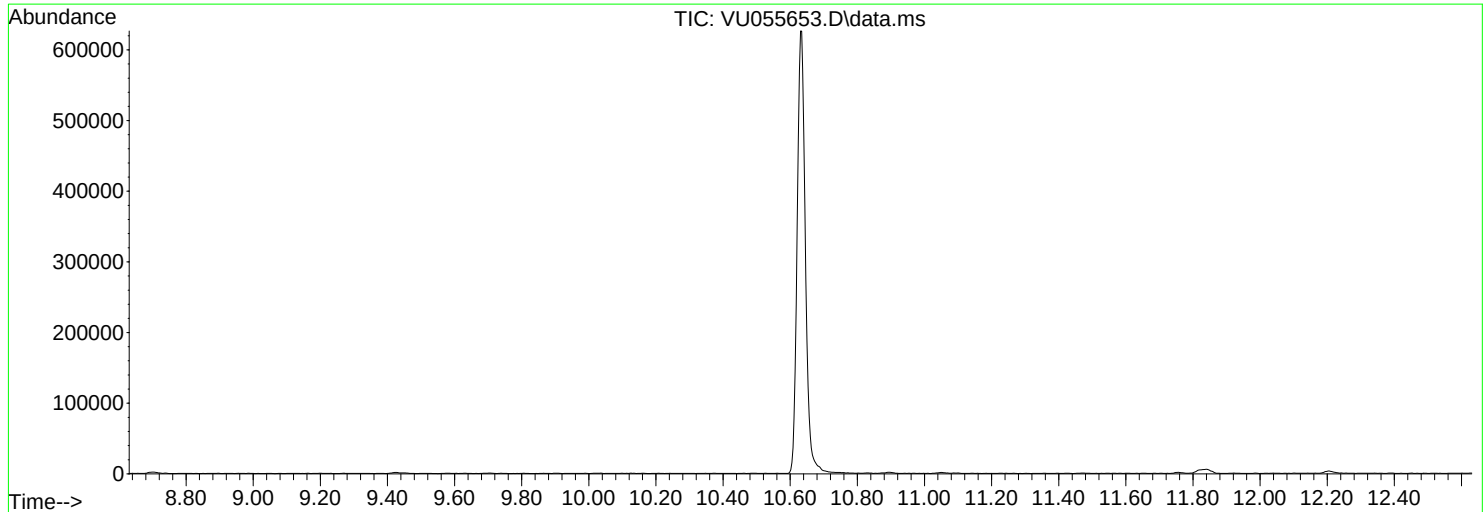

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	22797	PASS
75	95	30	80	51.1	63805	PASS
95	95	100	100	100.0	124811	PASS
96	95	5	9	6.7	8332	PASS
173	174	0.00	2	1.3	1255	PASS
174	95	50	120	77.5	96701	PASS
175	174	5	9	7.9	7658	PASS
176	174	95	101	95.6	92443	PASS
177	176	5	9	6.5	6006	PASS

m/z	Abundance
39.80	182.0
43.90	489.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
35.90	897.0
36.90	5278.0
37.90	4922.0
38.90	2001.0
39.80	148.0
43.90	1160.0
44.90	833.0
45.90	148.0
46.90	1394.0
47.90	872.0
48.90	4615.0
49.90	21656.0
50.90	7258.0
51.90	172.0
52.90	105.0
54.90	320.0
56.00	1908.0
56.90	3436.0
57.90	230.0
59.80	927.0
60.90	6092.0
62.00	6014.0
63.00	5050.0
64.00	590.0
65.00	1157.0
65.90	120.0
66.80	294.0
67.90	12096.0
68.90	11162.0
70.00	1115.0
71.90	560.0
72.90	5405.0
73.90	20952.0
75.00	60392.0
76.00	5358.0
76.80	724.0
78.00	456.0
78.80	5066.0
79.80	1503.0
80.90	4930.0
81.80	1107.0
82.90	136.0
85.80	252.0
86.90	5031.0
87.90	4892.0
90.80	463.0
91.90	3774.0
92.90	5426.0
93.90	14384.0
95.00	118568.0
96.00	7984.0
96.90	255.0
103.70	577.0
104.80	204.0
105.90	536.0
106.80	164.0
110.90	120.0
112.90	185.0
115.80	595.0
116.80	991.0
117.80	464.0
118.80	932.0
127.80	376.0
128.90	269.0
129.80	579.0
130.80	141.0
134.80	174.0
136.90	157.0
140.90	1155.0
142.90	1410.0
143.80	114.0
144.90	370.0
145.90	188.0
147.80	254.0
153.80	126.0
154.80	334.0
156.90	156.0
158.70	136.0
160.80	179.0
170.70	169.0
171.90	1150.0
172.90	1144.0
173.90	89776.0
174.90	6977.0
175.90	85136.0
176.90	5793.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
35.90	977.0
36.90	5685.0
37.90	5439.0
38.90	2201.0
39.80	129.0
43.90	1230.0
44.90	907.0
46.00	168.0
46.90	1525.0
47.90	968.0
48.90	5075.0
49.90	23384.0
50.90	7799.0
51.90	245.0
54.80	409.0
55.90	2204.0
56.90	3621.0
57.90	295.0
59.90	885.0
60.90	6432.0
62.00	6414.0
62.90	5456.0
64.00	690.0
65.00	1322.0
66.90	319.0
67.90	13145.0
68.90	12524.0
70.00	1184.0
72.00	695.0
72.90	6121.0
73.90	22760.0
75.00	65680.0
76.00	5596.0
76.90	746.0
77.90	478.0
78.80	5361.0
79.80	1654.0
80.90	5554.0
81.80	1247.0
82.90	143.0
85.80	188.0
86.90	5689.0
87.90	5430.0
90.80	627.0
91.90	4175.0
92.90	5985.0
94.00	16203.0
95.00	128720.0
96.00	8481.0
96.90	291.0
102.80	100.0
103.80	696.0
104.80	196.0
105.90	581.0
106.80	139.0
109.80	105.0
110.90	163.0
111.80	148.0
112.90	182.0
114.90	147.0
115.70	557.0
116.80	990.0
117.80	520.0
118.80	1209.0
127.70	438.0
128.70	265.0
129.80	539.0
130.80	205.0
134.80	202.0
136.90	139.0
140.90	1247.0
142.80	1584.0
143.80	109.0
144.90	528.0
145.90	215.0
147.80	281.0
149.90	153.0
153.90	108.0
154.80	395.0
156.90	129.0
158.70	131.0
160.80	233.0
170.70	195.0
171.90	1344.0
172.90	1262.0
173.90	99400.0
174.90	7959.0
175.90	95144.0
176.90	6246.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057

m/z	Abundance
35.90	1056.0
36.90	5498.0
37.90	5228.0
38.90	2402.0
39.80	154.0
43.90	1205.0
44.90	932.0
46.00	171.0
46.90	1423.0
47.90	789.0
48.90	5013.0
49.90	23352.0
50.90	7585.0
51.90	317.0
54.80	459.0
55.90	2224.0
56.90	3585.0
57.90	295.0
60.00	860.0
60.90	6188.0
62.00	6177.0
62.90	5248.0
64.00	726.0
65.00	1314.0
66.90	297.0
67.90	13046.0
68.90	13111.0
69.90	1072.0
72.00	708.0
72.90	6044.0
74.00	22304.0
74.90	65344.0
76.00	5590.0
76.90	762.0
77.90	537.0
78.80	5189.0
79.80	1697.0
80.90	5517.0
81.80	1234.0
82.80	123.0
85.70	126.0
86.90	5943.0
87.90	5541.0
90.80	703.0
91.90	4007.0
92.90	5832.0
93.90	16042.0
95.00	127144.0
95.90	8530.0
96.90	280.0
102.80	117.0
103.80	726.0
104.80	196.0
105.90	658.0
106.80	112.0
110.90	173.0
111.80	153.0
112.90	135.0
114.90	170.0
115.70	556.0
116.80	934.0
117.80	544.0
118.80	1215.0
127.70	409.0
128.70	234.0
129.80	426.0
130.80	209.0
134.80	231.0
136.70	143.0
140.90	1245.0
142.80	1625.0
144.90	572.0
145.90	163.0
147.80	258.0
150.00	180.0
153.90	106.0
154.80	392.0
156.80	120.0
158.70	117.0
160.80	233.0
170.70	184.0
171.90	1478.0
173.00	1358.0
173.90	100928.0
174.90	8038.0
175.90	97048.0
176.90	5979.0
177.90	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB057