

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U100518\
 Data File : VU027449.D
 Acq On : 05 Oct 2018 13:34
 Operator : MD/SY
 Sample : J5180-20ME
 Misc : 4.28g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JLC29ME

Quant Time: Oct 08 16:16:57 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 06 04:54:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	227916	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	222748	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	122636	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	66382	37.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.02%
7) Chloroethane-d5	1.64	69	45718	33.09	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	66.18%#
11) 1,1-Dichloroethene-d2	2.23	63	86157	25.61	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	51.22%#
21) 2-Butanone-d5	4.20	46	104528	72.19	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	72.19%
24) Chloroform-d	4.64	84	107909	37.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.22%
26) 1,2-Dichloroethane-d4	5.31	65	78784	39.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.38%
32) Benzene-d6	5.33	84	234512	36.74	ug/L	-0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	73.48%
36) 1,2-Dichloropropane-d6	6.33	67	83463	38.17	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	76.34%
41) Toluene-d8	7.56	98	206502	36.19	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	72.38%#
43) trans-1,3-Dichloropropene-	7.85	79	39075	37.08	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.16%
47) 2-Hexanone-d5	8.33	63	90920	82.33	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.33%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	121155	42.37	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.74%
64) 1,2-Dichlorobenzene-d4	11.86	152	91804	38.26	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	76.52%#


Target Compounds					Ovalue
13) Acetone	2.34	43	3912	3.294 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100518\
Data File : VU027449.D
Acq On : 05 Oct 2018 13:34
Operator : MD/SY
Sample : J5180-20ME
Misc : 4.28µ/5mL/100µL/5.0mL/MSVOA_U/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JLC29ME

Quant Time: Oct 08 16:16:57 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 06 04:54:09 2018
Response via : Initial Calibration

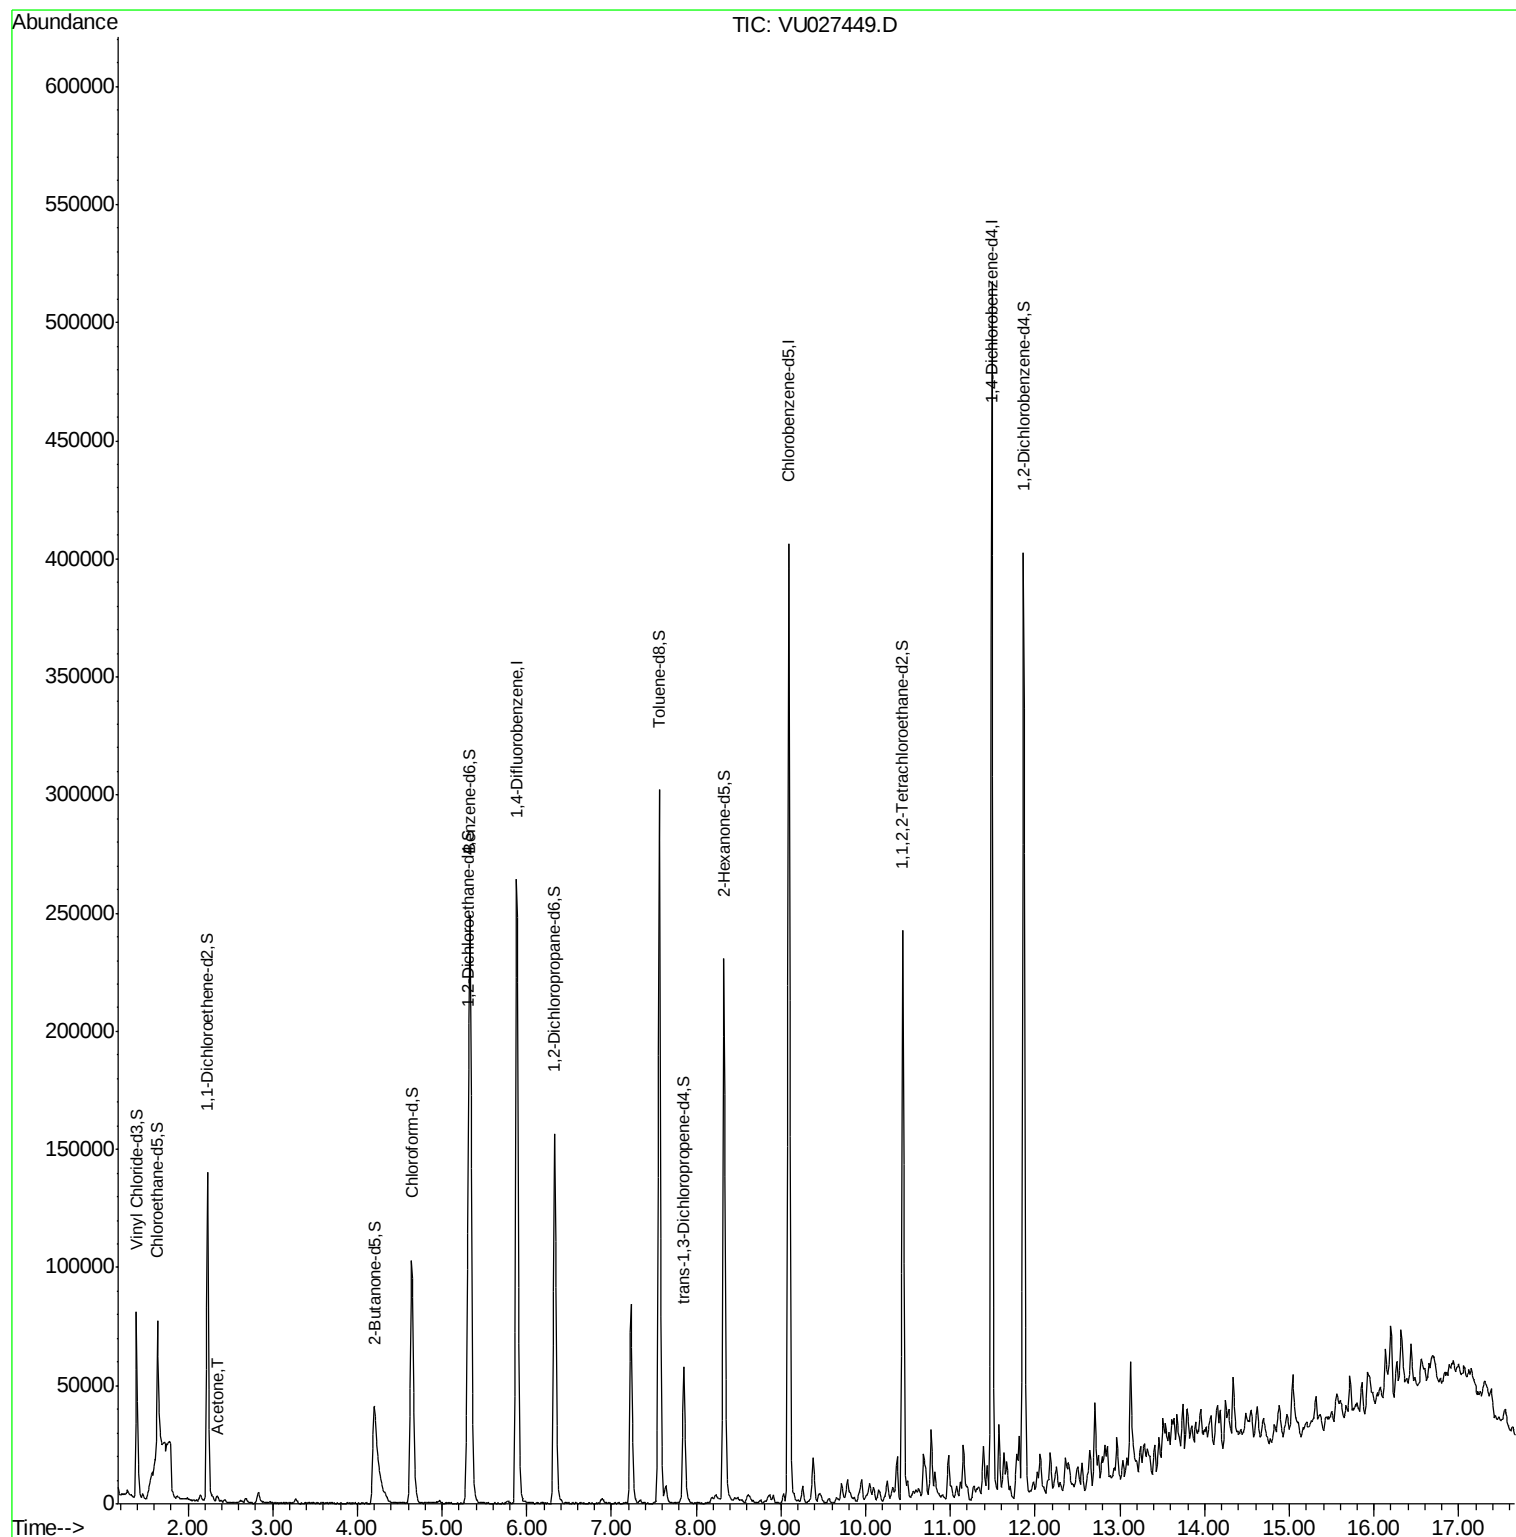

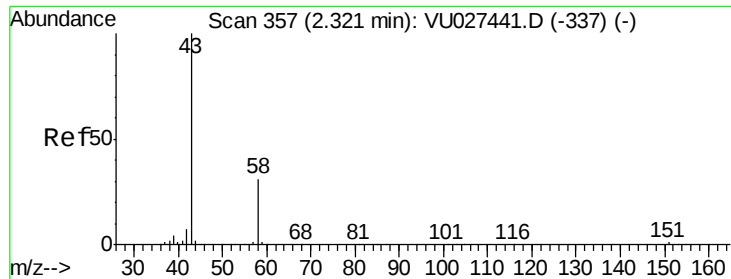

#13

Acetone

Concen: 3.294 ug/L

RT: 2.34 min Scan# 364

Delta R.T. 0.02 min

Lab File: VU027449.D

Acq: 05 Oct 2018 13:34

Instrument :

MSVOA_U

ClientSampleId :

JLC29ME

Tot Ion: 43 Resp: 3912

Ion Ratio Lower Upper

43 100

58 29.3 0.0 60.8

