

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U100518\
 Data File : VU027450.D
 Acq On : 05 Oct 2018 13:57
 Operator : MD/SY
 Sample : J5182-12ME
 Misc : 4.05µ/5mL/100µL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JLC61ME

Quant Time: Oct 06 05:12:46 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 06 04:54:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	230278	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	221856	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	119942	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	67417	37.20	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.40%
7) Chloroethane-d5	1.64	69	47598	34.09	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	68.18%#
11) 1,1-Dichloroethene-d2	2.23	63	95324	28.04	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	56.08%#
21) 2-Butanone-d5	4.20	46	110921	75.82	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	75.82%
24) Chloroform-d	4.65	84	112304	38.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.48%
26) 1,2-Dichloroethane-d4	5.30	65	80797	39.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.56%
32) Benzene-d6	5.33	84	244745	38.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.98%
36) 1,2-Dichloropropane-d6	6.33	67	86269	39.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	79.22%
41) Toluene-d8	7.57	98	213518	37.57	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	75.14%#
43) trans-1,3-Dichloropropene-	7.85	79	40168	38.27	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.54%
47) 2-Hexanone-d5	8.33	63	94958	86.33	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.33%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	124879	43.85	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.70%
64) 1,2-Dichlorobenzene-d4	11.86	152	92754	39.53	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.06%#


Target Compounds					Ovalue
13) Acetone	2.34	43	51482	42.904 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100518\
Data File : VU027450.D
Acq On : 05 Oct 2018 13:57
Operator : MD/SY
Sample : J5182-12ME
Misc : 4.05µL/100µL/5.0mL/MSVOA_U/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JLC61ME

Quant Time: Oct 06 05:12:46 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 06 04:54:09 2018
Response via : Initial Calibration

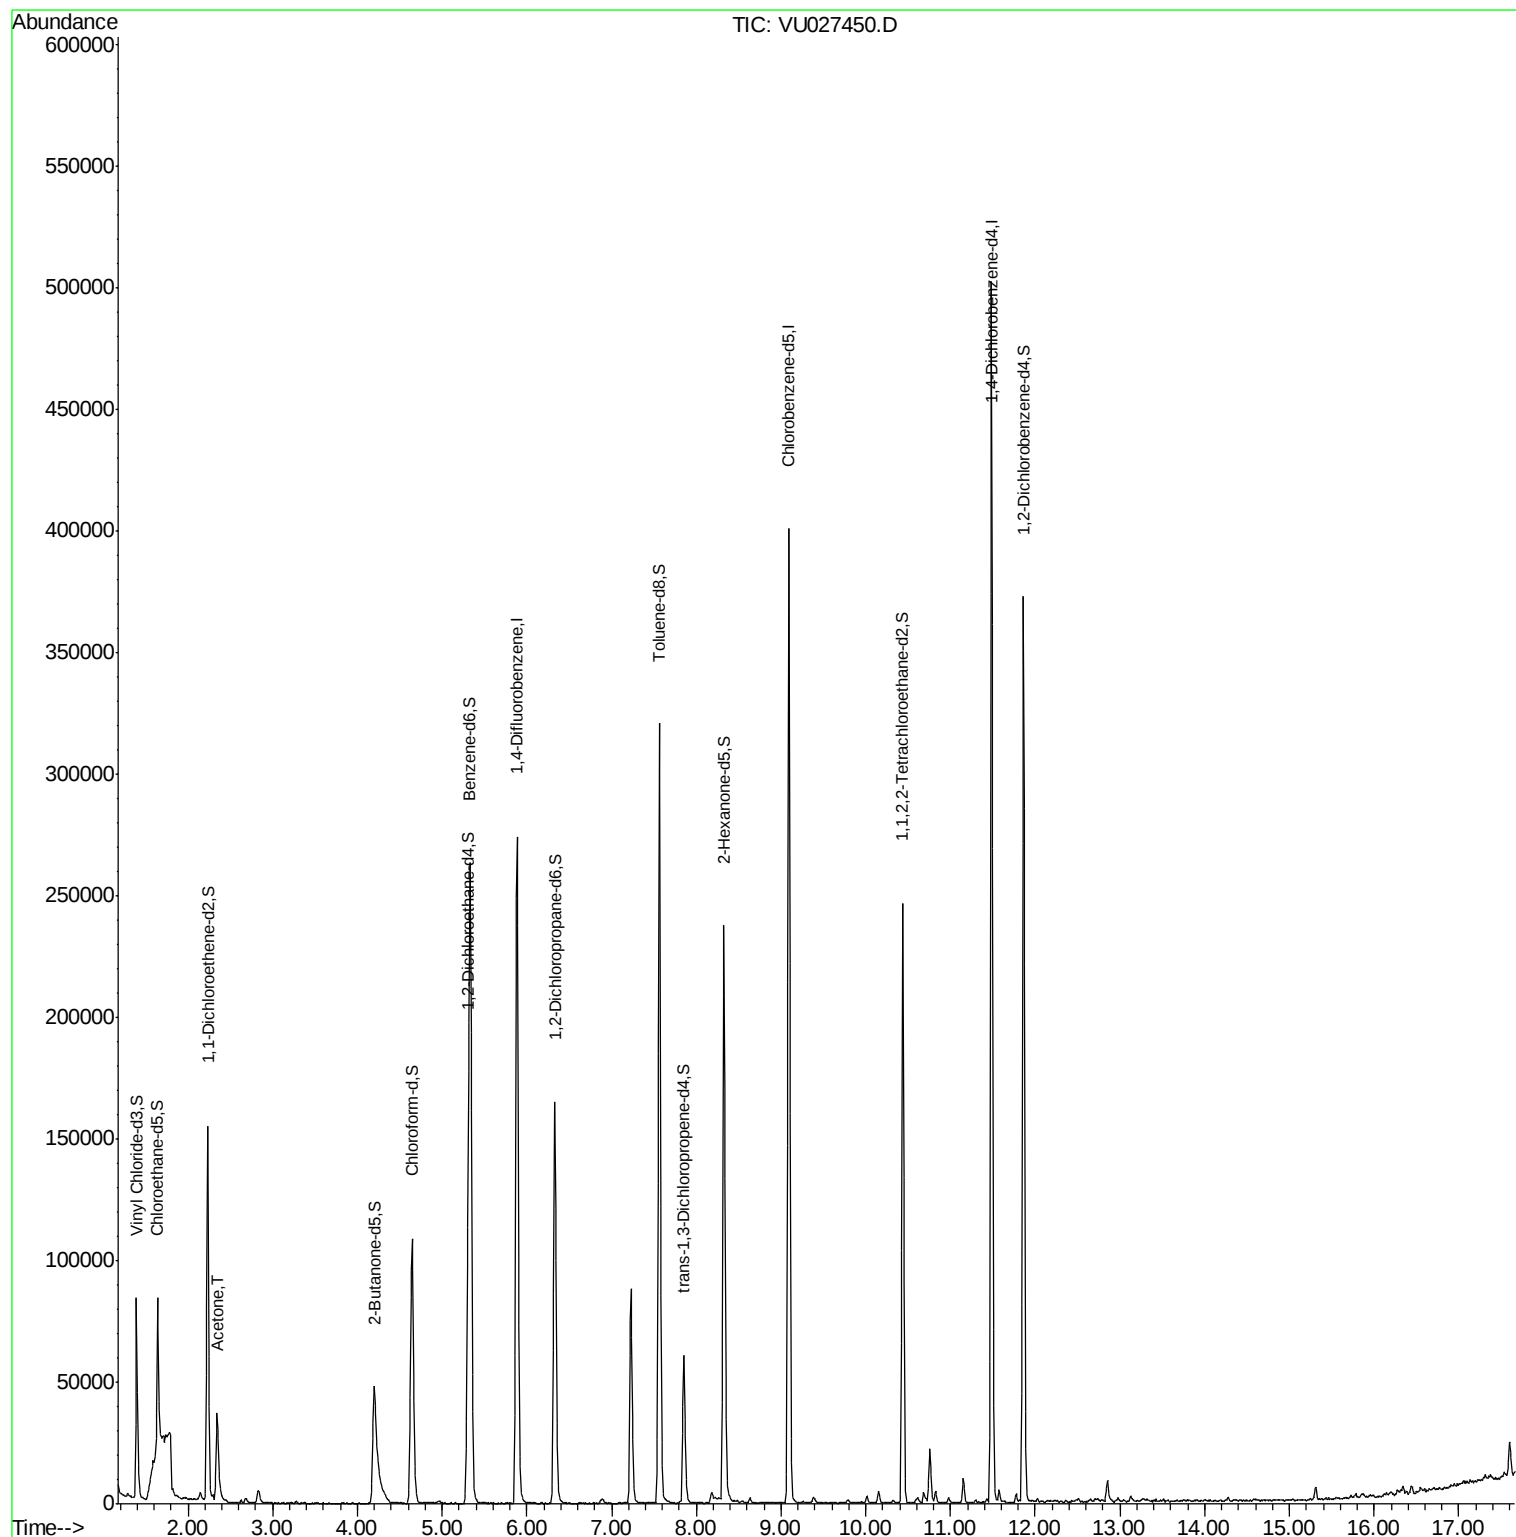

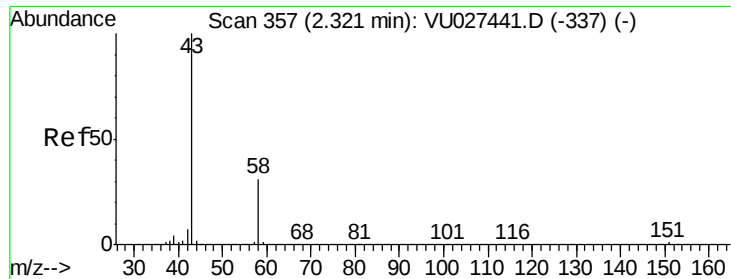

#13

Acetone

Concen: 42.904 ug/L

RT: 2.34 min Scan# 364

Delta R.T. 0.02 min

Lab File: VU027450.D

Acq: 05 Oct 2018 13:57

Instrument :

MSVOA_U

ClientSampleId :

JLC61ME

Tot Ion: 43 Resp: 51482

Ion Ratio Lower Upper

43 100

58 31.5 0.0 60.8

