

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100518\
 Data File : VU027453.D
 Acq On : 05 Oct 2018 15:18
 Operator : MD/SY
 Sample : J5250-03 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0911

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	63	70	80	rBV	123244	125522	14.25%	1.858%
2	1.682	151	158	181	rVB	94327	121296	13.77%	1.795%
3	2.273	331	342	356	rBV	193612	291772	33.12%	4.318%
4	2.518	415	418	420	rBV	199	119	0.01%	0.002%
5	2.665	462	464	467	rBV	164	79	0.01%	0.001%
6	2.701	470	475	477	rBV3	566	502	0.06%	0.007%
7	2.759	490	493	495	rBV	100	66	0.01%	0.001%
8	2.842	515	519	521	rBV2	351	298	0.03%	0.004%
9	2.910	539	540	542	rVB	131	51	0.01%	0.001%
10	3.042	579	581	588	rVB	191	118	0.01%	0.002%
11	3.154	615	616	618	rVB	136	48	0.01%	0.001%
12	3.202	627	631	633	rBV	219	151	0.02%	0.002%
13	3.296	658	660	663	rVB2	165	88	0.01%	0.001%
14	3.347	671	676	677	rBV	152	80	0.01%	0.001%
15	3.386	686	688	690	rVB	121	48	0.01%	0.001%
16	3.431	700	702	705	rVB	145	51	0.01%	0.001%
17	3.537	733	735	740	rVB	215	150	0.02%	0.002%
18	3.572	744	746	751	rBV	191	114	0.01%	0.002%
19	3.691	780	783	786	rBV	86	63	0.01%	0.001%
20	3.749	799	801	802	rBV	104	59	0.01%	0.001%
21	3.849	831	832	835	rBV	119	48	0.01%	0.001%
22	3.923	853	855	860	rBV	75	61	0.01%	0.001%
23	3.958	863	866	869	rVB2	220	179	0.02%	0.003%
24	4.048	892	894	896	rVB	120	66	0.01%	0.001%
25	4.080	902	904	908	rVB	164	72	0.01%	0.001%
26	4.180	920	935	968	rBV	85403	232199	26.36%	3.436%
27	4.543	1046	1048	1049	rBV	262	94	0.01%	0.001%
28	4.582	1058	1060	1063	rBV	125	72	0.01%	0.001%
29	4.652	1063	1082	1113	rBV	132084	333506	37.86%	4.935%
30	4.807	1125	1130	1135	rBV2	471	517	0.06%	0.008%
31	4.861	1145	1147	1149	rBV	103	74	0.01%	0.001%
32	4.894	1149	1157	1165	rVB4	553	1038	0.12%	0.015%
33	4.987	1183	1186	1188	rBV2	189	115	0.01%	0.002%
34	5.054	1203	1207	1211	rVB2	152	104	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100518\
 Data File : VU027453.D
 Acq On : 05 Oct 2018 15:18
 Operator : MD/SY
 Sample : J5250-03 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0911

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

35	5.138	1230	1233	1236	rBV	94	58	0.01%	0.001%
36	5.177	1242	1245	1248	rVB	122	72	0.01%	0.001%
37	5.341	1273	1296	1328	rBV2	293651	880923	100.00%	13.037%
38	5.665	1396	1397	1400	rVB	179	70	0.01%	0.001%
39	5.688	1400	1404	1407	rBV2	195	201	0.02%	0.003%
40	5.714	1407	1412	1420	rBV	88	100	0.01%	0.001%
41	5.749	1421	1423	1426	rBV	164	64	0.01%	0.001%
42	5.765	1426	1428	1431	rBV	120	49	0.01%	0.001%
43	5.778	1431	1432	1434	rBV	96	54	0.01%	0.001%
44	5.887	1451	1466	1503	rBV	270231	543953	61.75%	8.050%
45	6.170	1549	1554	1560	rBV	403	554	0.06%	0.008%
46	6.260	1576	1582	1584	rBV	234	300	0.03%	0.004%
47	6.334	1590	1605	1638	rBV	200838	410596	46.61%	6.076%
48	6.511	1658	1660	1663	rBV	212	170	0.02%	0.003%
49	6.556	1669	1674	1679	rBV2	299	299	0.03%	0.004%
50	6.627	1694	1696	1699	rBV	120	72	0.01%	0.001%
51	6.681	1711	1713	1718	rVB2	220	164	0.02%	0.002%
52	6.794	1746	1748	1751	rBV	181	99	0.01%	0.001%
53	6.826	1757	1758	1761	rVB	110	55	0.01%	0.001%
54	6.855	1761	1767	1769	rBV2	338	356	0.04%	0.005%
55	6.910	1780	1784	1787	rBV2	161	127	0.01%	0.002%
56	6.932	1787	1791	1793	rBV2	212	174	0.02%	0.003%
57	6.945	1793	1795	1798	rVB	181	59	0.01%	0.001%
58	6.971	1798	1803	1804	rBV	165	128	0.01%	0.002%
59	7.006	1811	1814	1817	rBV2	185	134	0.02%	0.002%
60	7.025	1817	1820	1821	rBV	140	88	0.01%	0.001%
61	7.112	1845	1847	1851	rVV2	112	72	0.01%	0.001%
62	7.157	1858	1861	1862	rBV	171	102	0.01%	0.002%
63	7.228	1871	1883	1915	rBV	111147	203220	23.07%	3.007%
64	7.389	1928	1933	1935	rBV3	241	216	0.02%	0.003%
65	7.459	1951	1955	1959	rBV2	204	159	0.02%	0.002%
66	7.485	1960	1963	1964	rBV	176	107	0.01%	0.002%
67	7.566	1975	1988	2020	rBV	375264	672052	76.29%	9.946%
68	7.787	2055	2057	2059	rBV	137	85	0.01%	0.001%
69	7.800	2059	2061	2065	rVB2	181	110	0.01%	0.002%
70	7.852	2065	2077	2099	rBV	78000	135989	15.44%	2.012%
71	8.012	2125	2127	2129	rBV	223	75	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100518\
 Data File : VU027453.D
 Acq On : 05 Oct 2018 15:18
 Operator : MD/SY
 Sample : J5250-03 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0911

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

72	8.048	2134	2138	2141	rBV3	299	229	0.03%	0.003%
73	8.183	2166	2180	2189	rBV4	3091	7464	0.85%	0.110%
74	8.312	2210	2220	2250	rVB	282077	489140	55.53%	7.239%
75	8.627	2315	2318	2320	rBV	149	68	0.01%	0.001%
76	8.707	2340	2343	2344	rBV	136	79	0.01%	0.001%
77	8.787	2366	2368	2371	rBV2	137	82	0.01%	0.001%
78	8.855	2386	2389	2391	rVB	180	97	0.01%	0.001%
79	8.884	2396	2398	2403	rVB2	156	112	0.01%	0.002%
80	8.919	2405	2409	2412	rVB2	167	126	0.01%	0.002%
81	8.938	2412	2415	2418	rBB2	246	140	0.02%	0.002%
82	8.967	2419	2424	2427	rBV2	167	149	0.02%	0.002%
83	9.090	2449	2462	2489	rBV	396142	664183	75.40%	9.829%
84	9.231	2504	2506	2509	rBV2	174	84	0.01%	0.001%
85	9.627	2624	2629	2631	rVB2	171	129	0.01%	0.002%
86	9.762	2668	2671	2675	rVB	307	198	0.02%	0.003%
87	9.784	2675	2678	2681	rBV2	274	182	0.02%	0.003%
88	9.810	2682	2686	2694	rVB2	244	252	0.03%	0.004%
89	10.048	2758	2760	2763	rBV	148	107	0.01%	0.002%
90	10.090	2769	2773	2778	rBV2	252	275	0.03%	0.004%
91	10.170	2795	2798	2800	rBV	263	167	0.02%	0.002%
92	10.234	2815	2818	2822	rBV	295	151	0.02%	0.002%
93	10.321	2838	2845	2849	rBV2	987	1210	0.14%	0.018%
94	10.434	2868	2880	2899	rBV	254410	409531	46.49%	6.061%
95	11.147	3096	3102	3103	rBV	612	439	0.05%	0.006%
96	11.273	3138	3141	3143	rBV	171	111	0.01%	0.002%
97	11.414	3183	3185	3188	rBV2	551	312	0.04%	0.005%
98	11.485	3194	3207	3231	rBV	398000	628134	71.30%	9.296%
99	11.861	3311	3324	3344	rBV	375261	593988	67.43%	8.790%
100	12.466	3510	3512	3513	rBV	476	234	0.03%	0.003%


Sum of corrected areas: 6757299

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100518\
Data File : VU027453.D
Acq On : 05 Oct 2018 15:18
Operator : MD/SY
Sample : J5250-03 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C0911

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

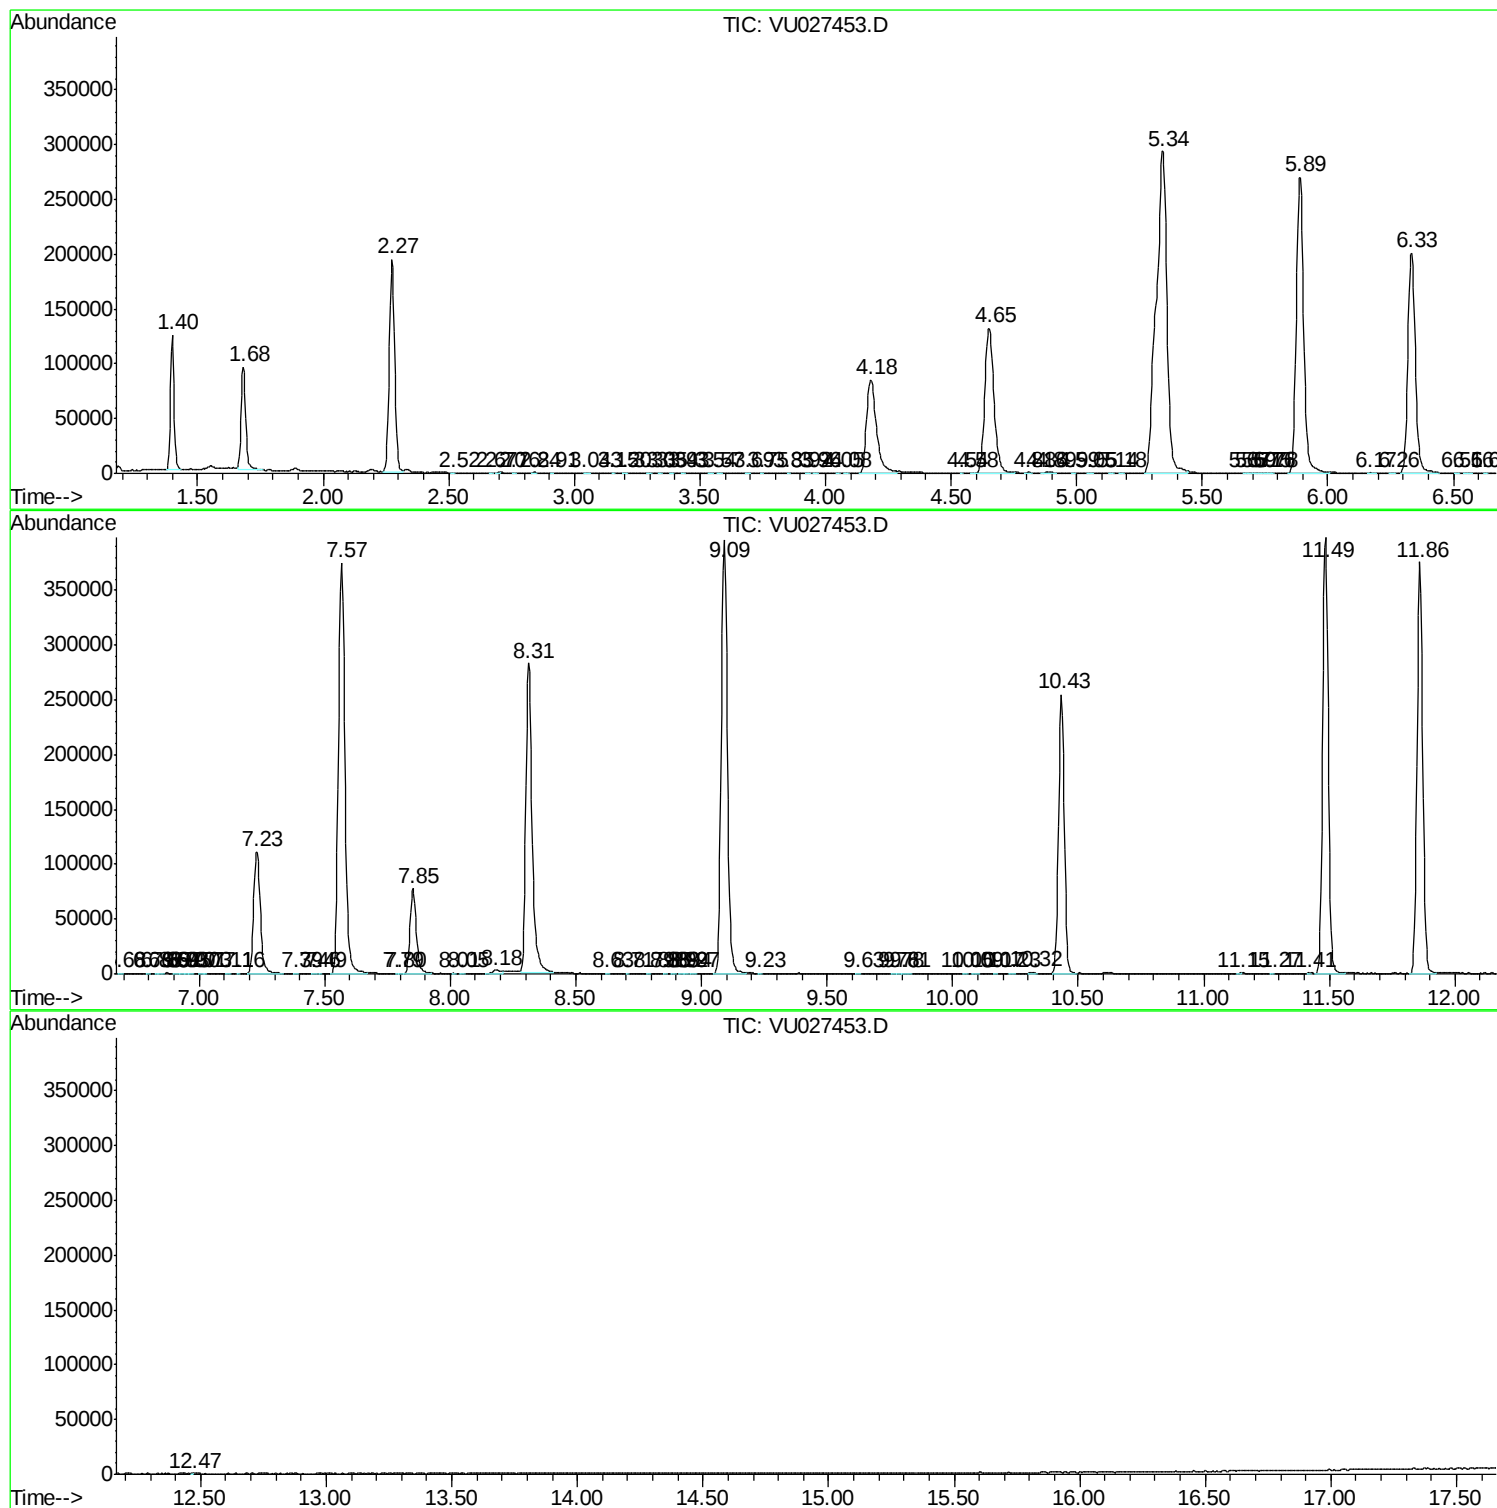

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU100518\
Data File : VU027453.D
Acq On : 05 Oct 2018 15:18
Operator : MD/SY
Sample : J5250-03 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0911

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU100518\
Data File : VU027453.D
Acq On : 05 Oct 2018 15:18
Operator : MD/SY
Sample : J5250-03 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0911

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc