


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100518\
Data File : VU027438.D
Acq On : 05 Oct 2018 07:37
Operator : MD/SY
Sample : BFB46
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB46

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Title : VOC Analysis
Last Update : Tue Oct 09 05:21:41 2018

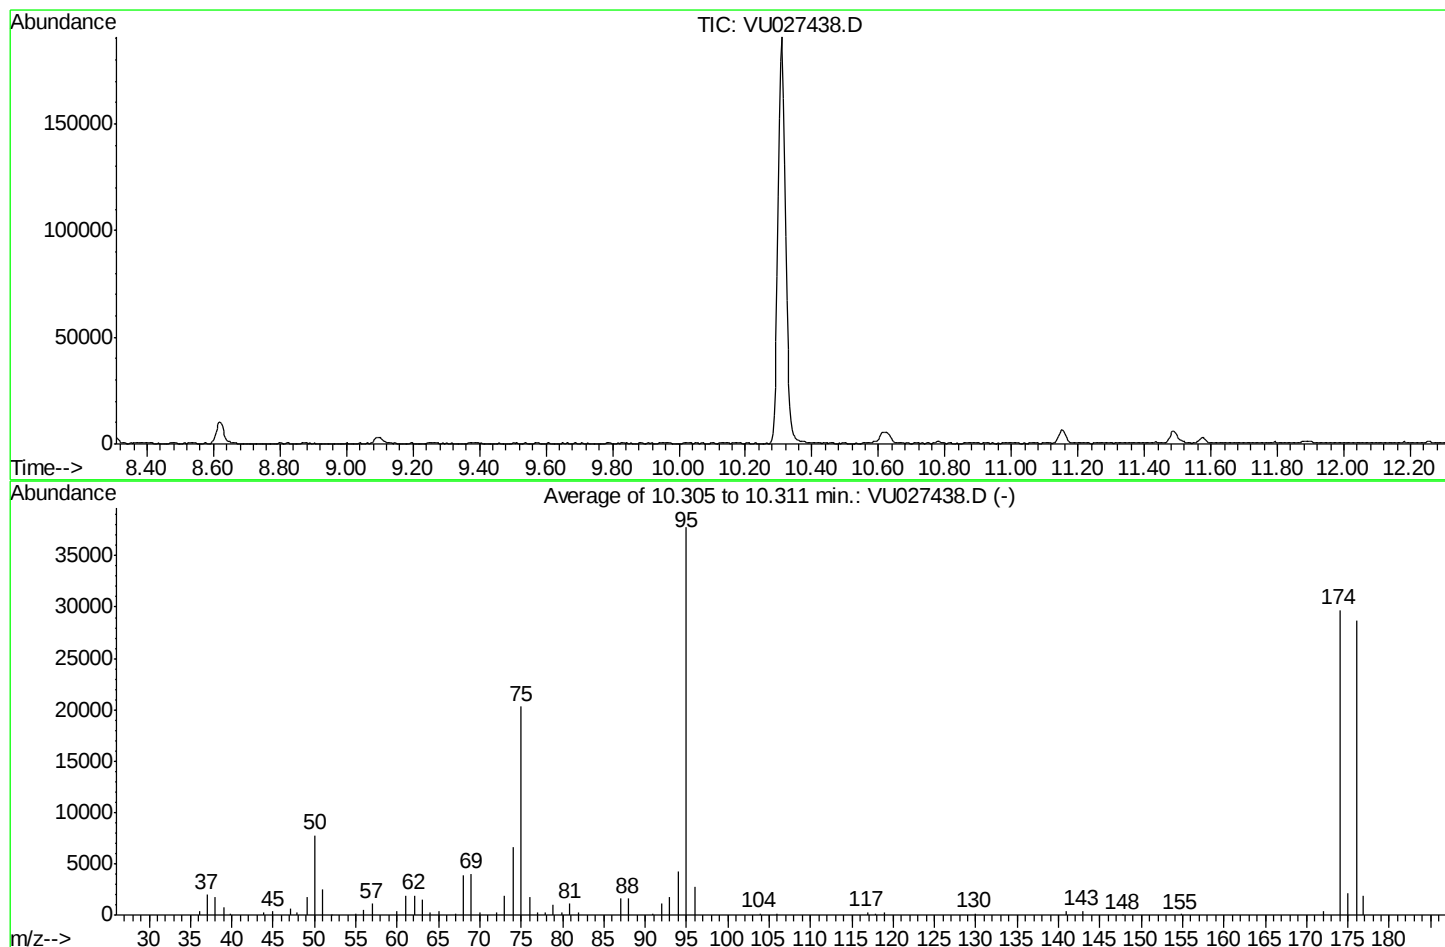

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	7765	PASS
75	95	30	80	53.7	20290	PASS
95	95	100	100	100.0	37773	PASS
96	95	5	9	7.1	2689	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.7	29717	PASS
175	174	5	9	7.2	2140	PASS
176	174	95	101	96.6	28706	PASS
177	176	5	9	6.4	1835	PASS

m/z	Abundance
43.90	305.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.10	385.0
37.00	1887.0
38.00	1760.0
39.00	834.0
39.90	118.0
43.90	535.0
45.00	387.0
47.10	632.0
47.90	240.0
49.00	1731.0
50.10	7532.0
51.00	2550.0
52.00	112.0
56.00	563.0
57.00	1088.0
59.90	400.0
61.00	1829.0
62.00	1858.0
63.00	1418.0
64.10	173.0
65.00	370.0
68.00	3788.0
69.00	3921.0
70.00	319.0
72.00	243.0
73.00	1772.0
74.00	6377.0
75.00	19792.0
76.00	1744.0
77.00	264.0
78.00	186.0
78.90	972.0
80.00	285.0
80.90	1094.0
81.90	254.0
87.00	1569.0
87.90	1487.0
90.90	180.0
92.00	1015.0
93.00	1660.0
94.00	4153.0
95.00	37264.0
96.00	2650.0
103.90	200.0
106.00	166.0
116.90	226.0
117.90	106.0
118.90	260.0
129.90	145.0
140.90	372.0
142.90	379.0
154.90	115.0
172.00	383.0
174.00	28472.0
174.90	1972.0
176.00	27248.0
176.90	1738.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.10	365.0
37.00	2077.0
38.00	1883.0
39.00	860.0
39.90	104.0
43.90	554.0
45.00	389.0
47.00	708.0
47.90	242.0
49.00	1778.0
50.00	8049.0
51.00	2560.0
55.00	100.0
55.90	567.0
57.00	1174.0
60.00	372.0
61.00	1858.0
62.10	1948.0
63.00	1536.0
64.00	204.0
65.00	398.0
67.10	112.0
68.00	3933.0
69.00	4172.0
70.00	296.0
72.00	283.0
73.00	1906.0
74.00	6869.0
75.00	21040.0
76.00	1837.0
77.10	252.0
77.90	251.0
78.90	1078.0
80.00	312.0
80.90	1134.0
81.90	268.0
87.00	1635.0
88.00	1677.0
90.90	176.0
92.00	1131.0
93.00	1734.0
94.00	4385.0
95.00	38864.0
96.00	2769.0
103.90	194.0
106.00	190.0
116.90	266.0
117.90	144.0
118.90	243.0
129.90	123.0
140.90	419.0
142.90	413.0
154.90	130.0
172.00	373.0
174.00	30744.0
175.00	2197.0
176.00	29592.0
176.90	1895.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	326.0
37.00	1993.0
38.00	1796.0
39.00	747.0
39.90	102.0
44.00	508.0
44.90	339.0
47.00	716.0
47.90	221.0
49.10	1699.0
50.00	7716.0
51.00	2334.0
54.90	117.0
55.90	543.0
57.00	1084.0
60.00	345.0
61.00	1766.0
62.10	1842.0
63.00	1493.0
64.00	218.0
65.00	396.0
66.90	120.0
68.00	3851.0
69.00	4020.0
70.00	241.0
72.10	253.0
73.00	1795.0
74.00	6726.0
75.00	20040.0
76.00	1790.0
77.00	235.0
77.90	252.0
78.90	1022.0
79.90	298.0
80.90	1002.0
81.90	234.0
87.00	1548.0
88.00	1669.0
90.90	139.0
92.00	1128.0
93.00	1719.0
94.00	4303.0
95.00	37192.0
96.00	2649.0
103.90	181.0
106.00	170.0
116.90	275.0
117.90	141.0
118.90	220.0
129.80	110.0
140.90	419.0
142.90	445.0
147.80	103.0
154.80	109.0
172.00	342.0
174.00	29936.0
175.00	2252.0
176.00	29280.0
176.90	1872.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46