

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U100520\
 Data File : VU040513.D
 Acq On : 05 Oct 2020 16:31
 Operator : SY/MD
 Sample : L4266-01DL 200X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFS99DL

Quant Time: Oct 06 08:53:35 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 06 07:45:27 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	106336	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	109444	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	47875	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	28337	5.38	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.60%
7) Chloroethane-d5	1.92	69	24718	5.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	107.20%
11) 1,1-Dichloroethene-d2	2.58	63	46226	3.65	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.00%
20) 2-Butanone-d5	4.65	46	127292	48.68	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.36%
24) Chloroform-d	5.08	84	62032	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
26) 1,2-Dichloroethane-d4	5.72	65	40783	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.80%
32) Benzene-d6	5.74	84	116801	5.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.20%
36) 1,2-Dichloropropane-d6	6.70	67	40683	5.05	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.00%
41) Toluene-d8	7.91	98	93026	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
43) trans-1,3-Dichloropropene-	8.19	79	16240	4.94	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.80%
46) 2-Hexanone-d5	8.64	63	92598	47.93	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.86%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	37993	4.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.00%
64) 1,2-Dichlorobenzene-d4	12.19	152	39126	5.39	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.80%


Target Compounds					Ovalue
47) Tetrachloroethene	8.56	164	199490	28.842 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100520\
Data File : VU040513.D
Acq On : 05 Oct 2020 16:31
Operator : SY/MD
Sample : L4266-01DL 200X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFS99DL

Quant Time: Oct 06 08:53:35 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR092920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 06 07:45:27 2020
Response via : Initial Calibration

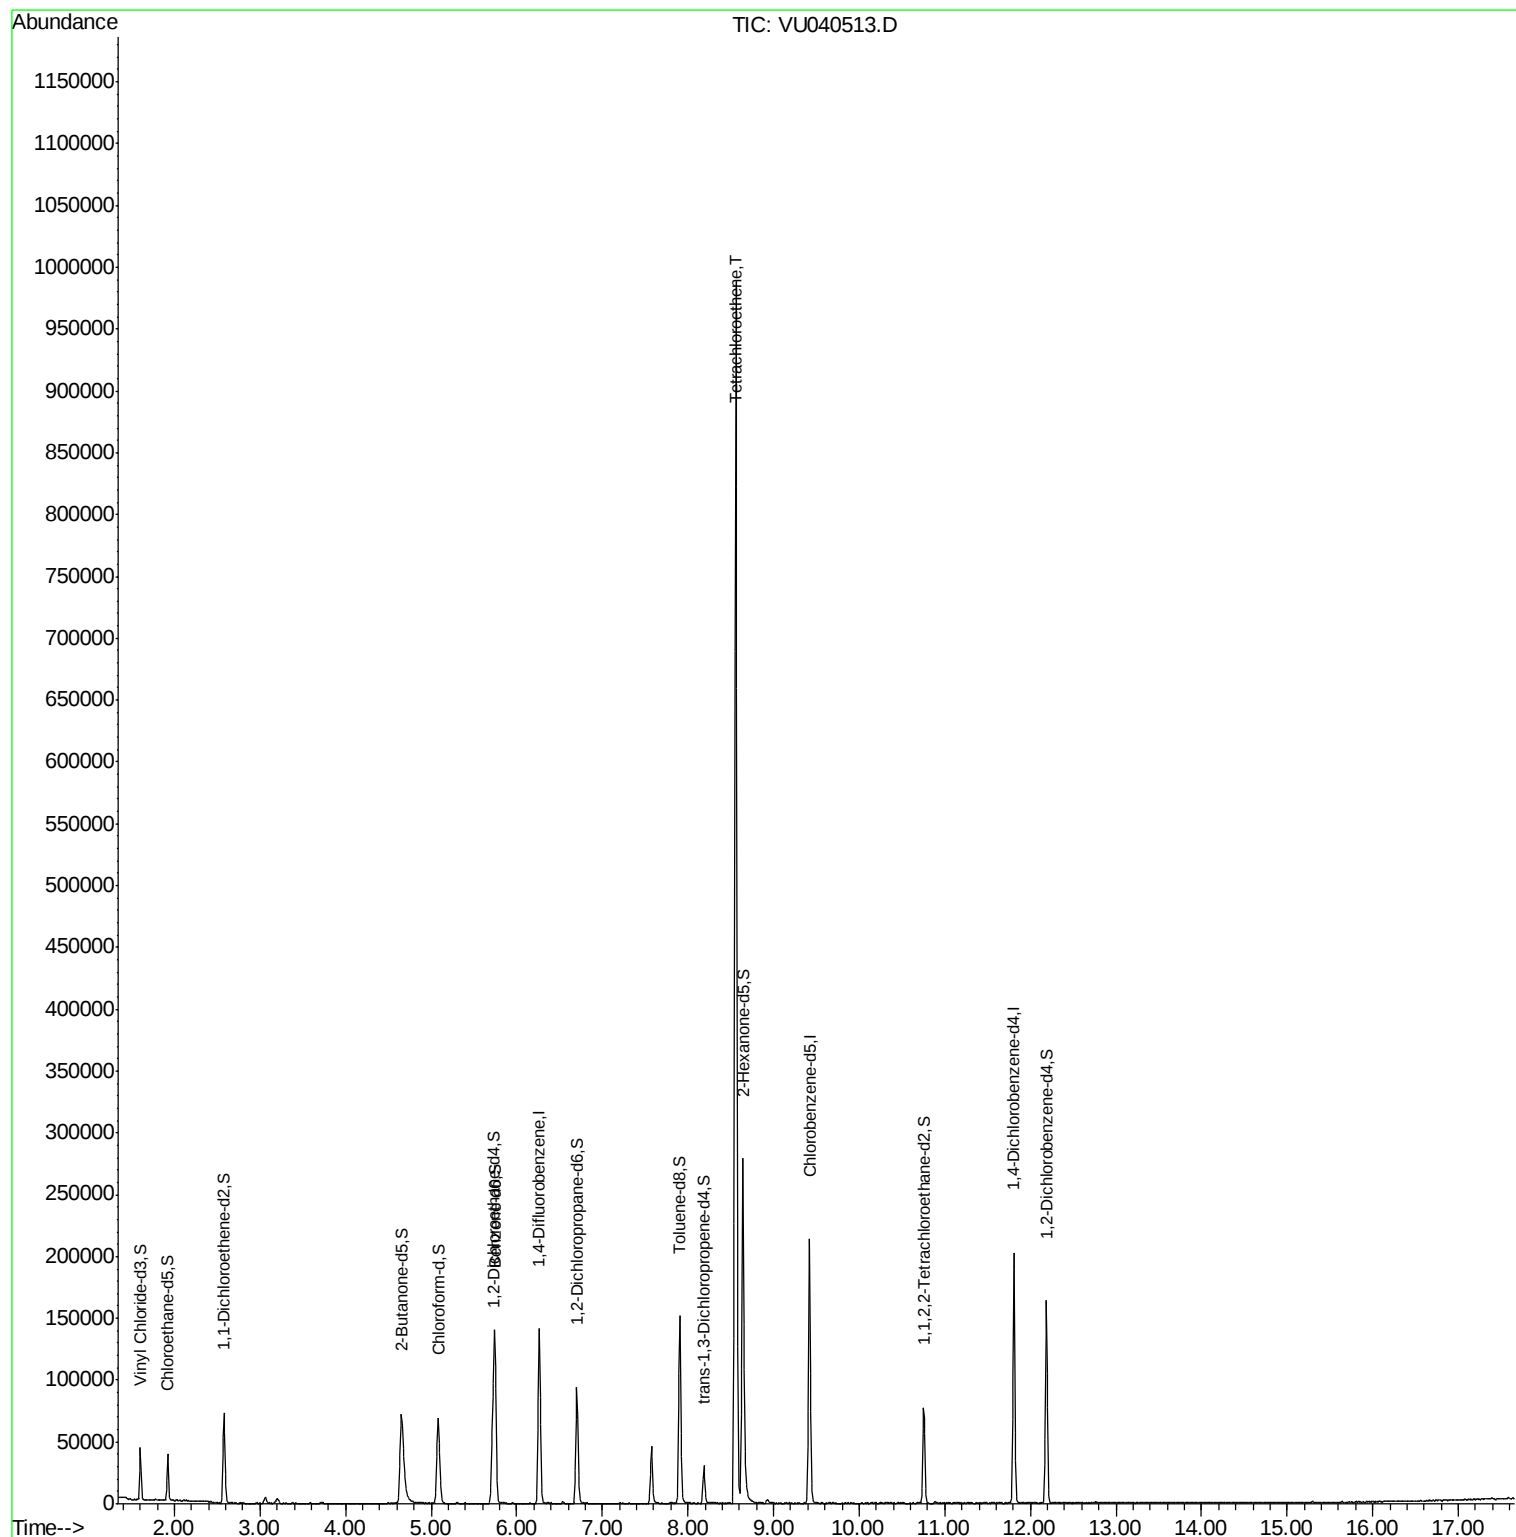

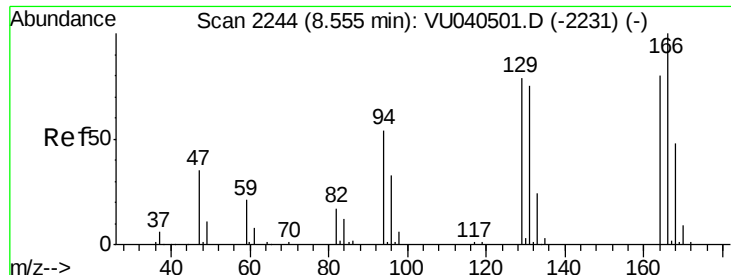

#47

Tetrachloroethene

Concen: 28.842 ug/L

RT: 8.56 min Scan# 2245

Delta R.T. 0.00 min

Lab File: VU040513.D

Acq: 05 Oct 2020 16:31

Instrument :

MSVOA_U

ClientSampleId :

BFS99DL

Tot Ion:164 Resp: 199490


Ion Ratio Lower Upper

164 100

129 101.0 70.3 130.7

131 97.6 69.2 128.6

166 129.2 91.1 169.3

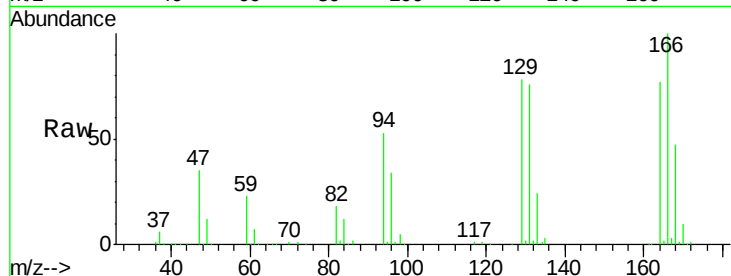

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

