

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045151.D
 Acq On : 05 Oct 2021 17:44
 Operator : SY/MD
 Sample : M4025-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	95	rBV	160412	188343	14.01%	1.763%
2	1.912	169	178	192	rVB	135694	187645	13.96%	1.757%
3	2.482	349	355	359	rBV2	254	320	0.02%	0.003%
4	2.572	370	383	401	rBV2	278919	474440	35.29%	4.442%
5	2.691	417	420	427	rVB2	180	221	0.02%	0.002%
6	2.777	441	447	448	rBV	279	261	0.02%	0.002%
7	2.906	485	487	493	rVB	230	191	0.01%	0.002%
8	2.948	494	500	502	rBV2	333	367	0.03%	0.003%
9	2.961	502	504	511	rVB	454	471	0.04%	0.004%
10	3.051	518	532	554	rBV	55172	107675	8.01%	1.008%
11	3.189	571	575	587	rVB3	761	1364	0.10%	0.013%
12	3.253	592	595	600	rVB2	165	185	0.01%	0.002%
13	3.298	606	609	615	rBV2	190	244	0.02%	0.002%
14	3.363	620	629	637	rBV2	2376	4232	0.31%	0.040%
15	3.578	692	696	700	rBV2	208	167	0.01%	0.002%
16	3.719	737	740	744	rVB2	236	179	0.01%	0.002%
17	3.803	760	766	771	rVB	279	286	0.02%	0.003%
18	3.871	783	787	788	rBV	520	310	0.02%	0.003%
19	4.083	850	853	857	rBV2	230	184	0.01%	0.002%
20	4.330	926	930	933	rVB2	192	173	0.01%	0.002%
21	4.440	956	964	966	rBV2	304	354	0.03%	0.003%
22	4.472	969	974	978	rBV	225	240	0.02%	0.002%
23	4.633	1003	1024	1057	rBV2	149837	464864	34.57%	4.352%
24	4.854	1089	1093	1096	rBV2	301	258	0.02%	0.002%
25	4.909	1108	1110	1118	rVB2	271	315	0.02%	0.003%
26	4.970	1126	1129	1134	rBV2	224	217	0.02%	0.002%
27	5.070	1140	1160	1190	rBV	236998	521738	38.80%	4.885%
28	5.176	1190	1193	1196	rVB2	320	169	0.01%	0.002%
29	5.195	1196	1199	1203	rVB	266	187	0.01%	0.002%
30	5.224	1203	1208	1211	rBV2	455	366	0.03%	0.003%
31	5.321	1224	1238	1252	rVB2	10877	23737	1.77%	0.222%
32	5.375	1252	1255	1258	rBV	341	284	0.02%	0.003%
33	5.436	1270	1274	1280	rVB	144	213	0.02%	0.002%
34	5.729	1343	1365	1387	rBV2	496070	1344551	100.00%	12.588%
35	6.047	1459	1464	1469	rVV2	291	402	0.03%	0.004%
36	6.144	1492	1494	1499	rBV	303	306	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045151.D
 Acq On : 05 Oct 2021 17:44
 Operator : SY/MD
 Sample : M4025-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.253	1512	1528	1550	rBV	394024	745415	55.44%	6.979%
38	6.427	1578	1582	1586	rBV2	255	279	0.02%	0.003%
39	6.462	1590	1593	1603	rVV3	424	588	0.04%	0.006%
40	6.546	1605	1619	1636	rVV	123040	235955	17.55%	2.209%
41	6.623	1641	1643	1648	rVB	243	173	0.01%	0.002%
42	6.697	1648	1666	1688	rBV	317262	616044	45.82%	5.768%
43	6.796	1695	1697	1698	rBV	456	187	0.01%	0.002%
44	6.841	1708	1711	1715	rBV2	273	185	0.01%	0.002%
45	6.864	1715	1718	1721	rBV2	207	170	0.01%	0.002%
46	6.999	1754	1760	1763	rBV	203	219	0.02%	0.002%
47	7.157	1804	1809	1810	rBV2	220	196	0.01%	0.002%
48	7.186	1810	1818	1829	rVB3	1933	3233	0.24%	0.030%
49	7.311	1851	1857	1859	rBV2	226	263	0.02%	0.002%
50	7.478	1906	1909	1913	rVB	179	166	0.01%	0.002%
51	7.571	1924	1938	1958	rBV	175482	308126	22.92%	2.885%
52	7.903	2027	2041	2056	rBV	613225	1044051	77.65%	9.775%
53	7.973	2057	2063	2079	rVB2	8959	16224	1.21%	0.152%
54	8.128	2106	2111	2115	rBV2	203	278	0.02%	0.003%
55	8.182	2115	2128	2149	rBV	123687	206608	15.37%	1.934%
56	8.472	2214	2218	2221	rBV2	193	214	0.02%	0.002%
57	8.533	2234	2237	2240	rVV2	261	209	0.02%	0.002%
58	8.555	2240	2244	2251	rVB3	978	903	0.07%	0.008%
59	8.639	2257	2270	2306	rBV	460740	807036	60.02%	7.556%
60	8.893	2343	2349	2351	rBV	266	297	0.02%	0.003%
61	9.317	2477	2481	2485	rBV2	207	246	0.02%	0.002%
62	9.366	2490	2496	2500	rBV2	190	303	0.02%	0.003%
63	9.420	2500	2513	2533	rBV	550213	910226	67.70%	8.522%
64	9.571	2555	2560	2564	rBV3	308	343	0.03%	0.003%
65	9.629	2575	2578	2584	rBV2	204	281	0.02%	0.003%
66	9.668	2586	2590	2593	rBV2	167	169	0.01%	0.002%
67	9.693	2593	2598	2599	rBV2	706	480	0.04%	0.004%
68	9.841	2640	2644	2645	rBV2	194	161	0.01%	0.002%
69	9.883	2654	2657	2662	rBV2	195	201	0.01%	0.002%
70	9.919	2662	2668	2671	rVB2	205	238	0.02%	0.002%
71	9.957	2676	2680	2683	rBV	261	236	0.02%	0.002%
72	10.102	2722	2725	2733	rVB2	250	334	0.02%	0.003%
73	10.163	2741	2744	2748	rBV	147	165	0.01%	0.002%
74	10.243	2765	2769	2773	rBV2	224	254	0.02%	0.002%
75	10.359	2800	2805	2807	rBV2	234	264	0.02%	0.002%
76	10.472	2838	2840	2845	rVB2	221	203	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045151.D
 Acq On : 05 Oct 2021 17:44
 Operator : SY/MD
 Sample : M4025-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.674	2894	2903	2911	rVV2	3480	5106	0.38%	0.048%
78	10.761	2917	2930	2948	rBV	432248	694264	51.64%	6.500%
79	10.867	2958	2963	2969	rBV2	575	832	0.06%	0.008%
80	11.002	3002	3005	3012	rVB3	403	472	0.04%	0.004%
81	11.041	3012	3017	3020	rBV	174	208	0.02%	0.002%
82	11.124	3039	3043	3046	rBV	532	438	0.03%	0.004%
83	11.189	3058	3063	3065	rBV2	180	205	0.02%	0.002%
84	11.462	3139	3148	3160	rVB4	2070	3707	0.28%	0.035%
85	11.578	3180	3184	3185	rBV	297	226	0.02%	0.002%
86	11.639	3198	3203	3208	rVB2	900	887	0.07%	0.008%
87	11.697	3215	3221	3230	rVB2	1337	1918	0.14%	0.018%
88	11.816	3244	3258	3283	rBV	535189	838804	62.39%	7.853%
89	11.947	3294	3299	3302	rBV3	770	781	0.06%	0.007%
90	12.195	3360	3376	3395	rBV	554847	903789	67.22%	8.462%
91	12.333	3415	3419	3422	rBV4	440	365	0.03%	0.003%
92	12.806	3561	3566	3569	rBV2	252	287	0.02%	0.003%
93	12.941	3605	3608	3611	rBV	300	217	0.02%	0.002%
94	13.652	3827	3829	3833	rBV2	220	181	0.01%	0.002%
95	13.857	3889	3893	3897	rBV	311	361	0.03%	0.003%
96	13.992	3932	3935	3941	rVB2	373	376	0.03%	0.004%
97	14.025	3941	3945	3946	rBV	215	176	0.01%	0.002%
98	14.102	3963	3969	3973	rBV2	420	485	0.04%	0.005%
99	14.269	4018	4021	4024	rBV2	270	237	0.02%	0.002%
100	14.796	4180	4185	4186	rBV3	248	235	0.02%	0.002%




Sum of corrected areas: 10681139

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045151.D
Acq On : 05 Oct 2021 17:44
Operator : SY/MD
Sample : M4025-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

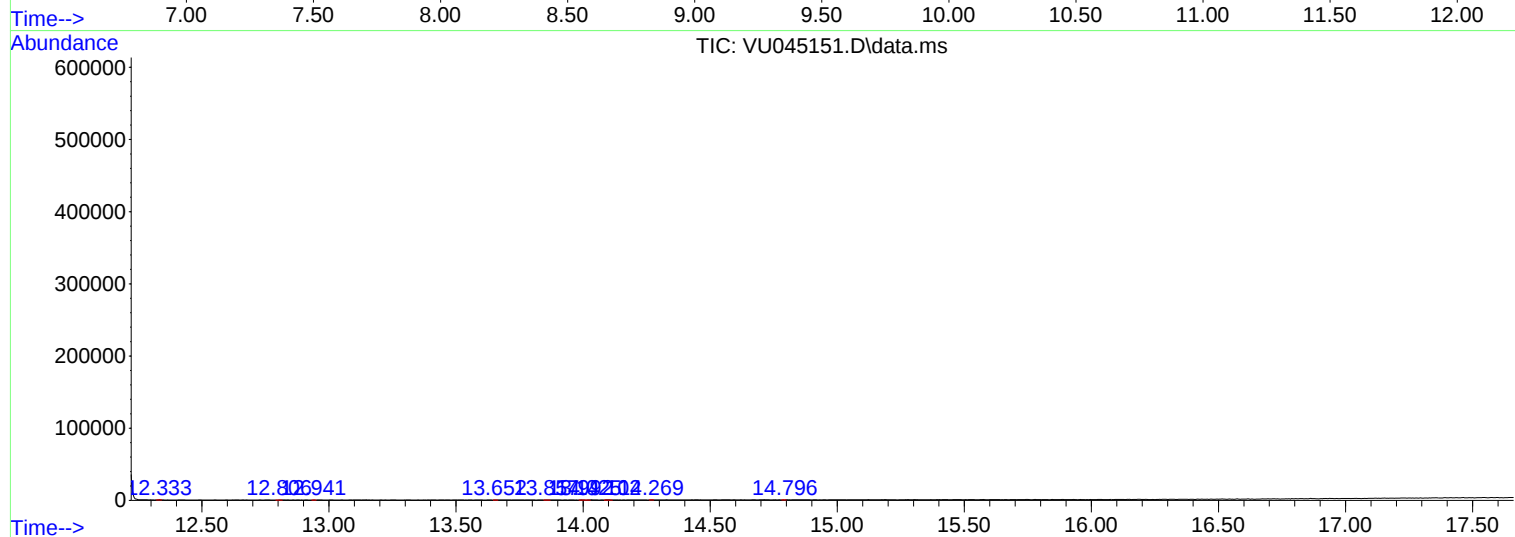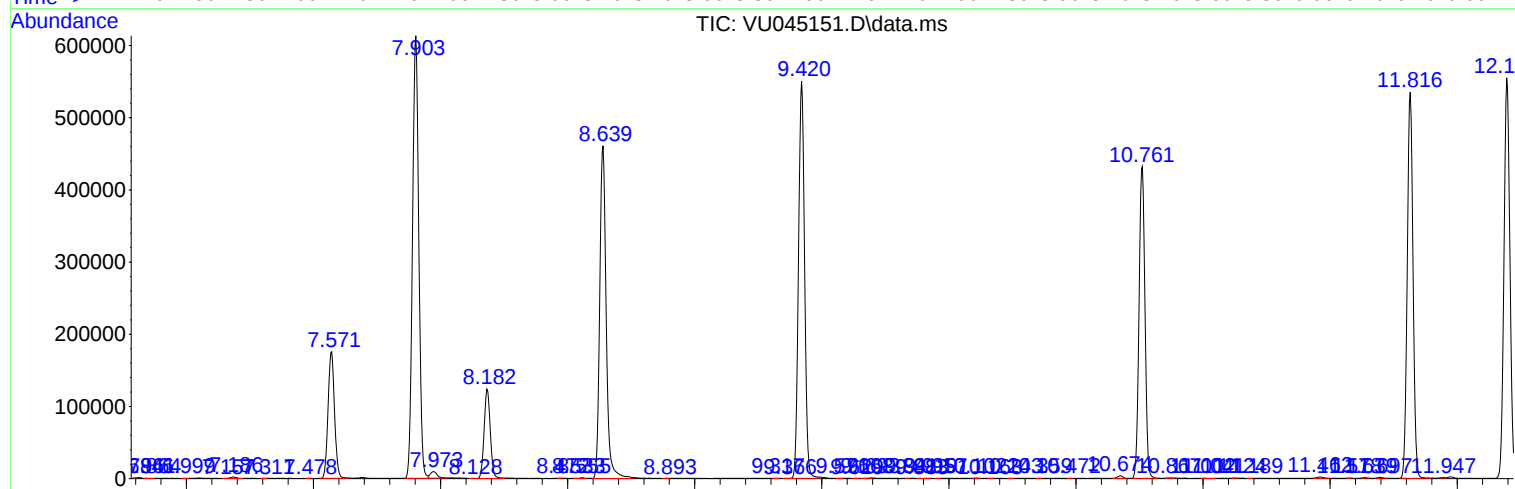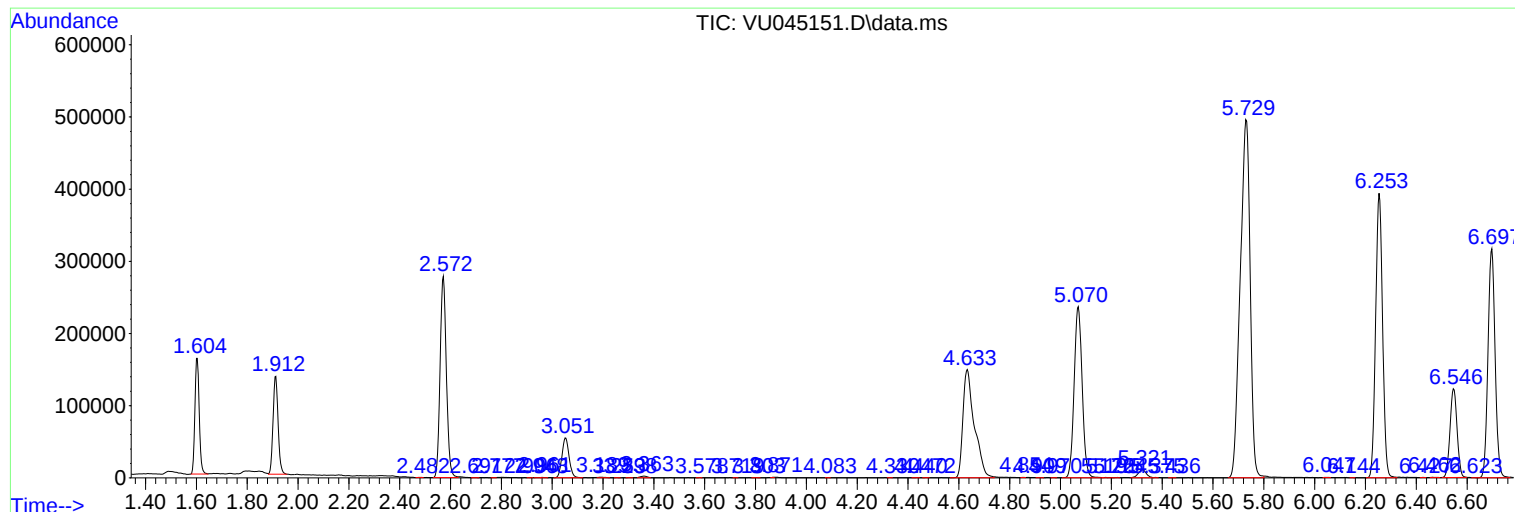

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045151.D
Acq On : 05 Oct 2021 17:44
Operator : SY/MD
Sample : M4025-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045151.D
Acq On : 05 Oct 2021 17:44
Operator : SY/MD
Sample : M4025-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
