

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045153.D
 Acq On : 05 Oct 2021 18:30
 Operator : SY/MD
 Sample : M4025-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045153.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	97	rBV	162713	185611	14.01%	1.854%
2	1.913	169	178	195	rVB	134248	184707	13.94%	1.845%
3	2.572	370	383	400	rBV	270501	450956	34.04%	4.505%
4	2.729	428	432	436	rBV2	285	233	0.02%	0.002%
5	2.768	439	444	447	rBV2	161	166	0.01%	0.002%
6	2.800	447	454	462	rVB3	785	1287	0.10%	0.013%
7	2.842	462	467	471	rBV2	248	226	0.02%	0.002%
8	2.900	480	485	488	rBV2	221	204	0.02%	0.002%
9	2.958	498	503	508	rBV2	395	472	0.04%	0.005%
10	3.048	526	531	537	rBV2	611	579	0.04%	0.006%
11	3.183	570	573	575	rVV2	320	255	0.02%	0.003%
12	3.199	576	578	584	rVB3	508	411	0.03%	0.004%
13	3.250	590	594	601	rBV2	191	271	0.02%	0.003%
14	3.372	627	632	636	rBV	260	279	0.02%	0.003%
15	3.398	638	640	643	rBV2	248	180	0.01%	0.002%
16	3.434	647	651	655	rBV2	210	218	0.02%	0.002%
17	3.508	670	674	678	rBV2	201	222	0.02%	0.002%
18	3.565	688	692	695	rBV2	192	147	0.01%	0.001%
19	4.003	824	828	836	rBV	213	158	0.01%	0.002%
20	4.067	843	848	851	rBV2	208	150	0.01%	0.001%
21	4.083	851	853	858	rVB2	199	146	0.01%	0.001%
22	4.115	858	863	866	rBV	179	191	0.01%	0.002%
23	4.173	877	881	891	rBV2	552	983	0.07%	0.010%
24	4.279	911	914	920	rBV2	138	152	0.01%	0.002%
25	4.630	1008	1023	1059	rBV	152352	379421	28.64%	3.790%
26	4.942	1117	1120	1125	rBV2	156	182	0.01%	0.002%
27	5.070	1143	1160	1189	rVV	235840	515502	38.91%	5.150%
28	5.295	1227	1230	1235	rVB2	524	518	0.04%	0.005%
29	5.360	1245	1250	1251	rBV2	247	223	0.02%	0.002%
30	5.372	1251	1254	1257	rVV3	243	205	0.02%	0.002%
31	5.549	1304	1309	1312	rVB	180	158	0.01%	0.002%
32	5.569	1312	1315	1320	rBV2	181	208	0.02%	0.002%
33	5.729	1342	1365	1389	rBV2	492385	1324758	100.00%	13.234%
34	5.839	1396	1399	1403	rVB3	487	361	0.03%	0.004%
35	5.929	1424	1427	1431	rVB2	246	155	0.01%	0.002%
36	6.118	1481	1486	1488	rBV3	269	277	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045153.D
 Acq On : 05 Oct 2021 18:30
 Operator : SY/MD
 Sample : M4025-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.253	1513	1528	1547	rBV	379718	712208	53.76%	7.115%
38	6.540	1606	1617	1626	rVB8	4701	8972	0.68%	0.090%
39	6.697	1651	1666	1690	rBV	311478	607407	45.85%	6.068%
40	6.806	1694	1700	1707	rVB4	940	1223	0.09%	0.012%
41	7.054	1767	1777	1787	rBV3	577	1184	0.09%	0.012%
42	7.183	1810	1817	1830	rVB	1829	3159	0.24%	0.032%
43	7.305	1851	1855	1857	rBV	154	151	0.01%	0.002%
44	7.472	1902	1907	1911	rBV2	233	241	0.02%	0.002%
45	7.568	1924	1937	1958	rBV	171175	301605	22.77%	3.013%
46	7.687	1969	1974	1986	rVB3	1729	2749	0.21%	0.027%
47	7.739	1986	1990	1995	rBV2	326	408	0.03%	0.004%
48	7.842	2019	2022	2027	rVB2	181	167	0.01%	0.002%
49	7.903	2027	2041	2056	rBV	597592	1031073	77.83%	10.300%
50	7.974	2057	2063	2074	rVB	9274	15207	1.15%	0.152%
51	8.183	2116	2128	2145	rBV	121697	201412	15.20%	2.012%
52	8.552	2237	2243	2244	rBV	634	478	0.04%	0.005%
53	8.591	2250	2255	2257	rBV2	312	275	0.02%	0.003%
54	8.639	2257	2270	2303	rBV	460667	803894	60.68%	8.030%
55	8.848	2331	2335	2339	rBV	253	205	0.02%	0.002%
56	9.420	2500	2513	2541	rBV	528694	871182	65.76%	8.703%
57	9.694	2592	2598	2606	rVB2	890	1378	0.10%	0.014%
58	9.800	2626	2631	2636	rBV2	221	250	0.02%	0.002%
59	10.099	2718	2724	2730	rVB3	345	432	0.03%	0.004%
60	10.182	2749	2750	2756	rVB2	177	155	0.01%	0.002%
61	10.211	2756	2759	2762	rBV2	175	183	0.01%	0.002%
62	10.260	2771	2774	2777	rVB2	257	187	0.01%	0.002%
63	10.350	2799	2802	2805	rBV2	191	145	0.01%	0.001%
64	10.401	2814	2818	2820	rBV2	235	193	0.01%	0.002%
65	10.527	2850	2857	2862	rBV2	252	348	0.03%	0.003%
66	10.565	2866	2869	2874	rBV2	135	165	0.01%	0.002%
67	10.674	2894	2903	2911	rVB4	2933	4169	0.31%	0.042%
68	10.758	2916	2929	2957	rVB	421584	684505	51.67%	6.838%
69	10.867	2958	2963	2967	rBV2	610	596	0.04%	0.006%
70	10.977	2989	2997	3000	rBV2	271	361	0.03%	0.004%
71	11.070	3024	3026	3035	rVB2	321	434	0.03%	0.004%
72	11.125	3035	3043	3047	rBV3	797	957	0.07%	0.010%
73	11.205	3066	3068	3075	rVB2	314	264	0.02%	0.003%
74	11.337	3105	3109	3115	rVB2	229	253	0.02%	0.003%
75	11.372	3116	3120	3122	rBV2	171	142	0.01%	0.001%
76	11.398	3125	3128	3130	rBV	265	210	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045153.D
 Acq On : 05 Oct 2021 18:30
 Operator : SY/MD
 Sample : M4025-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.459	3139	3147	3158	rVB5	1684	3128	0.24%	0.031%
78	11.555	3173	3177	3179	rBV2	168	154	0.01%	0.002%
79	11.636	3196	3202	3210	rVB3	1595	2323	0.18%	0.023%
80	11.690	3215	3219	3221	rBV3	838	629	0.05%	0.006%
81	11.816	3244	3258	3284	rBV	501185	797643	60.21%	7.968%
82	11.944	3291	3298	3302	rBV4	1135	1435	0.11%	0.014%
83	11.980	3306	3309	3316	rVB3	1705	1660	0.13%	0.017%
84	12.012	3316	3319	3323	rBV	158	157	0.01%	0.002%
85	12.070	3333	3337	3339	rBV2	277	251	0.02%	0.003%
86	12.195	3362	3376	3396	rBV	550031	890422	67.21%	8.895%
87	12.337	3415	3420	3425	rBV3	557	454	0.03%	0.005%
88	12.407	3438	3442	3445	rBV2	322	279	0.02%	0.003%
89	12.465	3458	3460	3463	rBV	228	140	0.01%	0.001%
90	12.491	3465	3468	3471	rBV	191	178	0.01%	0.002%
91	13.147	3670	3672	3678	rVB2	290	224	0.02%	0.002%
92	13.729	3848	3853	3862	rBV2	337	580	0.04%	0.006%
93	13.803	3873	3876	3880	rBV2	287	325	0.02%	0.003%
94	13.838	3882	3887	3892	rVV2	192	284	0.02%	0.003%
95	14.134	3976	3979	3981	rBV	269	160	0.01%	0.002%
96	14.250	4013	4015	4021	rBV2	335	359	0.03%	0.004%
97	14.385	4054	4057	4060	rVB2	323	214	0.02%	0.002%
98	14.813	4188	4190	4194	rBV2	234	153	0.01%	0.002%
99	15.131	4286	4289	4294	rBV3	328	328	0.02%	0.003%
100	15.510	4405	4407	4415	rVB	345	378	0.03%	0.004%


Sum of corrected areas: 10010557

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045153.D
Acq On : 05 Oct 2021 18:30
Operator : SY/MD
Sample : M4025-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

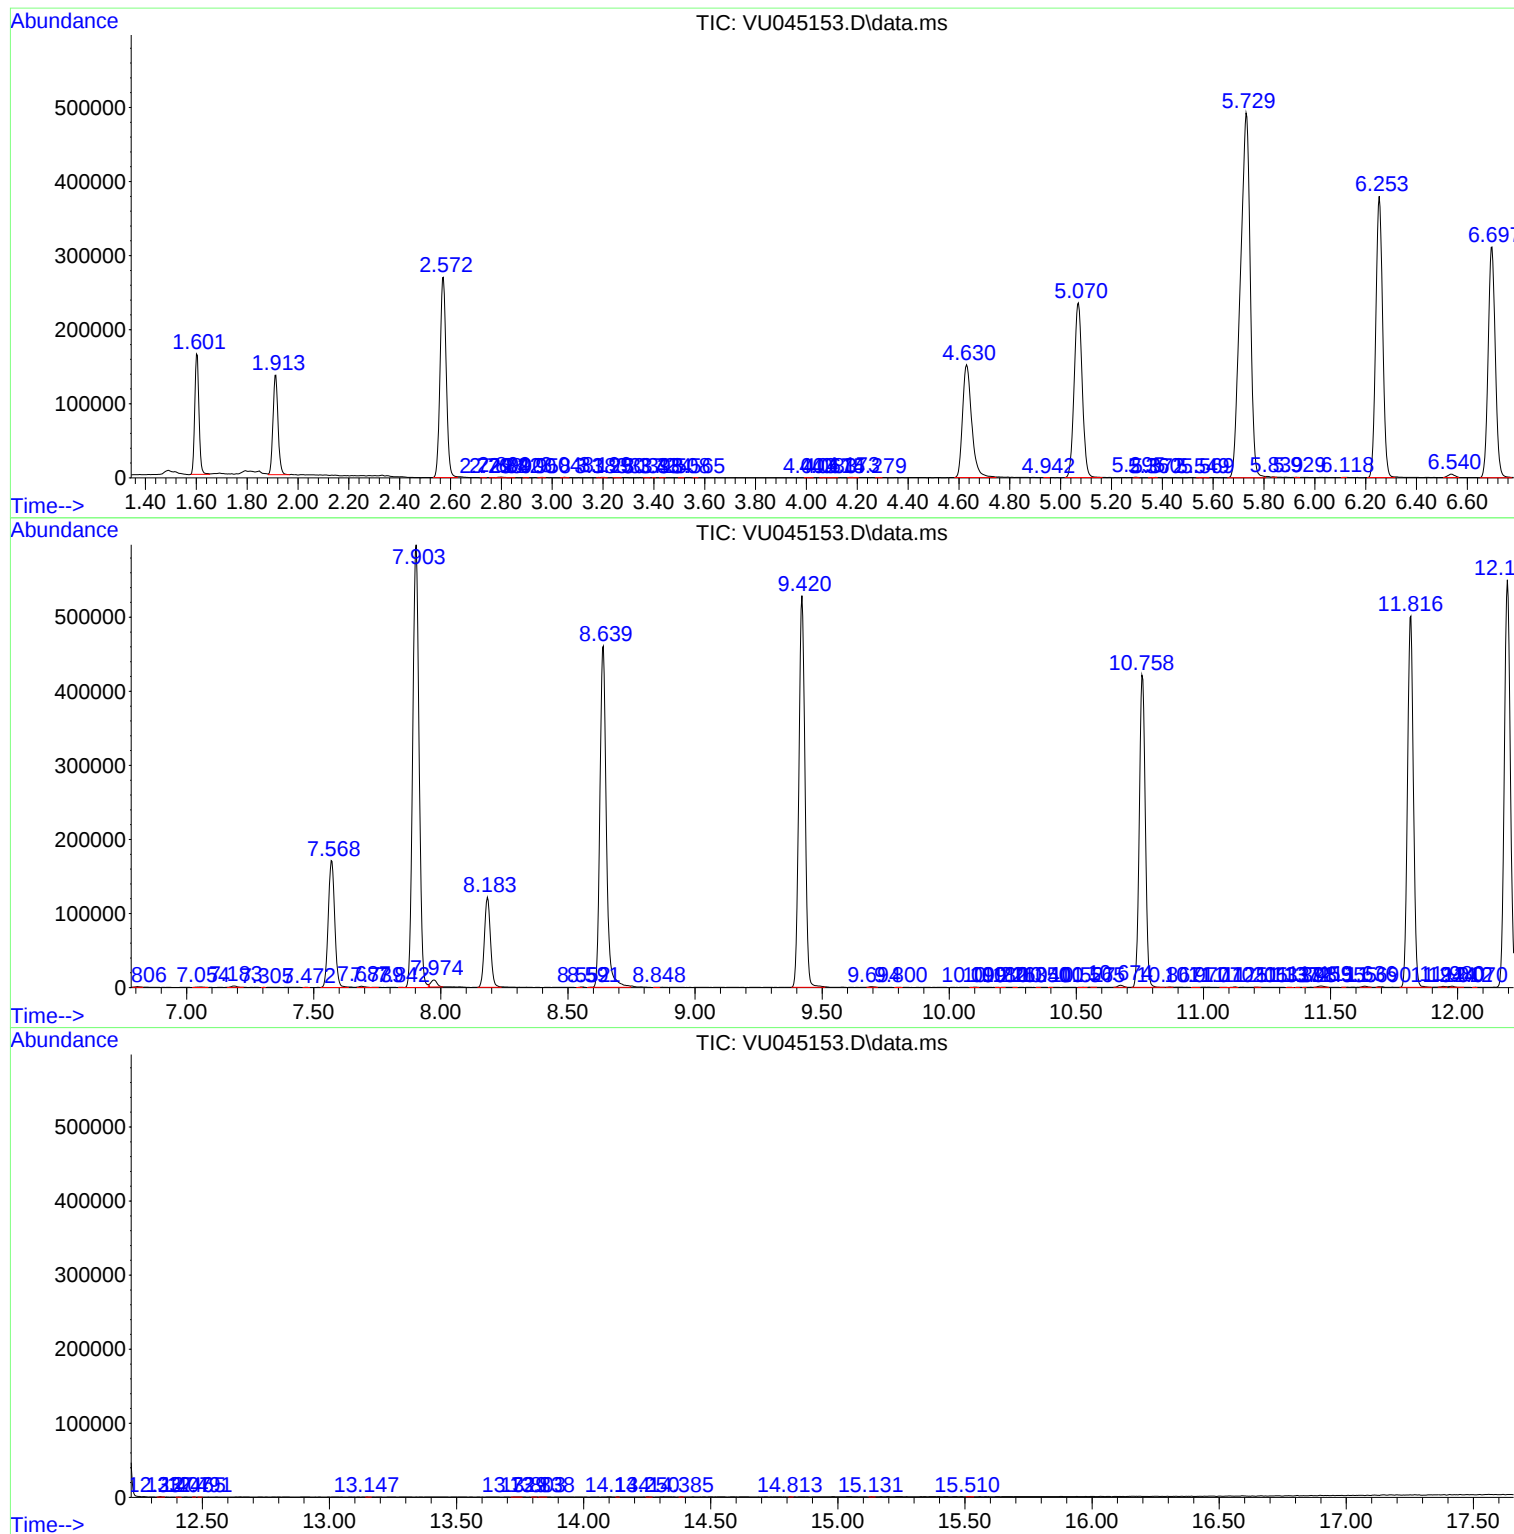

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045153.D
Acq On : 05 Oct 2021 18:30
Operator : SY/MD
Sample : M4025-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045153.D
Acq On : 05 Oct 2021 18:30
Operator : SY/MD
Sample : M4025-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
