

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045154.D
 Acq On : 05 Oct 2021 18:54
 Operator : SY/MD
 Sample : M4025-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU045154.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	94	rBV	159403	183581	13.93%	1.814%
2	1.912	169	178	194	rVB	135435	182753	13.86%	1.806%
3	2.571	370	383	398	rBV	270512	446589	33.88%	4.413%
4	2.787	437	450	477	rBV	8473	31275	2.37%	0.309%
5	2.912	486	489	492	rBV3	325	219	0.02%	0.002%
6	2.954	498	502	503	rBV	194	135	0.01%	0.001%
7	3.047	526	531	539	rVB4	858	1246	0.09%	0.012%
8	3.192	558	576	597	rBV	26743	65071	4.94%	0.643%
9	3.449	654	656	659	rBV	189	129	0.01%	0.001%
10	3.845	774	779	781	rBV	126	135	0.01%	0.001%
11	3.922	800	803	808	rVB	256	229	0.02%	0.002%
12	3.967	811	817	820	rBV2	117	133	0.01%	0.001%
13	4.009	823	830	835	rBV2	246	391	0.03%	0.004%
14	4.063	843	847	852	rVB	292	223	0.02%	0.002%
15	4.089	852	855	856	rBV2	199	136	0.01%	0.001%
16	4.192	883	887	888	rBV	189	158	0.01%	0.002%
17	4.237	896	901	902	rBV	204	185	0.01%	0.002%
18	4.520	985	989	994	rBV	219	290	0.02%	0.003%
19	4.632	1007	1024	1065	rBV	166173	439054	33.31%	4.339%
20	4.948	1118	1122	1123	rBV	168	151	0.01%	0.001%
21	5.002	1136	1139	1142	rVB2	261	186	0.01%	0.002%
22	5.070	1142	1160	1182	rBV	234171	511316	38.79%	5.053%
23	5.205	1197	1202	1206	rBV2	358	325	0.02%	0.003%
24	5.224	1206	1208	1210	rBV	221	134	0.01%	0.001%
25	5.321	1236	1238	1241	rVB	222	142	0.01%	0.001%
26	5.343	1241	1245	1246	rBV2	207	143	0.01%	0.001%
27	5.375	1253	1255	1259	rVB2	306	203	0.02%	0.002%
28	5.533	1301	1304	1308	rBV2	195	160	0.01%	0.002%
29	5.555	1308	1311	1315	rVB2	151	129	0.01%	0.001%
30	5.732	1342	1366	1392	rBV2	485393	1318089	100.00%	13.025%
31	6.140	1490	1493	1496	rVB2	327	223	0.02%	0.002%
32	6.253	1513	1528	1549	rBV	385878	720975	54.70%	7.125%
33	6.539	1606	1617	1627	rVB9	4436	8523	0.65%	0.084%
34	6.697	1651	1666	1684	rBV	308252	599295	45.47%	5.922%
35	6.800	1695	1698	1700	rBV	696	470	0.04%	0.005%
36	6.973	1749	1752	1757	rBV2	238	276	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045154.D
 Acq On : 05 Oct 2021 18:54
 Operator : SY/MD
 Sample : M4025-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.054	1768	1777	1783	rBV3	539	931	0.07%	0.009%
38	7.124	1797	1799	1802	rVB2	203	134	0.01%	0.001%
39	7.185	1802	1818	1827	rBV3	1797	3440	0.26%	0.034%
40	7.295	1848	1852	1858	rVV	178	208	0.02%	0.002%
41	7.385	1877	1880	1884	rVB2	208	190	0.01%	0.002%
42	7.410	1884	1888	1894	rBV2	293	356	0.03%	0.004%
43	7.439	1894	1897	1900	rVV	186	154	0.01%	0.002%
44	7.459	1900	1903	1908	rVB2	142	149	0.01%	0.001%
45	7.568	1924	1937	1954	rBV	170480	297286	22.55%	2.938%
46	7.690	1967	1975	1984	rBV5	1135	1847	0.14%	0.018%
47	7.806	2007	2011	2014	rBV2	266	213	0.02%	0.002%
48	7.902	2027	2041	2056	rBV	590916	1017429	77.19%	10.054%
49	7.973	2057	2063	2077	rVB	9107	15604	1.18%	0.154%
50	8.182	2116	2128	2149	rBV	118550	199565	15.14%	1.972%
51	8.369	2184	2186	2192	rBV2	122	139	0.01%	0.001%
52	8.481	2214	2221	2224	rBV2	453	604	0.05%	0.006%
53	8.639	2257	2270	2313	rVV	465219	813560	61.72%	8.039%
54	8.819	2324	2326	2328	rBV2	322	210	0.02%	0.002%
55	8.835	2329	2331	2335	rVB2	226	182	0.01%	0.002%
56	9.224	2449	2452	2455	rBV2	189	150	0.01%	0.001%
57	9.295	2471	2474	2479	rVB2	193	141	0.01%	0.001%
58	9.420	2500	2513	2538	rBV	533739	878254	66.63%	8.679%
59	9.571	2557	2560	2566	rBV2	416	485	0.04%	0.005%
60	9.697	2593	2599	2609	rVB4	975	1425	0.11%	0.014%
61	9.793	2625	2629	2635	rBV2	232	171	0.01%	0.002%
62	9.951	2673	2678	2681	rBV2	251	322	0.02%	0.003%
63	10.037	2698	2705	2706	rBV	264	281	0.02%	0.003%
64	10.105	2722	2726	2731	rBV2	288	373	0.03%	0.004%
65	10.304	2785	2788	2791	rVB2	188	129	0.01%	0.001%
66	10.327	2791	2795	2798	rBV2	163	146	0.01%	0.001%
67	10.391	2812	2815	2819	rBV2	209	174	0.01%	0.002%
68	10.468	2832	2839	2841	rBV	146	204	0.02%	0.002%
69	10.677	2896	2904	2916	rVB2	2608	3683	0.28%	0.036%
70	10.761	2916	2930	2953	rVB	428462	684778	51.95%	6.767%
71	10.844	2953	2956	2959	rBV2	178	157	0.01%	0.002%
72	10.996	2999	3003	3006	rBV3	298	263	0.02%	0.003%
73	11.118	3038	3041	3044	rVV2	319	245	0.02%	0.002%
74	11.465	3138	3149	3160	rBV5	1531	2644	0.20%	0.026%
75	11.577	3180	3184	3190	rBV3	365	401	0.03%	0.004%
76	11.680	3210	3216	3218	rBV2	310	351	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045154.D
 Acq On : 05 Oct 2021 18:54
 Operator : SY/MD
 Sample : M4025-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.700	3218	3222	3228	rVB2	942	1048	0.08%	0.010%
78	11.815	3245	3258	3274	rBV	505586	794636	60.29%	7.852%
79	11.973	3302	3307	3316	rVB3	1718	2428	0.18%	0.024%
80	12.108	3347	3349	3357	rVB2	208	151	0.01%	0.001%
81	12.195	3361	3376	3397	rVV	556422	876879	66.53%	8.665%
82	12.330	3416	3418	3421	rBV2	453	189	0.01%	0.002%
83	12.430	3446	3449	3452	rBV	227	177	0.01%	0.002%
84	12.777	3552	3557	3560	rBV2	184	223	0.02%	0.002%
85	12.831	3571	3574	3579	rBV	232	194	0.01%	0.002%
86	12.860	3579	3583	3585	rBV	188	176	0.01%	0.002%
87	13.053	3638	3643	3646	rBV2	212	226	0.02%	0.002%
88	13.227	3694	3697	3699	rBV	150	130	0.01%	0.001%
89	13.375	3738	3743	3746	rBV2	216	265	0.02%	0.003%
90	13.581	3804	3807	3809	rBV2	203	163	0.01%	0.002%
91	13.902	3902	3907	3908	rBV2	195	182	0.01%	0.002%
92	14.102	3964	3969	3972	rBV2	356	326	0.02%	0.003%
93	14.172	3988	3991	3995	rVB	411	304	0.02%	0.003%
94	14.201	3997	4000	4004	rBV	244	238	0.02%	0.002%
95	14.282	4021	4025	4029	rBV2	268	256	0.02%	0.003%
96	14.368	4048	4052	4054	rBV2	353	326	0.02%	0.003%
97	14.420	4063	4068	4071	rBV2	346	291	0.02%	0.003%
98	14.510	4092	4096	4103	rBV2	350	502	0.04%	0.005%
99	14.706	4154	4157	4160	rBV3	268	267	0.02%	0.003%
100	15.825	4503	4505	4511	rVB3	517	386	0.03%	0.004%


Sum of corrected areas: 10119613

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045154.D
Acq On : 05 Oct 2021 18:54
Operator : SY/MD
Sample : M4025-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

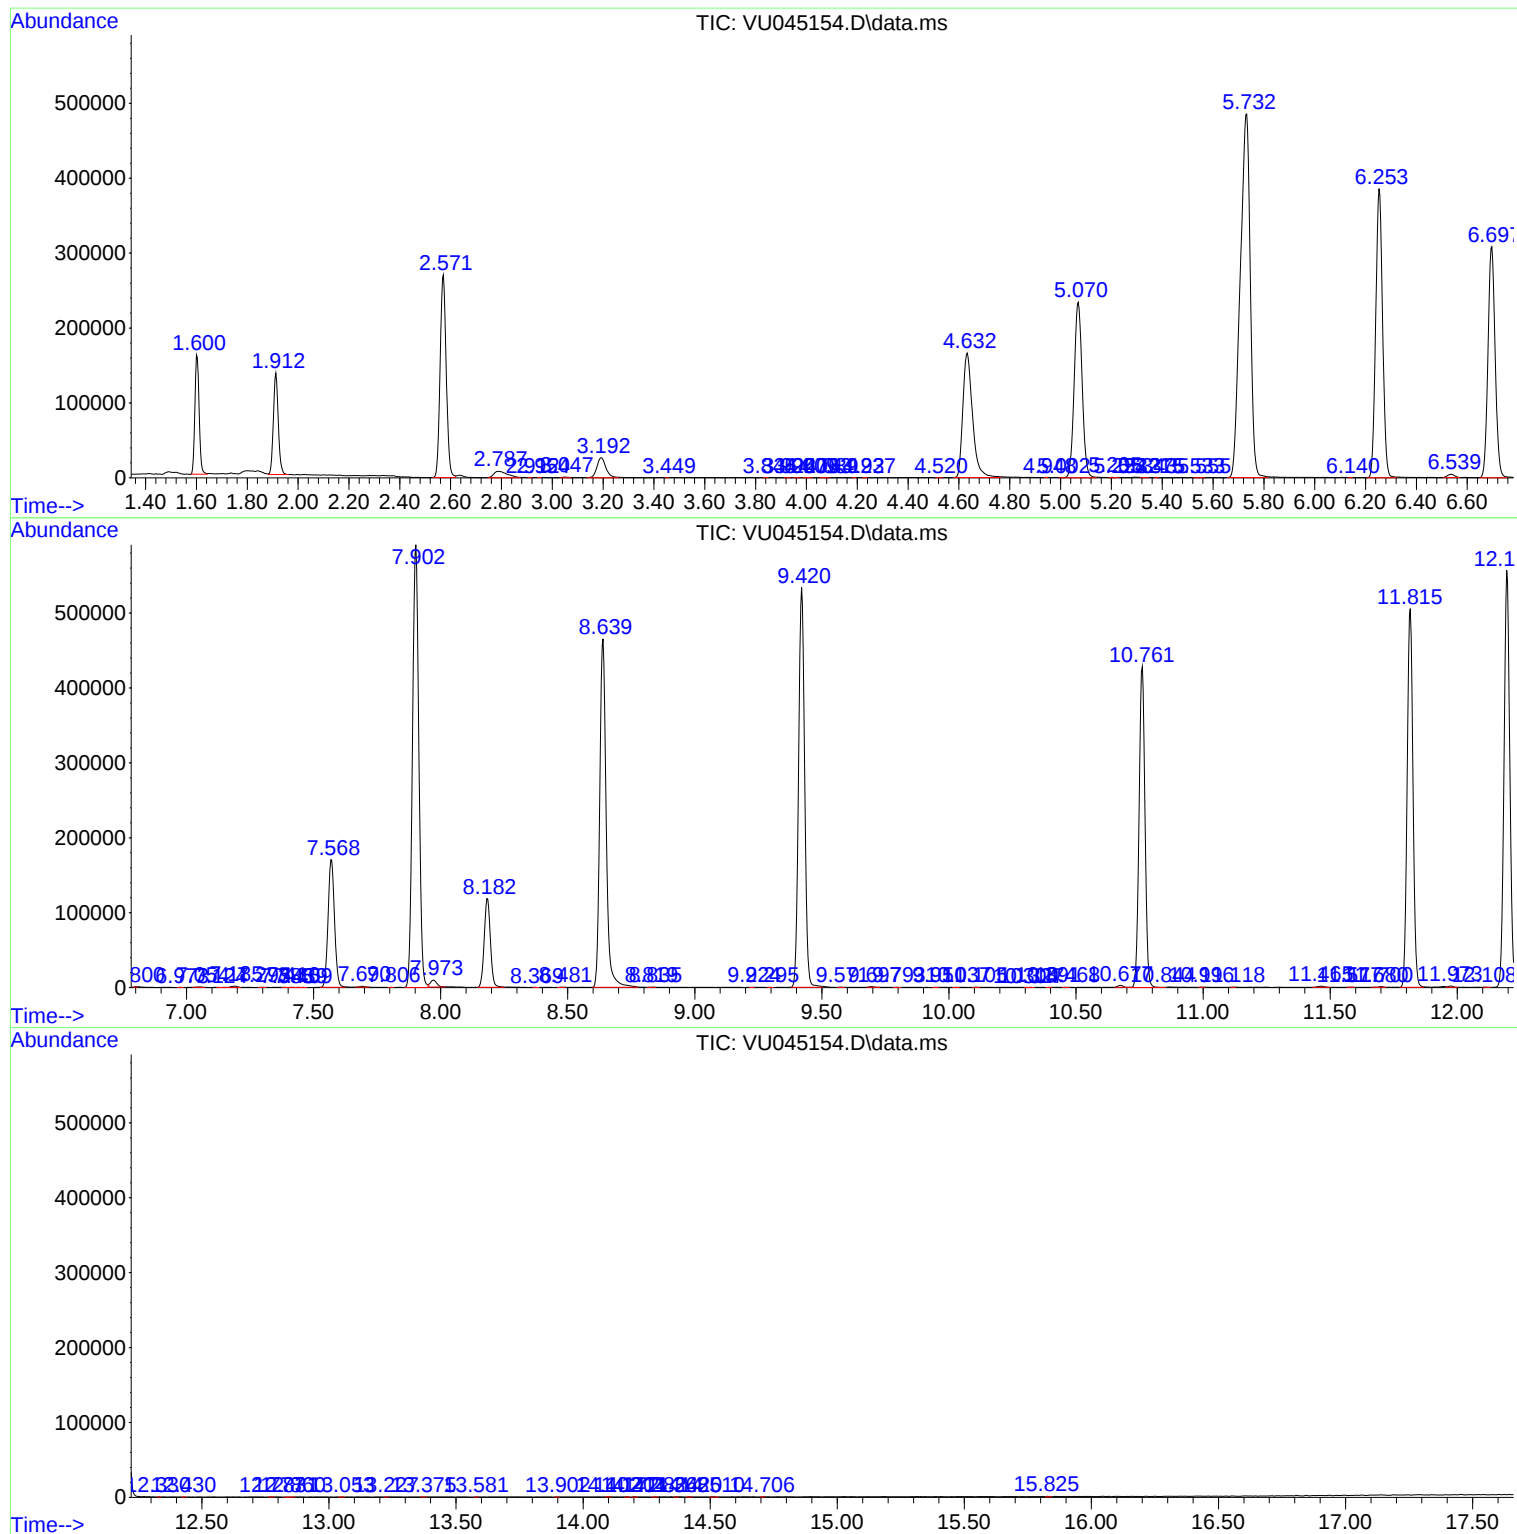

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045154.D
Acq On : 05 Oct 2021 18:54
Operator : SY/MD
Sample : M4025-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045154.D
Acq On : 05 Oct 2021 18:54
Operator : SY/MD
Sample : M4025-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
