

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045155.D
 Acq On : 05 Oct 2021 19:17
 Operator : SY/MD
 Sample : M4025-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045155.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	95	rBV	159900	190924	14.39%	1.899%
2	1.912	171	178	198	rVB	137254	184664	13.92%	1.837%
3	2.571	370	383	400	rBV	274884	450738	33.98%	4.484%
4	2.803	447	455	456	rBV2	1152	1301	0.10%	0.013%
5	2.915	486	490	492	rBV2	270	207	0.02%	0.002%
6	2.960	498	504	510	rBV3	785	1205	0.09%	0.012%
7	3.182	570	573	575	rBV2	288	229	0.02%	0.002%
8	3.195	575	577	583	rVB3	632	590	0.04%	0.006%
9	3.694	727	732	735	rVB	154	155	0.01%	0.002%
10	3.716	736	739	745	rBV2	180	178	0.01%	0.002%
11	3.758	750	752	757	rVB	199	195	0.01%	0.002%
12	3.864	783	785	789	rVB2	335	217	0.02%	0.002%
13	3.964	813	816	819	rBV	162	135	0.01%	0.001%
14	4.285	913	916	919	rVB	218	153	0.01%	0.002%
15	4.321	923	927	930	rBV2	203	223	0.02%	0.002%
16	4.504	980	984	988	rBV2	163	146	0.01%	0.001%
17	4.629	1008	1023	1059	rBV	155514	389106	29.33%	3.871%
18	5.070	1141	1160	1184	rBV	233081	510857	38.51%	5.082%
19	5.182	1193	1195	1198	rVV2	293	193	0.01%	0.002%
20	5.211	1200	1204	1207	rVV3	454	389	0.03%	0.004%
21	5.298	1224	1231	1236	rVB2	389	690	0.05%	0.007%
22	5.378	1250	1256	1258	rBV2	367	432	0.03%	0.004%
23	5.732	1343	1366	1397	rBV2	486622	1326537	100.00%	13.196%
24	6.009	1447	1452	1454	rBV3	277	281	0.02%	0.003%
25	6.108	1479	1483	1485	rBV2	226	186	0.01%	0.002%
26	6.156	1494	1498	1501	rBV2	327	308	0.02%	0.003%
27	6.253	1513	1528	1550	rBV	384360	715844	53.96%	7.121%
28	6.536	1607	1616	1629	rVB9	2852	5305	0.40%	0.053%
29	6.603	1629	1637	1639	rVV2	244	326	0.02%	0.003%
30	6.697	1650	1666	1688	rBV	309574	600806	45.29%	5.977%
31	6.806	1696	1700	1708	rVB4	1007	1292	0.10%	0.013%
32	6.841	1708	1711	1716	rVB3	379	363	0.03%	0.004%
33	6.864	1716	1718	1721	rBV	222	189	0.01%	0.002%
34	7.028	1763	1769	1770	rBV2	285	278	0.02%	0.003%
35	7.050	1770	1776	1782	rVV2	491	737	0.06%	0.007%
36	7.118	1794	1797	1801	rVB	193	171	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045155.D
 Acq On : 05 Oct 2021 19:17
 Operator : SY/MD
 Sample : M4025-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.144	1801	1805	1810	rBV	291	387	0.03%	0.004%
38	7.185	1810	1818	1827	rVB3	1968	3292	0.25%	0.033%
39	7.279	1844	1847	1852	rVB	227	189	0.01%	0.002%
40	7.356	1867	1871	1875	rBV2	176	198	0.01%	0.002%
41	7.439	1892	1897	1899	rBV	254	216	0.02%	0.002%
42	7.571	1925	1938	1956	rBV	170869	297112	22.40%	2.956%
43	7.690	1970	1975	1989	rVB5	1469	2340	0.18%	0.023%
44	7.902	2027	2041	2056	rBV	597804	1024824	77.26%	10.195%
45	8.182	2116	2128	2146	rBV	116928	199526	15.04%	1.985%
46	8.417	2197	2201	2204	rBV	203	190	0.01%	0.002%
47	8.455	2208	2213	2214	rVV2	214	167	0.01%	0.002%
48	8.475	2214	2219	2227	rVB2	582	870	0.07%	0.009%
49	8.639	2256	2270	2316	rBV	462276	825259	62.21%	8.210%
50	8.861	2337	2339	2343	rBV2	205	135	0.01%	0.001%
51	8.973	2368	2374	2377	rBV2	128	156	0.01%	0.002%
52	9.021	2385	2389	2392	rVB	238	200	0.02%	0.002%
53	9.047	2392	2397	2404	rBV2	245	343	0.03%	0.003%
54	9.086	2404	2409	2412	rBV2	138	177	0.01%	0.002%
55	9.118	2415	2419	2421	rBV	239	206	0.02%	0.002%
56	9.317	2478	2481	2488	rVB2	174	212	0.02%	0.002%
57	9.420	2499	2513	2548	rBV	539225	889103	67.02%	8.845%
58	9.693	2591	2598	2607	rBV3	944	1478	0.11%	0.015%
59	9.793	2627	2629	2633	rBV	158	150	0.01%	0.001%
60	9.886	2654	2658	2661	rBV2	234	225	0.02%	0.002%
61	9.934	2664	2673	2677	rBV2	295	446	0.03%	0.004%
62	9.973	2680	2685	2687	rBV2	185	174	0.01%	0.002%
63	10.105	2722	2726	2732	rBV	488	602	0.05%	0.006%
64	10.436	2826	2829	2831	rBV	163	135	0.01%	0.001%
65	10.529	2854	2858	2861	rVB2	216	192	0.01%	0.002%
66	10.674	2894	2903	2912	rVB2	2899	4404	0.33%	0.044%
67	10.761	2916	2930	2950	rVB	437286	699605	52.74%	6.960%
68	10.854	2956	2959	2960	rBV2	215	141	0.01%	0.001%
69	10.996	2999	3003	3005	rBV2	179	159	0.01%	0.002%
70	11.012	3005	3008	3010	rVB2	286	151	0.01%	0.002%
71	11.031	3011	3014	3018	rVB2	237	195	0.01%	0.002%
72	11.057	3018	3022	3025	rBV	271	256	0.02%	0.003%
73	11.121	3037	3042	3049	rBV5	545	746	0.06%	0.007%
74	11.237	3072	3078	3080	rBV	203	259	0.02%	0.003%
75	11.455	3141	3146	3162	rVB5	1737	3478	0.26%	0.035%
76	11.523	3162	3167	3169	rBV2	225	184	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045155.D
 Acq On : 05 Oct 2021 19:17
 Operator : SY/MD
 Sample : M4025-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.574	3180	3183	3184	rBV2	325	210	0.02%	0.002%
78	11.696	3215	3221	3235	rVB4	1049	1659	0.13%	0.017%
79	11.758	3235	3240	3242	rBV2	197	209	0.02%	0.002%
80	11.815	3245	3258	3274	rBV	509826	810315	61.08%	8.061%
81	11.944	3293	3298	3300	rBV2	564	549	0.04%	0.005%
82	11.973	3305	3307	3316	rVB3	1881	2084	0.16%	0.021%
83	12.047	3327	3330	3333	rBV2	207	210	0.02%	0.002%
84	12.195	3360	3376	3395	rBV	551723	889310	67.04%	8.847%
85	12.336	3416	3420	3424	rVB2	579	482	0.04%	0.005%
86	12.446	3449	3454	3463	rVB2	225	404	0.03%	0.004%
87	12.484	3463	3466	3467	rBV	269	174	0.01%	0.002%
88	12.549	3482	3486	3489	rBV	262	268	0.02%	0.003%
89	12.600	3500	3502	3507	rBV2	219	188	0.01%	0.002%
90	12.700	3530	3533	3536	rBV2	243	212	0.02%	0.002%
91	13.024	3631	3634	3637	rBV2	169	146	0.01%	0.001%
92	13.413	3751	3755	3759	rBV	180	171	0.01%	0.002%
93	13.523	3785	3789	3791	rBV	221	178	0.01%	0.002%
94	13.802	3870	3876	3879	rBV2	189	234	0.02%	0.002%
95	13.857	3890	3893	3899	rBV	171	152	0.01%	0.002%
96	14.195	3991	3998	4003	rBV2	295	419	0.03%	0.004%
97	14.417	4065	4067	4070	rBV	201	139	0.01%	0.001%
98	14.603	4122	4125	4128	rBV2	286	215	0.02%	0.002%
99	14.658	4139	4142	4143	rBV	324	228	0.02%	0.002%
100	15.063	4263	4268	4272	rBV2	326	469	0.04%	0.005%




Sum of corrected areas: 10052257

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045155.D
Acq On : 05 Oct 2021 19:17
Operator : SY/MD
Sample : M4025-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

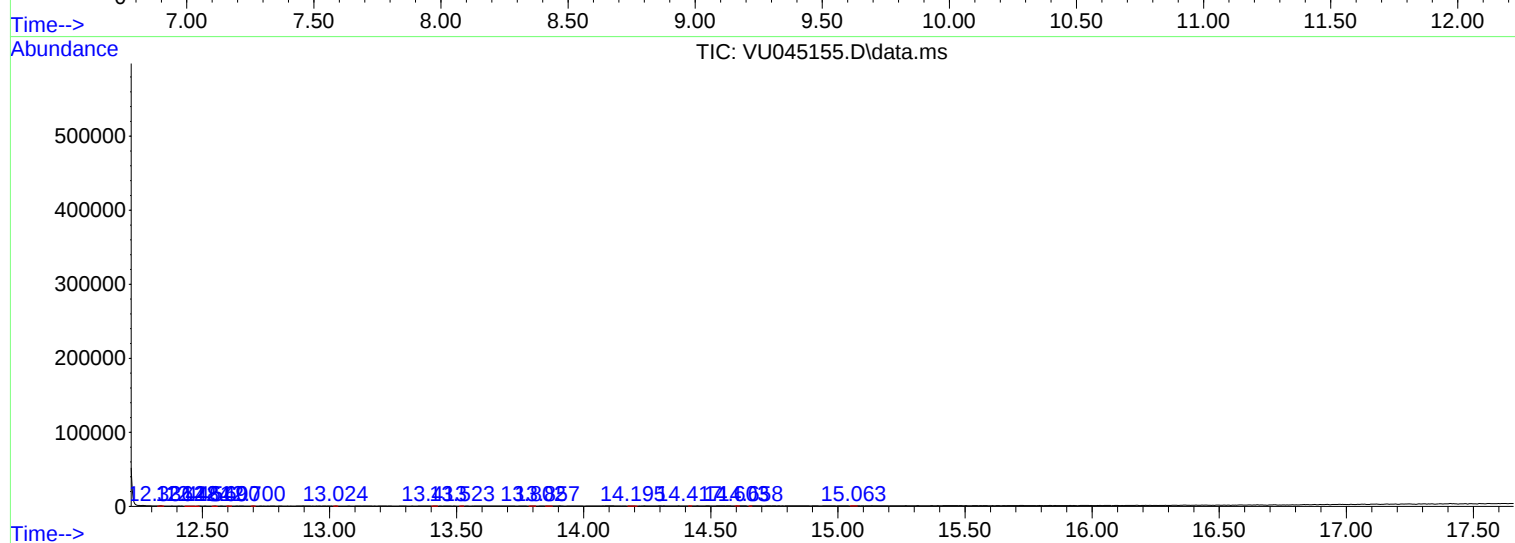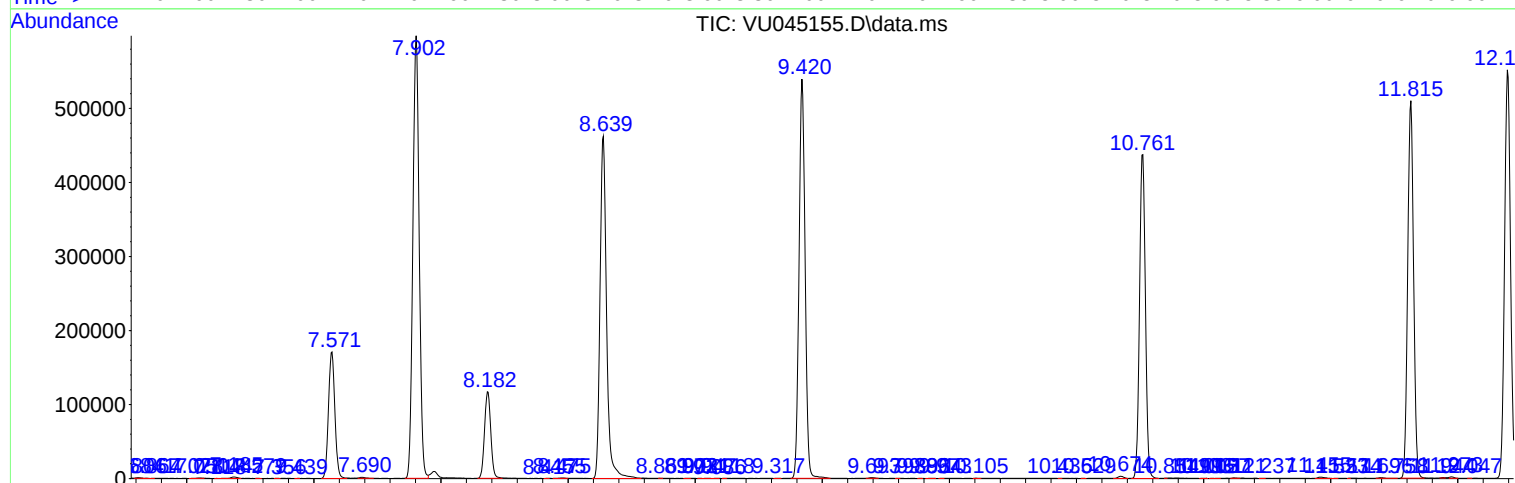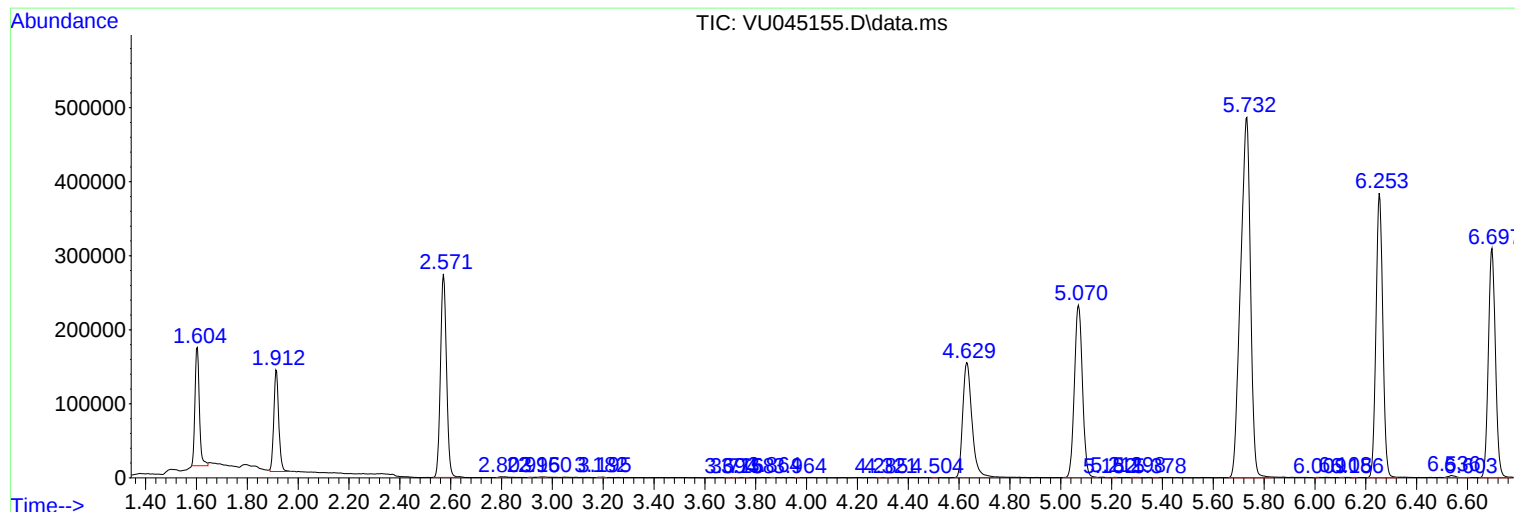

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045155.D
Acq On : 05 Oct 2021 19:17
Operator : SY/MD
Sample : M4025-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045155.D
Acq On : 05 Oct 2021 19:17
Operator : SY/MD
Sample : M4025-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
