

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045156.D
 Acq On : 05 Oct 2021 19:40
 Operator : SY/MD
 Sample : M4025-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU045156.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rBV	154410	181794	13.81%	1.824%
2	1.909	168	177	196	rVB	131611	183571	13.94%	1.842%
3	2.568	370	382	400	rBV	271621	450799	34.23%	4.523%
4	2.745	432	437	440	rVB	260	237	0.02%	0.002%
5	2.793	440	452	455	rBV3	1527	2887	0.22%	0.029%
6	2.951	497	501	502	rBV3	364	302	0.02%	0.003%
7	3.009	516	519	522	rVV	155	151	0.01%	0.002%
8	3.047	526	531	539	rVB3	970	1242	0.09%	0.012%
9	3.118	550	553	557	rVB2	202	139	0.01%	0.001%
10	3.147	557	562	565	rBV	541	536	0.04%	0.005%
11	3.195	569	577	585	rVB2	786	1701	0.13%	0.017%
12	3.417	642	646	649	rBV2	121	126	0.01%	0.001%
13	3.488	663	668	671	rBV2	170	205	0.02%	0.002%
14	3.681	723	728	734	rBV2	230	343	0.03%	0.003%
15	4.102	856	859	862	rBV	172	155	0.01%	0.002%
16	4.353	934	937	943	rBV2	149	147	0.01%	0.001%
17	4.571	1002	1005	1008	rBV	229	194	0.01%	0.002%
18	4.629	1008	1023	1059	rBV	146405	370439	28.13%	3.716%
19	5.070	1142	1160	1181	rBV	233589	515964	39.18%	5.176%
20	5.295	1224	1230	1236	rBV3	404	592	0.04%	0.006%
21	5.356	1243	1249	1254	rBV2	150	233	0.02%	0.002%
22	5.382	1254	1257	1261	rVV2	305	249	0.02%	0.002%
23	5.475	1282	1286	1289	rVB2	223	183	0.01%	0.002%
24	5.729	1340	1365	1396	rBV2	486800	1316848	100.00%	13.211%
25	6.195	1504	1510	1513	rBV2	144	176	0.01%	0.002%
26	6.253	1513	1528	1555	rBV	387406	724291	55.00%	7.266%
27	6.350	1555	1558	1563	rVB2	458	382	0.03%	0.004%
28	6.375	1563	1566	1569	rBV3	168	167	0.01%	0.002%
29	6.456	1588	1591	1594	rBV2	173	153	0.01%	0.002%
30	6.542	1606	1618	1629	rVB5	5578	11173	0.85%	0.112%
31	6.587	1629	1632	1634	rBV	189	128	0.01%	0.001%
32	6.623	1640	1643	1646	rVB	197	150	0.01%	0.002%
33	6.694	1650	1665	1685	rBV	308045	599157	45.50%	6.011%
34	6.809	1696	1701	1710	rVB4	882	1337	0.10%	0.013%
35	7.102	1785	1792	1796	rBV2	205	251	0.02%	0.003%
36	7.186	1810	1818	1831	rBV3	2171	3472	0.26%	0.035%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045156.D
 Acq On : 05 Oct 2021 19:40
 Operator : SY/MD
 Sample : M4025-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.369	1872	1875	1880	rBV	225	223	0.02%	0.002%
38	7.395	1880	1883	1889	rVB2	249	248	0.02%	0.002%
39	7.423	1889	1892	1900	rVB2	266	268	0.02%	0.003%
40	7.462	1900	1904	1905	rBV	263	215	0.02%	0.002%
41	7.568	1925	1937	1958	rBV	168356	293406	22.28%	2.944%
42	7.690	1970	1975	1988	rVB4	1361	1878	0.14%	0.019%
43	7.903	2027	2041	2056	rBV	597271	1016927	77.22%	10.202%
44	7.973	2057	2063	2076	rVB	8812	13700	1.04%	0.137%
45	8.182	2115	2128	2148	rBV	115644	195521	14.85%	1.962%
46	8.324	2168	2172	2174	rBV2	297	244	0.02%	0.002%
47	8.414	2197	2200	2202	rBV	212	137	0.01%	0.001%
48	8.639	2256	2270	2299	rBV	453132	790174	60.00%	7.927%
49	9.157	2428	2431	2434	rVB	234	172	0.01%	0.002%
50	9.182	2434	2439	2442	rBV2	215	239	0.02%	0.002%
51	9.420	2500	2513	2548	rVV	544078	887085	67.36%	8.899%
52	9.574	2556	2561	2565	rBV	267	318	0.02%	0.003%
53	9.661	2585	2588	2590	rBV2	172	126	0.01%	0.001%
54	9.697	2593	2599	2605	rVB2	780	995	0.08%	0.010%
55	9.886	2652	2658	2661	rBV2	186	192	0.01%	0.002%
56	9.919	2666	2668	2674	rVB2	154	128	0.01%	0.001%
57	9.986	2686	2689	2691	rBV	211	148	0.01%	0.001%
58	10.102	2720	2725	2728	rBV2	213	233	0.02%	0.002%
59	10.140	2731	2737	2740	rBV2	185	220	0.02%	0.002%
60	10.327	2791	2795	2798	rBV	180	190	0.01%	0.002%
61	10.369	2804	2808	2817	rBV2	202	403	0.03%	0.004%
62	10.472	2836	2840	2841	rBV	200	146	0.01%	0.001%
63	10.639	2888	2892	2895	rBV2	278	164	0.01%	0.002%
64	10.674	2895	2903	2913	rBV3	3553	4890	0.37%	0.049%
65	10.761	2917	2930	2949	rBV	422772	685576	52.06%	6.878%
66	10.870	2958	2964	2969	rBV3	666	896	0.07%	0.009%
67	11.012	3003	3008	3013	rVV3	186	231	0.02%	0.002%
68	11.082	3024	3030	3034	rBV2	279	329	0.02%	0.003%
69	11.121	3039	3042	3046	rBV3	445	419	0.03%	0.004%
70	11.263	3084	3086	3092	rVB2	202	177	0.01%	0.002%
71	11.320	3102	3104	3107	rBV2	204	150	0.01%	0.002%
72	11.465	3134	3149	3158	rBV5	1945	3866	0.29%	0.039%
73	11.513	3161	3164	3167	rVB2	172	149	0.01%	0.001%
74	11.636	3195	3202	3208	rVB2	827	1177	0.09%	0.012%
75	11.664	3208	3211	3215	rBV2	228	272	0.02%	0.003%
76	11.700	3215	3222	3228	rVV2	1203	1573	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045156.D
 Acq On : 05 Oct 2021 19:40
 Operator : SY/MD
 Sample : M4025-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.758	3237	3240	3245	rBV2	208	236	0.02%	0.002%
78	11.812	3245	3257	3280	rBV	514593	810449	61.54%	8.131%
79	11.925	3287	3292	3293	rBV	326	277	0.02%	0.003%
80	11.944	3293	3298	3302	rVV5	1160	1530	0.12%	0.015%
81	11.976	3302	3308	3316	rVB3	1758	2607	0.20%	0.026%
82	12.044	3323	3329	3332	rBV	220	236	0.02%	0.002%
83	12.066	3332	3336	3338	rBV2	247	214	0.02%	0.002%
84	12.111	3347	3350	3353	rBV2	226	178	0.01%	0.002%
85	12.195	3362	3376	3398	rBV	542344	874534	66.41%	8.774%
86	12.336	3415	3420	3423	rBV4	623	615	0.05%	0.006%
87	12.407	3439	3442	3444	rBV2	516	267	0.02%	0.003%
88	12.629	3508	3511	3516	rBV2	196	209	0.02%	0.002%
89	12.767	3550	3554	3558	rVB	324	260	0.02%	0.003%
90	13.298	3716	3719	3722	rBV2	220	200	0.02%	0.002%
91	13.655	3826	3830	3834	rBV2	240	258	0.02%	0.003%
92	13.754	3855	3861	3868	rBV2	262	470	0.04%	0.005%
93	13.883	3899	3901	3905	rBV2	185	186	0.01%	0.002%
94	13.976	3927	3930	3933	rBV	292	199	0.02%	0.002%
95	14.024	3940	3945	3950	rBV2	254	349	0.03%	0.004%
96	14.311	4030	4034	4037	rBV2	289	274	0.02%	0.003%
97	14.385	4055	4057	4058	rBV	274	130	0.01%	0.001%
98	14.642	4135	4137	4140	rBV3	305	247	0.02%	0.002%
99	14.745	4163	4169	4173	rBV3	346	464	0.04%	0.005%
100	15.179	4301	4304	4305	rBV2	271	154	0.01%	0.002%




Sum of corrected areas: 9967822

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045156.D
Acq On : 05 Oct 2021 19:40
Operator : SY/MD
Sample : M4025-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

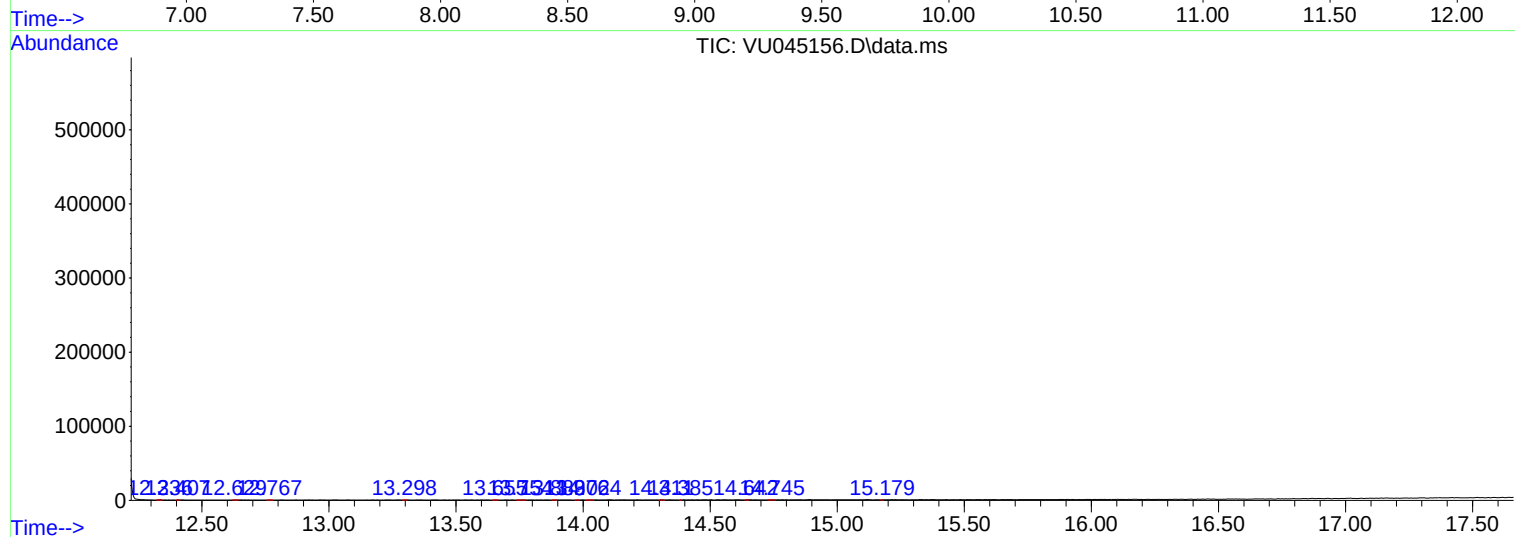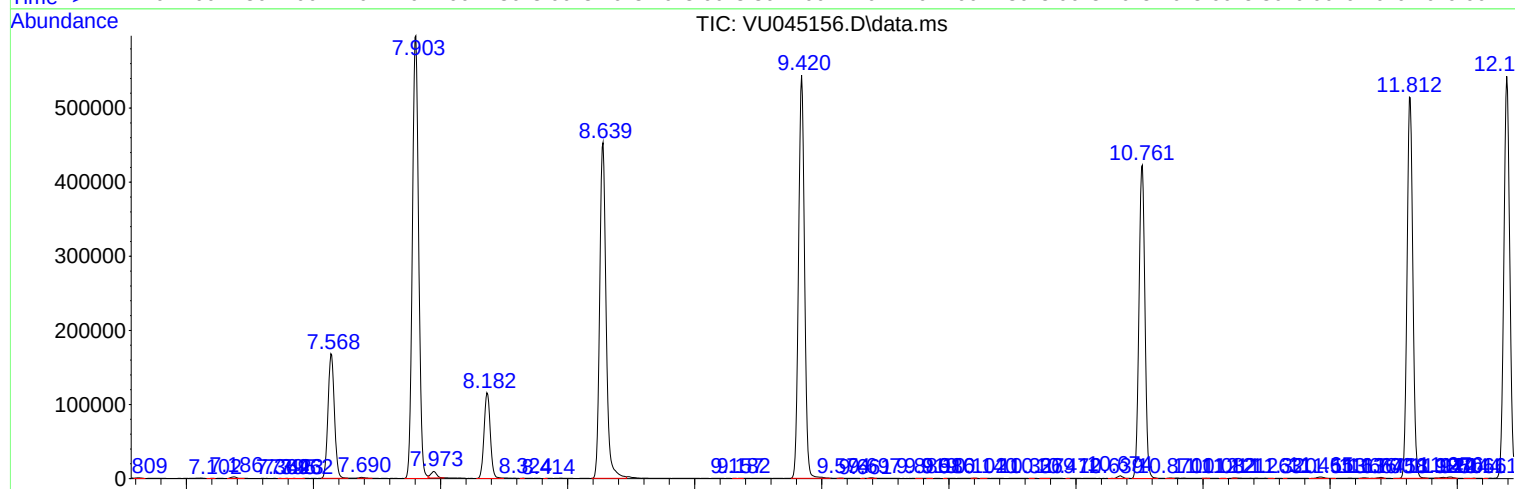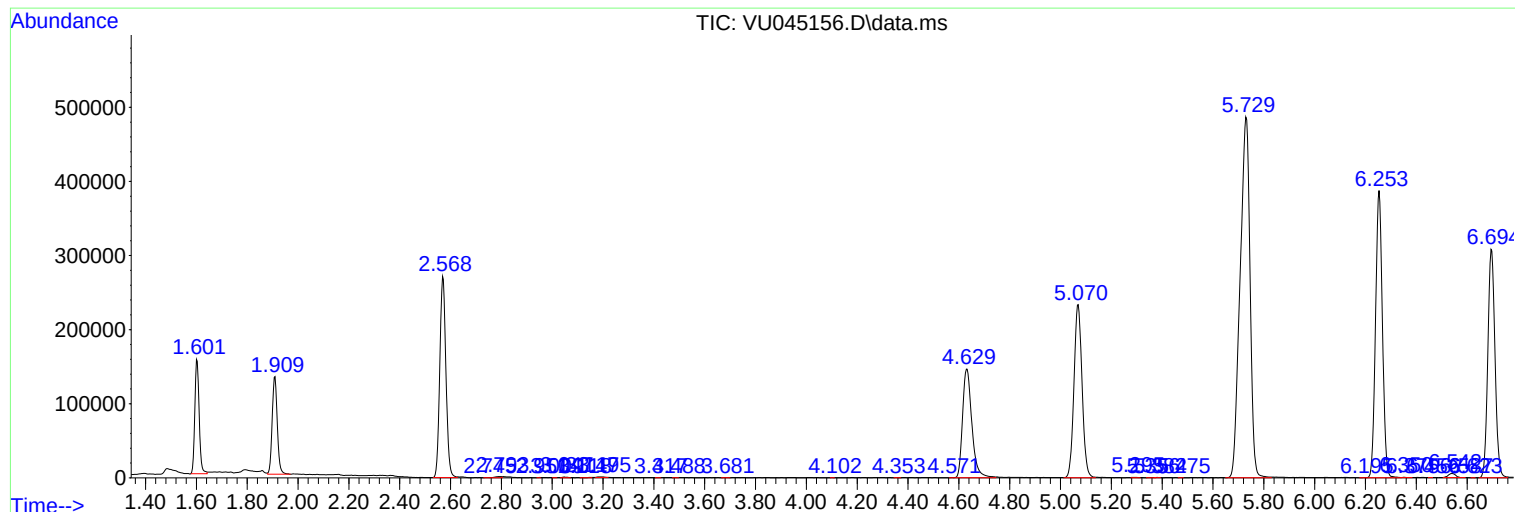

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045156.D
Acq On : 05 Oct 2021 19:40
Operator : SY/MD
Sample : M4025-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045156.D
Acq On : 05 Oct 2021 19:40
Operator : SY/MD
Sample : M4025-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
