

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045157.D
 Acq On : 05 Oct 2021 20:03
 Operator : SY/MD
 Sample : M4023-02 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045157.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	95	rBV	159902	186719	13.93%	1.657%
2	1.909	169	177	193	rVB	134915	181824	13.57%	1.614%
3	2.449	343	345	348	rVB3	376	170	0.01%	0.002%
4	2.572	370	383	402	rBV2	290755	508667	37.95%	4.514%
5	2.690	414	420	427	rVB2	307	446	0.03%	0.004%
6	2.745	432	437	441	rBV2	195	197	0.01%	0.002%
7	2.768	441	444	448	rVB	130	132	0.01%	0.001%
8	2.800	448	454	457	rBV3	580	612	0.05%	0.005%
9	2.893	481	483	488	rVB	225	157	0.01%	0.001%
10	2.954	497	502	503	rBV	367	262	0.02%	0.002%
11	3.051	517	532	549	rBV	27340	52525	3.92%	0.466%
12	3.192	567	576	586	rVV4	1237	2421	0.18%	0.021%
13	3.234	587	589	594	rVB2	188	149	0.01%	0.001%
14	3.462	657	660	663	rVB2	242	164	0.01%	0.001%
15	3.494	663	670	672	rBV	166	139	0.01%	0.001%
16	3.697	729	733	737	rVB2	231	196	0.01%	0.002%
17	3.758	750	752	755	rBV2	178	155	0.01%	0.001%
18	3.871	780	787	789	rBV2	767	965	0.07%	0.009%
19	4.028	834	836	839	rBV	187	156	0.01%	0.001%
20	4.150	870	874	878	rBV2	144	134	0.01%	0.001%
21	4.221	892	896	900	rBV2	213	223	0.02%	0.002%
22	4.501	979	983	985	rBV2	167	147	0.01%	0.001%
23	4.565	1000	1003	1007	rBV2	178	196	0.01%	0.002%
24	4.629	1007	1023	1064	rVV	156520	439953	32.83%	3.904%
25	4.813	1076	1080	1083	rBV2	304	264	0.02%	0.002%
26	4.832	1083	1086	1095	rVV2	505	483	0.04%	0.004%
27	5.070	1143	1160	1181	rBV	238063	521007	38.87%	4.623%
28	5.321	1222	1238	1256	rBV2	50349	111064	8.29%	0.986%
29	5.504	1291	1295	1300	rBV	206	208	0.02%	0.002%
30	5.632	1329	1335	1338	rBV	199	266	0.02%	0.002%
31	5.729	1342	1365	1392	rBV2	492041	1340247	100.00%	11.893%
32	6.038	1458	1461	1465	rBV2	200	172	0.01%	0.002%
33	6.079	1470	1474	1479	rBV2	209	237	0.02%	0.002%
34	6.169	1498	1502	1506	rVB2	186	215	0.02%	0.002%
35	6.198	1506	1511	1513	rBV	222	190	0.01%	0.002%
36	6.253	1513	1528	1549	rBV	386950	728960	54.39%	6.469%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045157.D
 Acq On : 05 Oct 2021 20:03
 Operator : SY/MD
 Sample : M4023-02 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.456	1588	1591	1594	rBV3	151	147	0.01%	0.001%
38	6.546	1604	1619	1651	rBV	458760	862106	64.32%	7.650%
39	6.697	1651	1666	1691	rVB	315488	616174	45.97%	5.468%
40	6.813	1697	1702	1703	rBV2	414	333	0.02%	0.003%
41	7.050	1768	1776	1780	rVV3	408	651	0.05%	0.006%
42	7.189	1809	1819	1826	rVV3	1886	3182	0.24%	0.028%
43	7.259	1838	1841	1842	rBV	197	138	0.01%	0.001%
44	7.568	1923	1937	1954	rBV	173602	301866	22.52%	2.679%
45	7.694	1968	1976	1985	rVB3	1355	2064	0.15%	0.018%
46	7.902	2026	2041	2055	rBV	599780	1035098	77.23%	9.186%
47	8.182	2113	2128	2148	rBV	120459	204243	15.24%	1.812%
48	8.404	2193	2197	2202	rBV3	580	543	0.04%	0.005%
49	8.475	2213	2219	2222	rBV3	232	264	0.02%	0.002%
50	8.555	2239	2244	2247	rBV2	307	237	0.02%	0.002%
51	8.636	2256	2269	2299	rBV	457329	795403	59.35%	7.058%
52	8.857	2333	2338	2340	rBV2	291	279	0.02%	0.002%
53	8.931	2358	2361	2364	rBV2	275	242	0.02%	0.002%
54	9.420	2500	2513	2546	rBV	548175	896635	66.90%	7.957%
55	9.571	2554	2560	2561	rBV2	881	810	0.06%	0.007%
56	9.636	2577	2580	2585	rVB2	194	195	0.01%	0.002%
57	9.693	2590	2598	2612	rVV2	4980	7465	0.56%	0.066%
58	9.915	2664	2667	2672	rVB	241	182	0.01%	0.002%
59	9.944	2672	2676	2679	rBV	146	135	0.01%	0.001%
60	9.963	2679	2682	2686	rBV	171	193	0.01%	0.002%
61	10.105	2718	2726	2736	rBV	2679	3757	0.28%	0.033%
62	10.243	2766	2769	2772	rBV	224	212	0.02%	0.002%
63	10.340	2795	2799	2803	rBV2	212	239	0.02%	0.002%
64	10.488	2843	2845	2855	rBV2	274	297	0.02%	0.003%
65	10.597	2875	2879	2883	rVB2	156	141	0.01%	0.001%
66	10.626	2883	2888	2889	rBV	233	195	0.01%	0.002%
67	10.674	2895	2903	2912	rBV2	3060	4261	0.32%	0.038%
68	10.761	2915	2930	2947	rBV	428799	695226	51.87%	6.169%
69	10.870	2957	2964	2968	rBV2	496	613	0.05%	0.005%
70	10.999	3001	3004	3005	rBV	327	169	0.01%	0.001%
71	11.031	3010	3014	3017	rBV2	199	150	0.01%	0.001%
72	11.057	3017	3022	3026	rBV2	221	252	0.02%	0.002%
73	11.118	3038	3041	3044	rBV2	591	500	0.04%	0.004%
74	11.346	3109	3112	3116	rVB2	261	195	0.01%	0.002%
75	11.462	3137	3148	3159	rBV5	2013	4197	0.31%	0.037%
76	11.581	3180	3185	3194	rVB3	459	581	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045157.D
 Acq On : 05 Oct 2021 20:03
 Operator : SY/MD
 Sample : M4023-02 2000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.626	3194	3199	3203	rBV2	260	306	0.02%	0.003%
78	11.697	3217	3221	3222	rBV2	837	522	0.04%	0.005%
79	11.816	3245	3258	3275	rBV	521582	826570	61.67%	7.335%
80	11.944	3294	3298	3303	rBV4	805	992	0.07%	0.009%
81	11.973	3303	3307	3316	rVB3	1724	2214	0.17%	0.020%
82	12.057	3330	3333	3340	rVB2	314	306	0.02%	0.003%
83	12.089	3340	3343	3347	rBV2	145	143	0.01%	0.001%
84	12.195	3359	3376	3393	rBV	569828	914084	68.20%	8.112%
85	12.516	3473	3476	3479	rBV2	217	166	0.01%	0.001%
86	12.668	3520	3523	3529	rBV2	156	147	0.01%	0.001%
87	12.716	3534	3538	3540	rBV2	212	207	0.02%	0.002%
88	12.832	3571	3574	3578	rBV2	362	339	0.03%	0.003%
89	13.330	3726	3729	3733	rBV	260	257	0.02%	0.002%
90	13.635	3821	3824	3825	rBV	240	146	0.01%	0.001%
91	13.664	3831	3833	3835	rBV	210	145	0.01%	0.001%
92	13.780	3865	3869	3874	rBV3	253	293	0.02%	0.003%
93	13.925	3906	3914	3918	rBV2	287	462	0.03%	0.004%
94	13.995	3933	3936	3939	rVB2	265	198	0.01%	0.002%
95	14.018	3940	3943	3946	rBV	306	220	0.02%	0.002%
96	14.227	4005	4008	4012	rBV	173	145	0.01%	0.001%
97	14.311	4031	4034	4039	rBV2	243	225	0.02%	0.002%
98	14.346	4043	4045	4050	rVB2	361	264	0.02%	0.002%
99	14.809	4186	4189	4191	rBV	268	209	0.02%	0.002%
100	15.163	4293	4299	4303	rBV	500	665	0.05%	0.006%




Sum of corrected areas: 11268817

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045157.D
Acq On : 05 Oct 2021 20:03
Operator : SY/MD
Sample : M4023-02 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

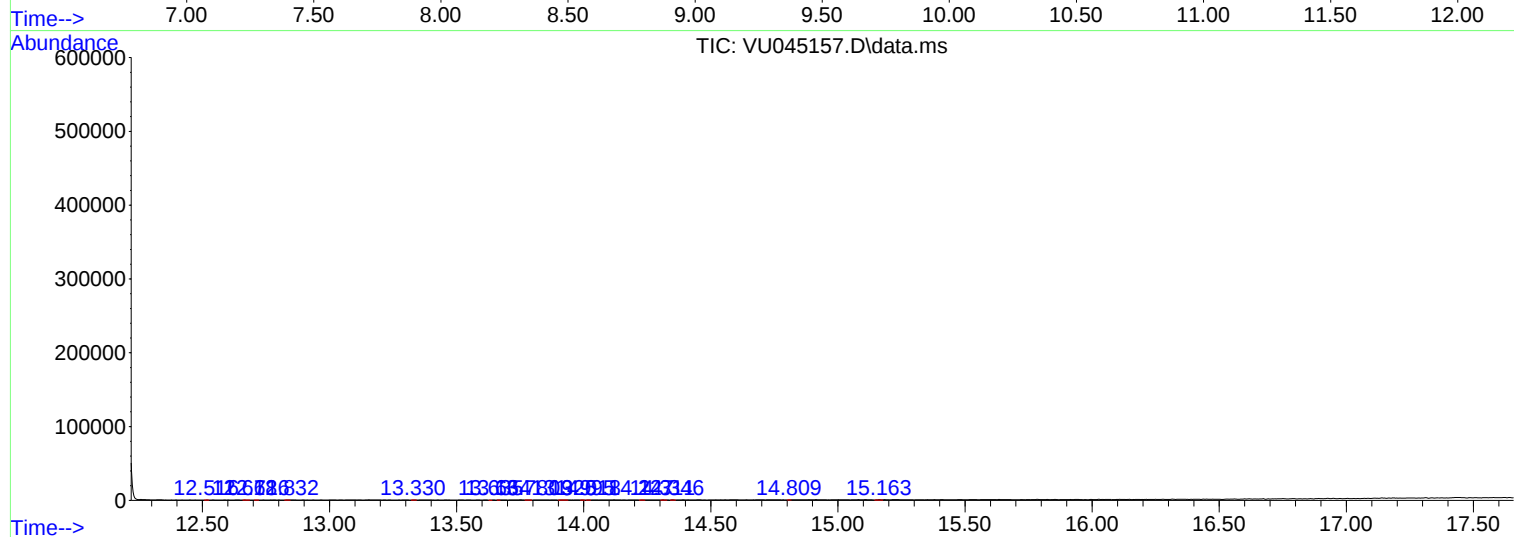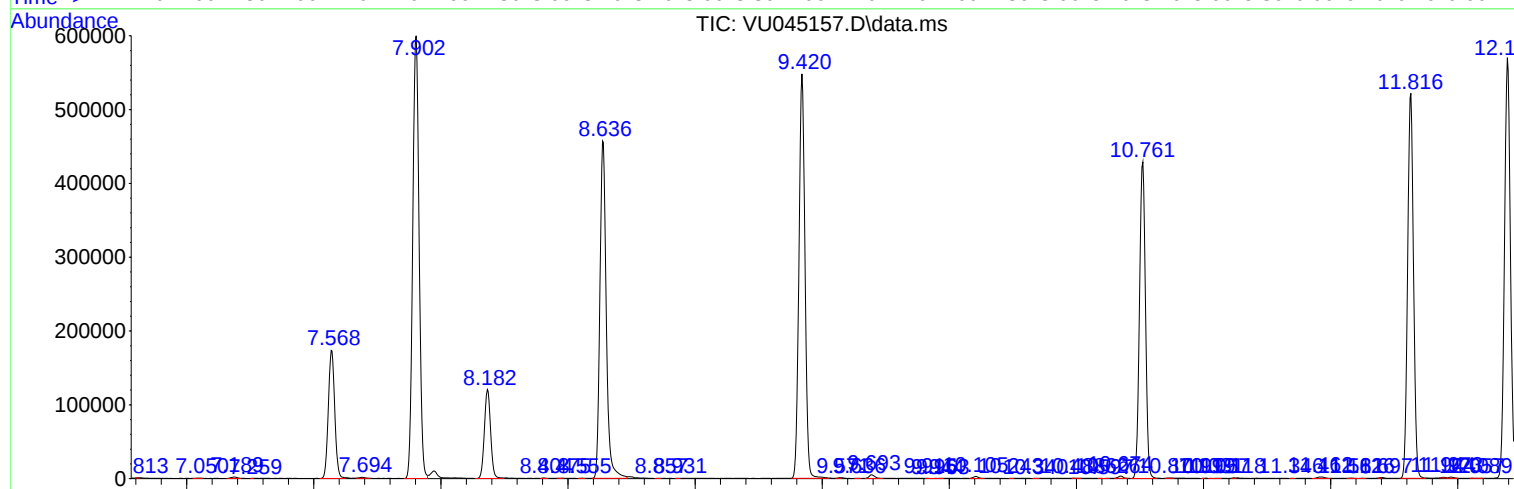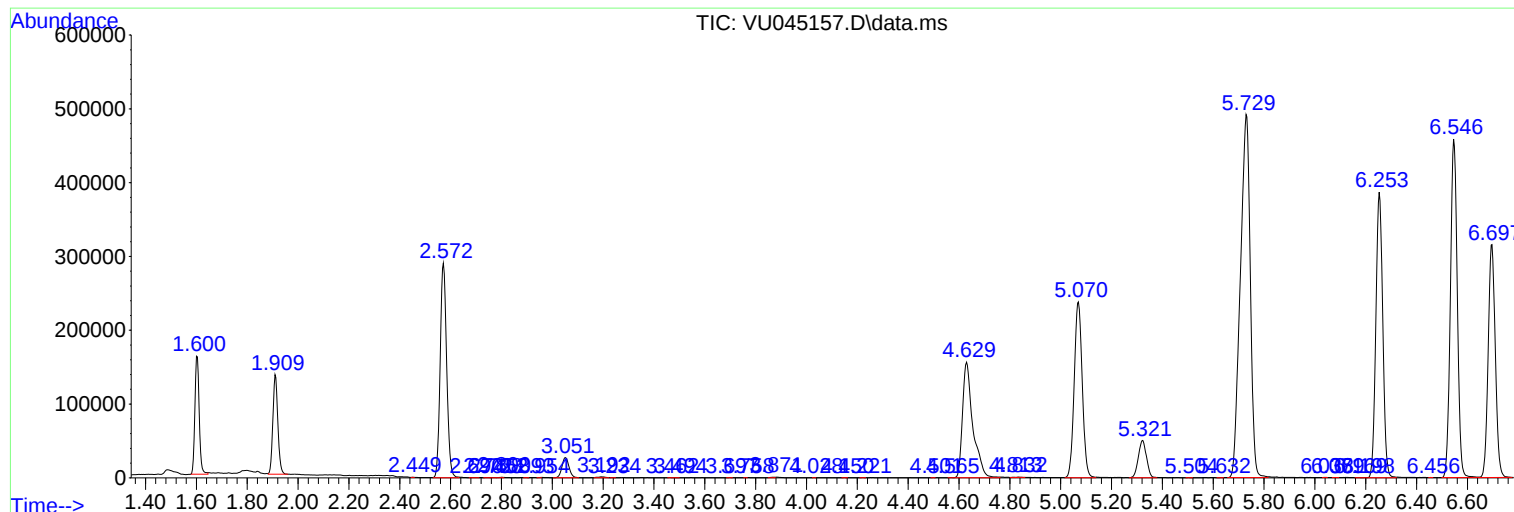

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045157.D
Acq On : 05 Oct 2021 20:03
Operator : SY/MD
Sample : M4023-02 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045157.D
Acq On : 05 Oct 2021 20:03
Operator : SY/MD
Sample : M4023-02 2000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
