

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045160.D
 Acq On : 05 Oct 2021 21:36
 Operator : SY/MD
 Sample : VU1005WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU045160.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	99	rVB	168610	196058	14.41%	1.962%
2	1.903	168	175	191	rVB	152464	197959	14.55%	1.981%
3	2.417	333	335	337	rVB3	468	201	0.01%	0.002%
4	2.568	367	382	407	rBV	282567	472727	34.74%	4.732%
5	2.748	435	438	443	rVB2	158	170	0.01%	0.002%
6	2.793	444	452	460	rBV3	1007	1592	0.12%	0.016%
7	2.961	494	504	509	rBV4	590	998	0.07%	0.010%
8	3.047	524	531	540	rVB4	1579	2836	0.21%	0.028%
9	3.192	570	576	583	rVB3	383	515	0.04%	0.005%
10	3.440	648	653	658	rVV2	189	222	0.02%	0.002%
11	3.694	727	732	739	rVB2	159	223	0.02%	0.002%
12	3.912	797	800	806	rVB2	176	235	0.02%	0.002%
13	3.951	808	812	816	rVB2	247	218	0.02%	0.002%
14	4.382	944	946	953	rVV2	164	184	0.01%	0.002%
15	4.485	974	978	981	rBV2	198	180	0.01%	0.002%
16	4.632	1004	1024	1072	rBV	146185	388546	28.56%	3.889%
17	4.928	1112	1116	1119	rVB3	258	230	0.02%	0.002%
18	4.951	1119	1123	1128	rVB	282	319	0.02%	0.003%
19	5.067	1143	1159	1183	rBV	234693	520144	38.23%	5.206%
20	5.282	1221	1226	1227	rBV2	297	208	0.02%	0.002%
21	5.295	1227	1230	1234	rVV3	457	502	0.04%	0.005%
22	5.382	1251	1257	1259	rBV3	347	292	0.02%	0.003%
23	5.443	1273	1276	1280	rVB2	199	193	0.01%	0.002%
24	5.472	1280	1285	1289	rVB2	159	212	0.02%	0.002%
25	5.533	1302	1304	1311	rVB2	231	245	0.02%	0.002%
26	5.575	1311	1317	1324	rBV2	225	382	0.03%	0.004%
27	5.729	1343	1365	1394	rBV2	508416	1360573	100.00%	13.618%
28	5.919	1420	1424	1428	rBV3	230	230	0.02%	0.002%
29	5.989	1443	1446	1452	rVB3	304	209	0.02%	0.002%
30	6.015	1452	1454	1458	rBV2	308	269	0.02%	0.003%
31	6.092	1475	1478	1480	rBV2	317	204	0.01%	0.002%
32	6.185	1500	1507	1510	rBV2	262	295	0.02%	0.003%
33	6.253	1512	1528	1551	rBV	343915	641278	47.13%	6.419%
34	6.394	1569	1572	1577	rBV3	195	224	0.02%	0.002%
35	6.439	1581	1586	1592	rBV2	564	684	0.05%	0.007%
36	6.533	1606	1615	1628	rVV4	4042	6691	0.49%	0.067%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045160.D
 Acq On : 05 Oct 2021 21:36
 Operator : SY/MD
 Sample : VU1005WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.697	1651	1666	1688	rBV	317262	616843	45.34%	6.174%
38	6.800	1695	1698	1700	rBV2	375	238	0.02%	0.002%
39	6.951	1740	1745	1752	rVB	219	300	0.02%	0.003%
40	7.054	1765	1777	1784	rBV3	785	1588	0.12%	0.016%
41	7.128	1796	1800	1810	rVV2	131	232	0.02%	0.002%
42	7.189	1810	1819	1830	rVV4	2030	3334	0.25%	0.033%
43	7.308	1851	1856	1859	rBV2	150	179	0.01%	0.002%
44	7.459	1900	1903	1907	rVB2	207	198	0.01%	0.002%
45	7.568	1924	1937	1959	rBV2	168794	296102	21.76%	2.964%
46	7.690	1967	1975	1984	rVV3	1170	1967	0.14%	0.020%
47	7.793	2003	2007	2010	rBV2	307	293	0.02%	0.003%
48	7.902	2026	2041	2056	rBV	611467	1052734	77.37%	10.537%
49	7.970	2057	2062	2081	rVB	9371	16019	1.18%	0.160%
50	8.182	2116	2128	2147	rBV	118180	199111	14.63%	1.993%
51	8.558	2241	2245	2247	rVB	270	210	0.02%	0.002%
52	8.639	2255	2270	2304	rBV	468436	819291	60.22%	8.200%
53	8.828	2326	2329	2333	rBV	200	216	0.02%	0.002%
54	8.951	2362	2367	2372	rBV	222	308	0.02%	0.003%
55	9.237	2452	2456	2461	rVB2	227	268	0.02%	0.003%
56	9.266	2462	2465	2470	rBV2	169	192	0.01%	0.002%
57	9.324	2478	2483	2486	rBV	146	180	0.01%	0.002%
58	9.420	2499	2513	2531	rBV	482881	783611	57.59%	7.843%
59	9.578	2554	2562	2571	rBV3	794	1335	0.10%	0.013%
60	9.693	2592	2598	2599	rBV	1078	929	0.07%	0.009%
61	9.780	2622	2625	2629	rVB2	248	205	0.02%	0.002%
62	9.912	2662	2666	2670	rBV2	267	272	0.02%	0.003%
63	10.044	2703	2707	2712	rBV2	208	303	0.02%	0.003%
64	10.108	2719	2727	2734	rBV5	823	1331	0.10%	0.013%
65	10.385	2808	2813	2816	rVB	277	275	0.02%	0.003%
66	10.414	2816	2822	2825	rVB2	284	321	0.02%	0.003%
67	10.491	2839	2846	2854	rBV2	527	863	0.06%	0.009%
68	10.671	2895	2902	2914	rVB3	3102	4632	0.34%	0.046%
69	10.761	2917	2930	2947	rBV	446278	723300	53.16%	7.240%
70	10.870	2958	2964	2971	rBV4	614	957	0.07%	0.010%
71	10.931	2980	2983	2986	rVB2	332	230	0.02%	0.002%
72	10.999	3001	3004	3009	rBV2	312	235	0.02%	0.002%
73	11.028	3009	3013	3015	rBV	303	278	0.02%	0.003%
74	11.092	3026	3033	3038	rVV2	683	972	0.07%	0.010%
75	11.118	3039	3041	3047	rVV3	582	566	0.04%	0.006%
76	11.150	3048	3051	3053	rVV2	350	230	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045160.D
 Acq On : 05 Oct 2021 21:36
 Operator : SY/MD
 Sample : VU1005WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.163	3053	3055	3059	rVB2	312	194	0.01%	0.002%
78	11.205	3066	3068	3072	rVB	325	217	0.02%	0.002%
79	11.253	3080	3083	3087	rBV2	180	187	0.01%	0.002%
80	11.420	3130	3135	3137	rBV2	207	212	0.02%	0.002%
81	11.462	3137	3148	3160	rVB5	2896	5180	0.38%	0.052%
82	11.697	3213	3221	3231	rVB6	1635	2344	0.17%	0.023%
83	11.748	3231	3237	3245	rBV5	820	1062	0.08%	0.011%
84	11.815	3245	3258	3275	rBV	455550	718069	52.78%	7.187%
85	11.925	3286	3292	3293	rBV2	420	360	0.03%	0.004%
86	11.944	3293	3298	3301	rBV2	1160	1240	0.09%	0.012%
87	12.195	3362	3376	3394	rBV	569765	914330	67.20%	9.152%
88	12.333	3414	3419	3423	rVB3	589	647	0.05%	0.006%
89	12.394	3433	3438	3439	rBV3	343	274	0.02%	0.003%
90	12.504	3468	3472	3475	rBV2	276	303	0.02%	0.003%
91	12.774	3551	3556	3561	rBV	432	489	0.04%	0.005%
92	13.147	3667	3672	3676	rBV4	437	518	0.04%	0.005%
93	13.221	3690	3695	3703	rBV4	1047	1173	0.09%	0.012%
94	13.423	3754	3758	3761	rBV2	214	202	0.01%	0.002%
95	13.610	3807	3816	3818	rBV2	266	431	0.03%	0.004%
96	13.844	3882	3889	3897	rVB4	2183	2742	0.20%	0.027%
97	14.092	3956	3966	3977	rBV	5867	9361	0.69%	0.094%
98	14.333	4034	4041	4047	rBV3	2404	3245	0.24%	0.032%
99	14.536	4099	4104	4107	rBV	244	300	0.02%	0.003%
100	14.581	4113	4118	4125	rBV3	559	773	0.06%	0.008%




Sum of corrected areas: 9990749

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045160.D
Acq On : 05 Oct 2021 21:36
Operator : SY/MD
Sample : VU1005WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

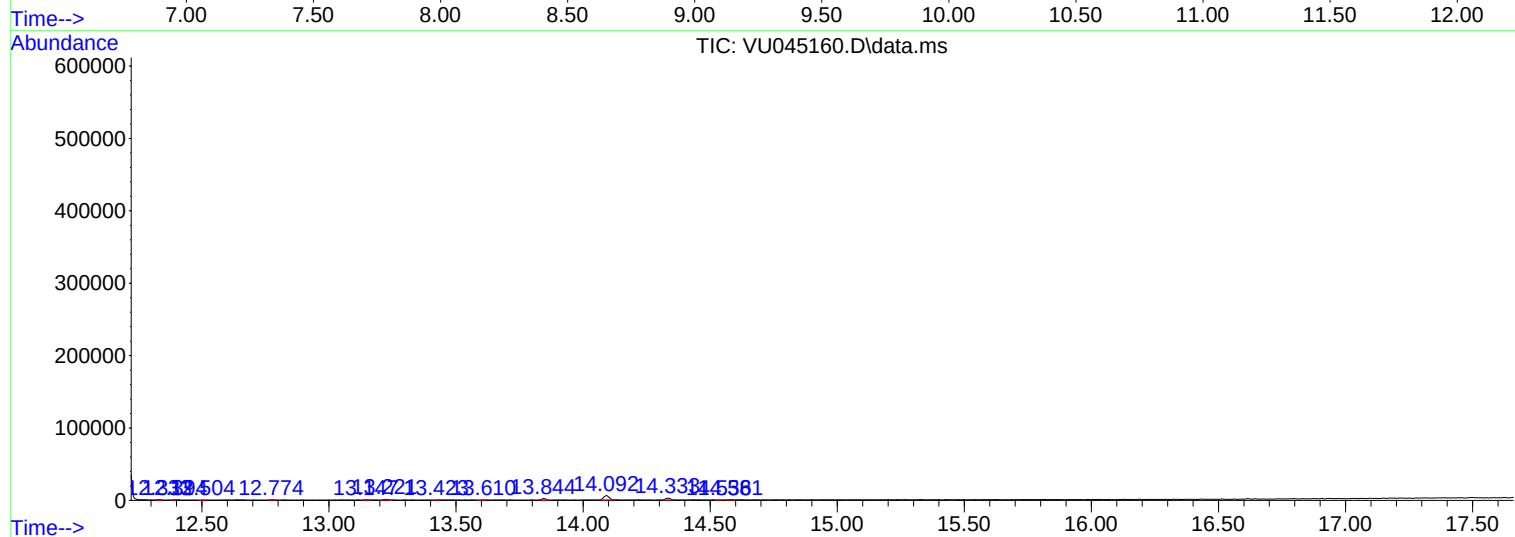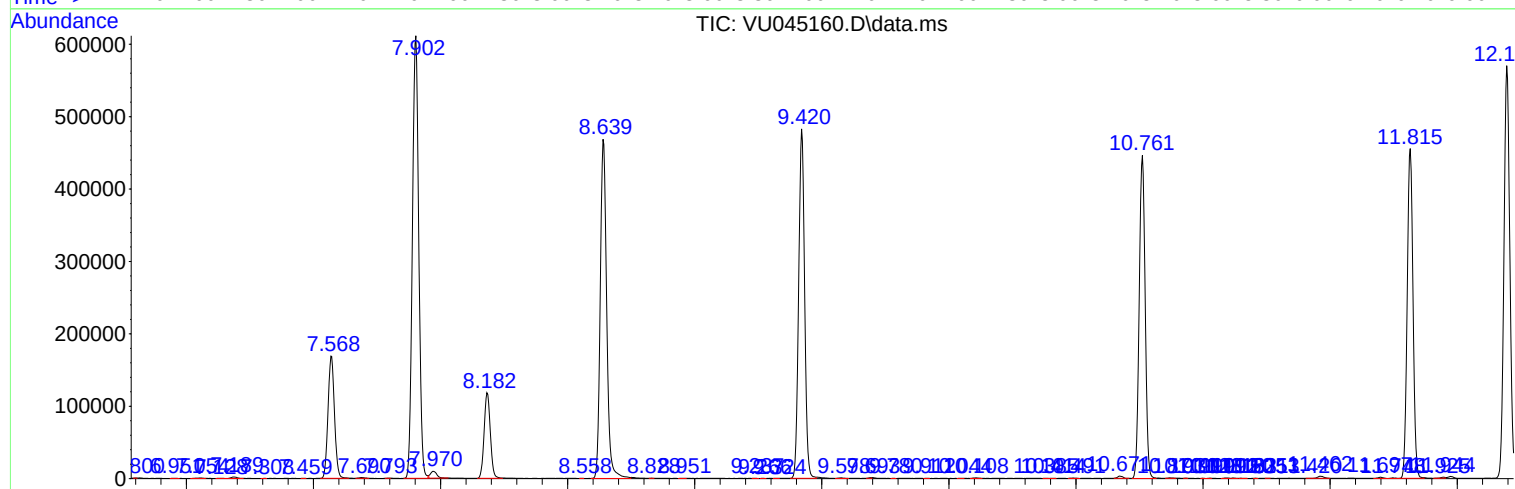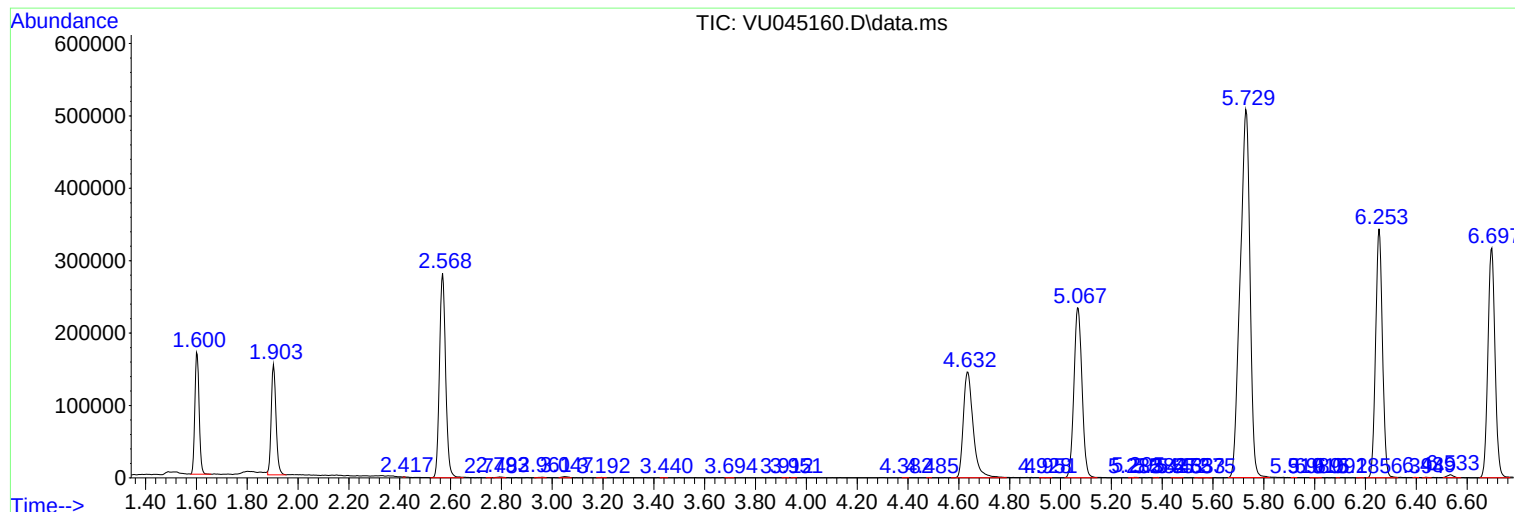

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045160.D
Acq On : 05 Oct 2021 21:36
Operator : SY/MD
Sample : VU1005WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045160.D
Acq On : 05 Oct 2021 21:36
Operator : SY/MD
Sample : VU1005WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
