

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045161.D
 Acq On : 05 Oct 2021 22:00
 Operator : SY/MD
 Sample : M4023-11 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045161.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	94	rVB	159296	185949	12.48%	1.388%
2	1.906	167	176	191	rVB	137270	192909	12.95%	1.440%
3	2.571	369	383	403	rBV3	312147	573848	38.53%	4.284%
4	2.710	423	426	429	rBV	288	217	0.01%	0.002%
5	2.793	447	452	457	rBV2	415	625	0.04%	0.005%
6	2.915	488	490	495	rVB2	230	194	0.01%	0.001%
7	2.957	495	503	506	rBV3	613	870	0.06%	0.006%
8	3.051	517	532	557	rBV	272092	527830	35.44%	3.941%
9	3.189	566	575	587	rBV2	1192	2675	0.18%	0.020%
10	3.353	617	626	628	rBV2	507	579	0.04%	0.004%
11	3.546	683	686	692	rVB2	197	207	0.01%	0.002%
12	3.755	746	751	755	rBV2	255	208	0.01%	0.002%
13	3.819	768	771	775	rBV2	239	172	0.01%	0.001%
14	3.874	775	788	802	rBV	11455	25942	1.74%	0.194%
15	4.067	845	848	853	rVB2	205	171	0.01%	0.001%
16	4.099	853	858	862	rBV2	185	174	0.01%	0.001%
17	4.214	888	894	897	rBV	139	181	0.01%	0.001%
18	4.301	916	921	924	rBV	176	225	0.02%	0.002%
19	4.378	942	945	954	rVB	265	360	0.02%	0.003%
20	4.417	954	957	962	rVB2	245	209	0.01%	0.002%
21	4.671	1006	1036	1072	rBV2	276645	958936	64.38%	7.160%
22	4.922	1110	1114	1117	rVB	222	204	0.01%	0.002%
23	4.944	1118	1121	1125	rBV	224	210	0.01%	0.002%
24	4.976	1128	1131	1132	rBV	283	167	0.01%	0.001%
25	5.070	1143	1160	1187	rBV	236667	523226	35.13%	3.906%
26	5.205	1196	1202	1205	rBV3	370	394	0.03%	0.003%
27	5.321	1221	1238	1255	rBV	168447	376871	25.30%	2.814%
28	5.439	1270	1275	1278	rBV	216	167	0.01%	0.001%
29	5.475	1281	1286	1291	rVB2	208	307	0.02%	0.002%
30	5.729	1343	1365	1384	rBV2	498641	1345564	90.34%	10.046%
31	5.874	1407	1410	1414	rBV	318	261	0.02%	0.002%
32	5.954	1431	1435	1438	rVB3	227	204	0.01%	0.002%
33	6.044	1458	1463	1468	rVB2	453	506	0.03%	0.004%
34	6.111	1481	1484	1485	rVV2	351	186	0.01%	0.001%
35	6.253	1512	1528	1551	rBV	396211	742006	49.82%	5.540%
36	6.546	1604	1619	1646	rBV	800589	1489440	100.00%	11.120%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045161.D
 Acq On : 05 Oct 2021 22:00
 Operator : SY/MD
 Sample : M4023-11 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.697	1651	1666	1686	rVB	315504	616263	41.38%	4.601%
38	6.800	1692	1698	1699	rBV3	538	444	0.03%	0.003%
39	6.870	1714	1720	1723	rBV	342	380	0.03%	0.003%
40	7.050	1769	1776	1784	rVB3	735	1020	0.07%	0.008%
41	7.185	1810	1818	1827	rBV5	2502	4114	0.28%	0.031%
42	7.237	1829	1834	1839	rBV2	223	282	0.02%	0.002%
43	7.568	1924	1937	1960	rVV	172948	304728	20.46%	2.275%
44	7.690	1968	1975	1984	rVB3	1453	2158	0.14%	0.016%
45	7.796	2004	2008	2016	rVB3	383	515	0.03%	0.004%
46	7.902	2027	2041	2056	rBV	606031	1048816	70.42%	7.831%
47	7.973	2057	2063	2074	rVB	10441	17068	1.15%	0.127%
48	8.182	2113	2128	2151	rBV	120540	203657	13.67%	1.521%
49	8.404	2190	2197	2206	rVB4	3030	4543	0.31%	0.034%
50	8.517	2229	2232	2237	rBV2	231	315	0.02%	0.002%
51	8.639	2257	2270	2300	rBV	476904	817578	54.89%	6.104%
52	8.841	2330	2333	2338	rVB2	288	218	0.01%	0.002%
53	9.047	2391	2397	2402	rBV2	232	326	0.02%	0.002%
54	9.169	2431	2435	2438	rVB2	204	193	0.01%	0.001%
55	9.420	2500	2513	2538	rBV	560946	910003	61.10%	6.794%
56	9.574	2554	2561	2570	rVB	1997	2691	0.18%	0.020%
57	9.693	2587	2598	2610	rVB2	7990	12883	0.86%	0.096%
58	9.751	2610	2616	2619	rBV2	194	215	0.01%	0.002%
59	9.825	2635	2639	2643	rBV2	198	225	0.02%	0.002%
60	9.902	2653	2663	2668	rBV2	268	531	0.04%	0.004%
61	10.008	2694	2696	2700	rVB	289	206	0.01%	0.002%
62	10.034	2700	2704	2707	rBV2	190	176	0.01%	0.001%
63	10.105	2717	2726	2735	rVB3	4069	6255	0.42%	0.047%
64	10.301	2784	2787	2791	rBV2	224	204	0.01%	0.002%
65	10.491	2841	2846	2853	rBV3	324	398	0.03%	0.003%
66	10.626	2883	2888	2889	rBV2	202	182	0.01%	0.001%
67	10.674	2895	2903	2910	rVB3	3016	4011	0.27%	0.030%
68	10.761	2917	2930	2950	rVB	449061	717220	48.15%	5.355%
69	10.870	2957	2964	2970	rBV3	369	680	0.05%	0.005%
70	10.928	2977	2982	2989	rVB3	290	378	0.03%	0.003%
71	10.960	2989	2992	2998	rVB	218	192	0.01%	0.001%
72	11.005	3003	3006	3010	rBV	253	220	0.01%	0.002%
73	11.089	3027	3032	3037	rBV2	524	561	0.04%	0.004%
74	11.118	3037	3041	3046	rBV4	442	514	0.03%	0.004%
75	11.182	3058	3061	3065	rBV2	225	218	0.01%	0.002%
76	11.205	3065	3068	3071	rVB2	304	206	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045161.D
 Acq On : 05 Oct 2021 22:00
 Operator : SY/MD
 Sample : M4023-11 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.224	3071	3074	3078	rVB	279	177	0.01%	0.001%
78	11.253	3078	3083	3086	rBV2	289	353	0.02%	0.003%
79	11.468	3139	3150	3158	rBV5	2109	3550	0.24%	0.027%
80	11.587	3180	3187	3193	rVB3	558	812	0.05%	0.006%
81	11.700	3214	3222	3228	rBV5	1141	1749	0.12%	0.013%
82	11.748	3233	3237	3238	rBV3	299	211	0.01%	0.002%
83	11.815	3245	3258	3276	rBV	529630	831466	55.82%	6.208%
84	11.944	3293	3298	3302	rBV2	805	764	0.05%	0.006%
85	12.015	3317	3320	3323	rBV2	264	205	0.01%	0.002%
86	12.195	3359	3376	3398	rBV	568988	913035	61.30%	6.817%
87	12.336	3415	3420	3426	rVB3	563	669	0.04%	0.005%
88	12.487	3462	3467	3468	rBV	196	177	0.01%	0.001%
89	12.594	3496	3500	3503	rBV	197	186	0.01%	0.001%
90	12.835	3572	3575	3580	rVB	306	229	0.02%	0.002%
91	13.063	3641	3646	3649	rBV2	249	290	0.02%	0.002%
92	13.150	3669	3673	3676	rVB2	353	299	0.02%	0.002%
93	13.230	3695	3698	3700	rVB2	330	204	0.01%	0.002%
94	13.745	3854	3858	3862	rBV2	328	283	0.02%	0.002%
95	13.838	3883	3887	3897	rVB3	687	1023	0.07%	0.008%
96	14.024	3940	3945	3947	rBV2	193	213	0.01%	0.002%
97	14.092	3957	3966	3975	rBV2	2434	3631	0.24%	0.027%
98	14.333	4037	4041	4047	rVB3	617	709	0.05%	0.005%
99	14.706	4154	4157	4160	rVB2	351	238	0.02%	0.002%
100	16.564	4732	4735	4736	rBV2	653	409	0.03%	0.003%




Sum of corrected areas: 13393863

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045161.D
Acq On : 05 Oct 2021 22:00
Operator : SY/MD
Sample : M4023-11 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

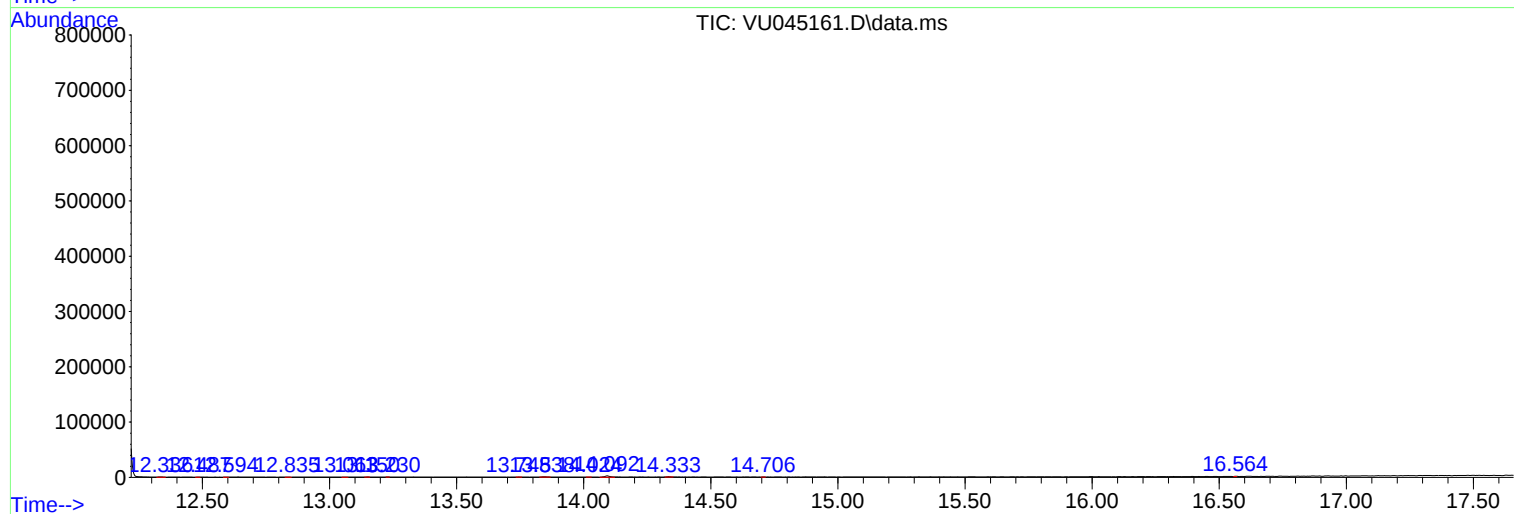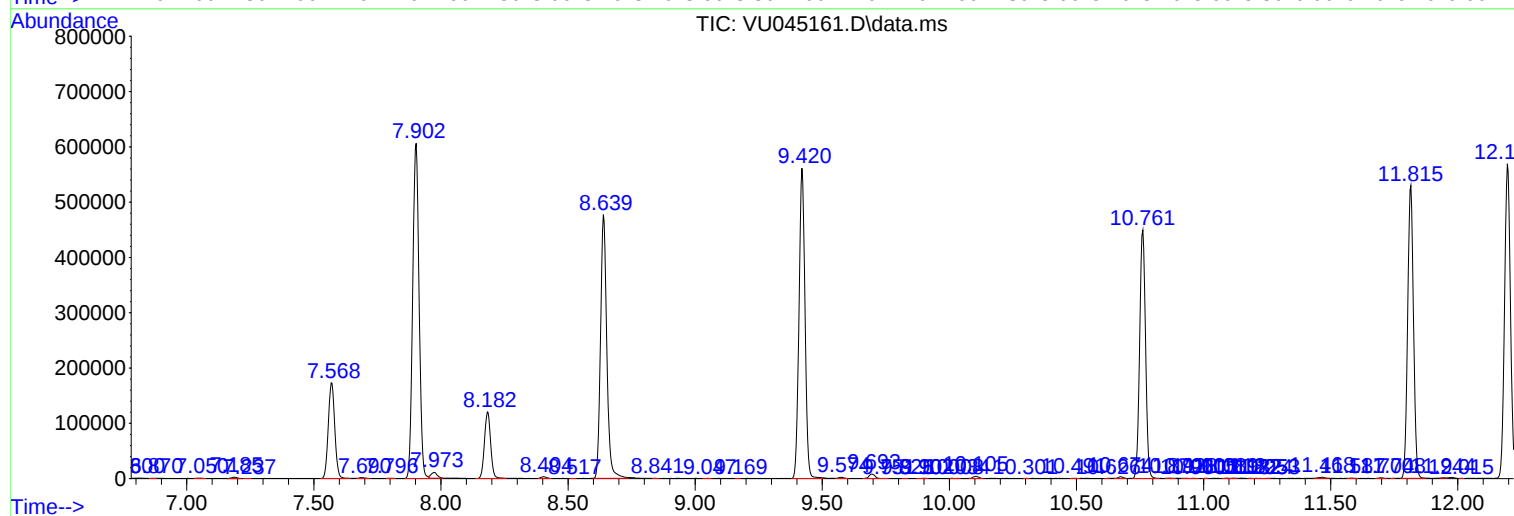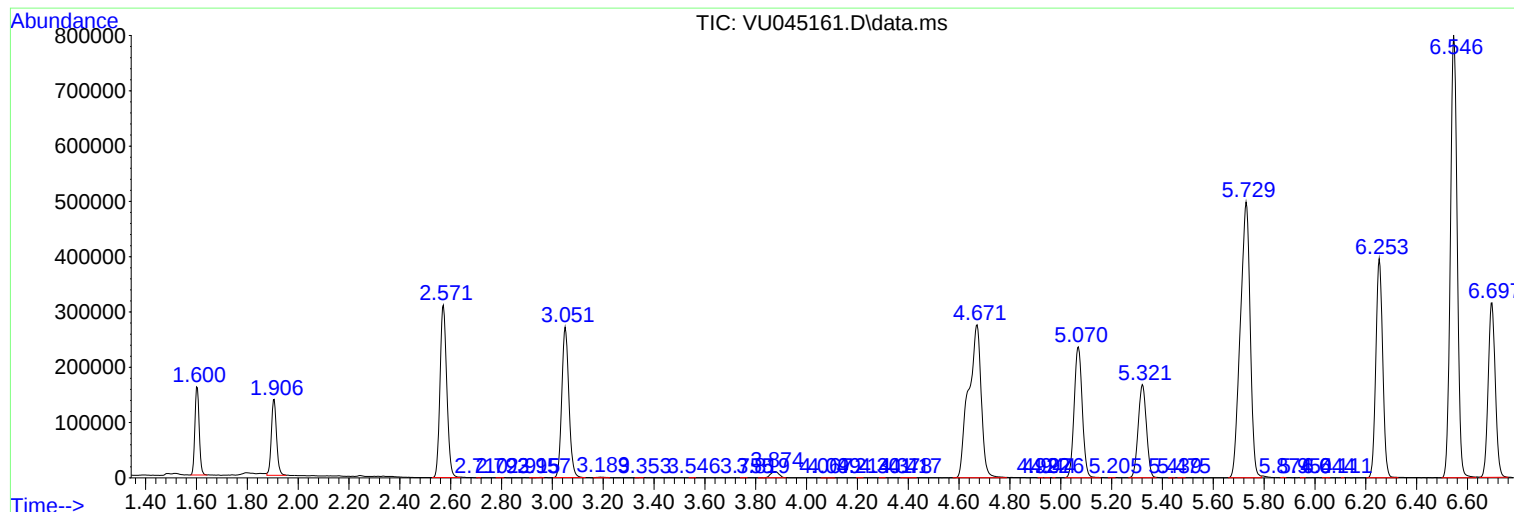

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045161.D
Acq On : 05 Oct 2021 22:00
Operator : SY/MD
Sample : M4023-11 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045161.D
Acq On : 05 Oct 2021 22:00
Operator : SY/MD
Sample : M4023-11 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
