

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045162.D
 Acq On : 05 Oct 2021 22:23
 Operator : SY/MD
 Sample : M4023-12 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU045162.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rBV	156373	182984	12.82%	1.373%
2	1.906	167	176	191	rVB	133424	189652	13.29%	1.424%
3	2.572	369	383	406	rBV3	304868	559014	39.17%	4.196%
4	2.678	413	416	420	rVB3	302	234	0.02%	0.002%
5	2.729	429	432	437	rVB2	267	222	0.02%	0.002%
6	2.771	442	445	448	rBV2	248	216	0.02%	0.002%
7	2.800	448	454	461	rVB2	419	611	0.04%	0.005%
8	2.954	498	502	508	rBV2	385	418	0.03%	0.003%
9	3.051	520	532	551	rVB	42372	80788	5.66%	0.606%
10	3.186	565	574	575	rBV2	1043	1029	0.07%	0.008%
11	3.356	616	627	640	rVB2	13883	27238	1.91%	0.204%
12	3.729	739	743	746	rBV2	146	176	0.01%	0.001%
13	3.874	774	788	805	rVB2	12071	28535	2.00%	0.214%
14	4.250	902	905	908	rBV2	235	180	0.01%	0.001%
15	4.452	960	968	972	rVB2	234	257	0.02%	0.002%
16	4.671	1008	1036	1063	rBV2	484153	1427224	100.00%	10.713%
17	4.870	1096	1098	1104	rVB2	283	232	0.02%	0.002%
18	4.903	1104	1108	1110	rBV3	286	194	0.01%	0.001%
19	4.983	1130	1133	1138	rVB3	253	202	0.01%	0.002%
20	5.067	1142	1159	1186	rBV	240073	526249	36.87%	3.950%
21	5.198	1197	1200	1203	rVB2	328	186	0.01%	0.001%
22	5.221	1203	1207	1209	rBV2	341	202	0.01%	0.002%
23	5.321	1218	1238	1257	rBV	153949	346124	24.25%	2.598%
24	5.729	1343	1365	1394	rBV2	507574	1367464	95.81%	10.264%
25	5.970	1437	1440	1446	rVB2	186	177	0.01%	0.001%
26	6.044	1457	1463	1467	rVB3	417	469	0.03%	0.004%
27	6.115	1483	1485	1488	rBV	200	174	0.01%	0.001%
28	6.253	1512	1528	1553	rBV	385399	727623	50.98%	5.462%
29	6.395	1569	1572	1575	rBV2	232	161	0.01%	0.001%
30	6.546	1603	1619	1643	rBV	760415	1423375	99.73%	10.684%
31	6.697	1651	1666	1685	rVB	321682	622440	43.61%	4.672%
32	6.806	1697	1700	1710	rVB4	884	1143	0.08%	0.009%
33	6.967	1743	1750	1753	rVB2	225	187	0.01%	0.001%
34	7.015	1761	1765	1768	rBV2	231	192	0.01%	0.001%
35	7.041	1768	1773	1775	rBV3	695	663	0.05%	0.005%
36	7.083	1783	1786	1791	rVB	333	244	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045162.D
 Acq On : 05 Oct 2021 22:23
 Operator : SY/MD
 Sample : M4023-12 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.108	1791	1794	1801	rBV2	151	166	0.01%	0.001%
38	7.186	1810	1818	1830	rVB4	2511	3964	0.28%	0.030%
39	7.311	1853	1857	1861	rVB	243	184	0.01%	0.001%
40	7.333	1861	1864	1868	rBV	171	175	0.01%	0.001%
41	7.517	1918	1921	1924	rBV	250	204	0.01%	0.002%
42	7.568	1924	1937	1960	rVV	176491	308197	21.59%	2.313%
43	7.671	1965	1969	1970	rVV2	533	462	0.03%	0.003%
44	7.687	1970	1974	1981	rVV4	1780	2474	0.17%	0.019%
45	7.739	1985	1990	1994	rBV2	165	171	0.01%	0.001%
46	7.803	2007	2010	2013	rBV2	248	177	0.01%	0.001%
47	7.903	2027	2041	2056	rBV	614637	1059019	74.20%	7.949%
48	7.970	2056	2062	2076	rVB2	10002	16795	1.18%	0.126%
49	8.115	2105	2107	2111	rVB	216	163	0.01%	0.001%
50	8.182	2116	2128	2149	rBV	120553	204837	14.35%	1.538%
51	8.404	2187	2197	2206	rBV4	3511	5503	0.39%	0.041%
52	8.472	2213	2218	2226	rBV2	381	631	0.04%	0.005%
53	8.639	2257	2270	2315	rBV	473310	821068	57.53%	6.163%
54	8.896	2347	2350	2356	rVB	175	209	0.01%	0.002%
55	8.976	2373	2375	2381	rVB2	217	190	0.01%	0.001%
56	9.247	2454	2459	2461	rBV	213	213	0.01%	0.002%
57	9.292	2468	2473	2475	rBV2	264	296	0.02%	0.002%
58	9.420	2499	2513	2544	rBV	547945	895422	62.74%	6.721%
59	9.571	2554	2560	2571	rBV3	793	1172	0.08%	0.009%
60	9.693	2591	2598	2609	rVB4	3070	4508	0.32%	0.034%
61	9.806	2628	2633	2636	rBV	236	212	0.01%	0.002%
62	9.845	2636	2645	2652	rBV2	180	455	0.03%	0.003%
63	9.983	2683	2688	2691	rBV	285	306	0.02%	0.002%
64	10.105	2716	2726	2734	rBV3	2793	3882	0.27%	0.029%
65	10.259	2770	2774	2781	rVB2	224	295	0.02%	0.002%
66	10.304	2784	2788	2793	rBV2	191	209	0.01%	0.002%
67	10.330	2793	2796	2802	rVB2	198	245	0.02%	0.002%
68	10.398	2811	2817	2820	rBV2	259	328	0.02%	0.002%
69	10.558	2864	2867	2872	rBV2	271	262	0.02%	0.002%
70	10.674	2895	2903	2916	rVB3	3238	4772	0.33%	0.036%
71	10.761	2916	2930	2948	rBV	448892	728852	51.07%	5.471%
72	10.877	2958	2966	2972	rBV5	633	986	0.07%	0.007%
73	10.925	2977	2981	2985	rVB2	270	280	0.02%	0.002%
74	11.118	3038	3041	3046	rVB3	426	447	0.03%	0.003%
75	11.372	3113	3120	3121	rBV3	252	235	0.02%	0.002%
76	11.462	3139	3148	3157	rVV6	2202	3559	0.25%	0.027%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045162.D
 Acq On : 05 Oct 2021 22:23
 Operator : SY/MD
 Sample : M4023-12 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.581	3180	3185	3188	rBV2	366	489	0.03%	0.004%
78	11.642	3201	3204	3207	rBV	205	179	0.01%	0.001%
79	11.697	3212	3221	3227	rBV3	1193	1553	0.11%	0.012%
80	11.816	3245	3258	3280	rBV	521466	807692	56.59%	6.063%
81	11.893	3280	3282	3288	rVB	327	209	0.01%	0.002%
82	11.941	3293	3297	3302	rVV3	1216	1614	0.11%	0.012%
83	11.973	3302	3307	3317	rVB5	1718	2605	0.18%	0.020%
84	12.195	3358	3376	3398	rBV	563601	914539	64.08%	6.865%
85	12.330	3415	3418	3430	rVB6	731	944	0.07%	0.007%
86	12.391	3433	3437	3440	rBV	270	256	0.02%	0.002%
87	12.526	3476	3479	3482	rBV2	179	174	0.01%	0.001%
88	12.584	3494	3497	3501	rBV	256	234	0.02%	0.002%
89	12.629	3506	3511	3515	rBV3	382	504	0.04%	0.004%
90	12.716	3535	3538	3542	rBV	229	243	0.02%	0.002%
91	13.262	3705	3708	3711	rBV	207	161	0.01%	0.001%
92	13.822	3880	3882	3887	rBV2	148	162	0.01%	0.001%
93	13.922	3910	3913	3918	rBV2	214	269	0.02%	0.002%
94	14.092	3961	3966	3977	rBV2	921	1267	0.09%	0.010%
95	14.169	3987	3990	3992	rBV	208	165	0.01%	0.001%
96	14.568	4112	4114	4118	rVB2	342	217	0.02%	0.002%
97	14.915	4219	4222	4223	rBV2	360	237	0.02%	0.002%
98	14.986	4236	4244	4247	rBV3	269	440	0.03%	0.003%
99	15.352	4354	4358	4361	rBV2	368	295	0.02%	0.002%
100	15.921	4532	4535	4538	rBV3	337	275	0.02%	0.002%




Sum of corrected areas: 13322727

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045162.D
Acq On : 05 Oct 2021 22:23
Operator : SY/MD
Sample : M4023-12 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

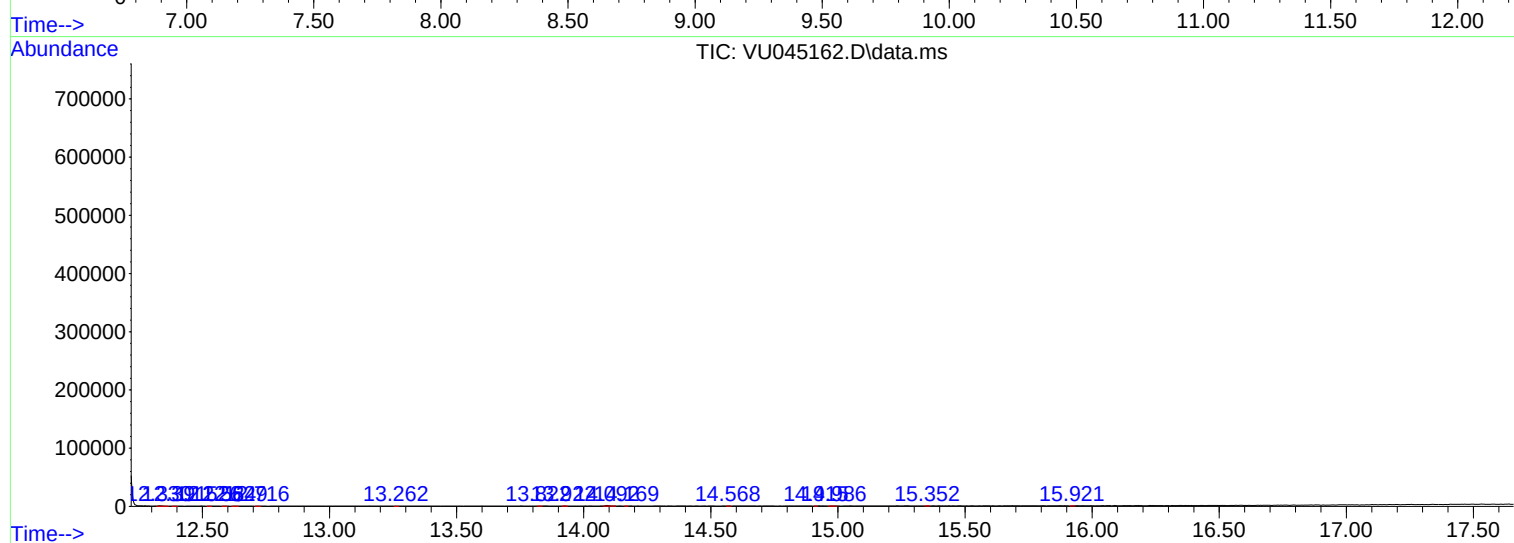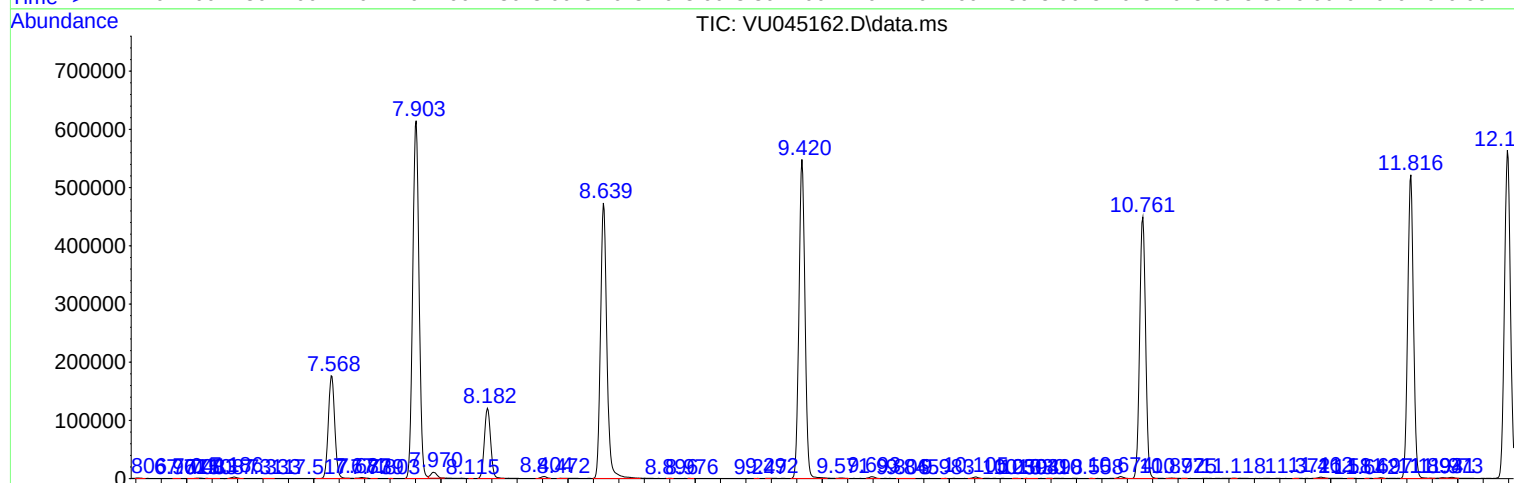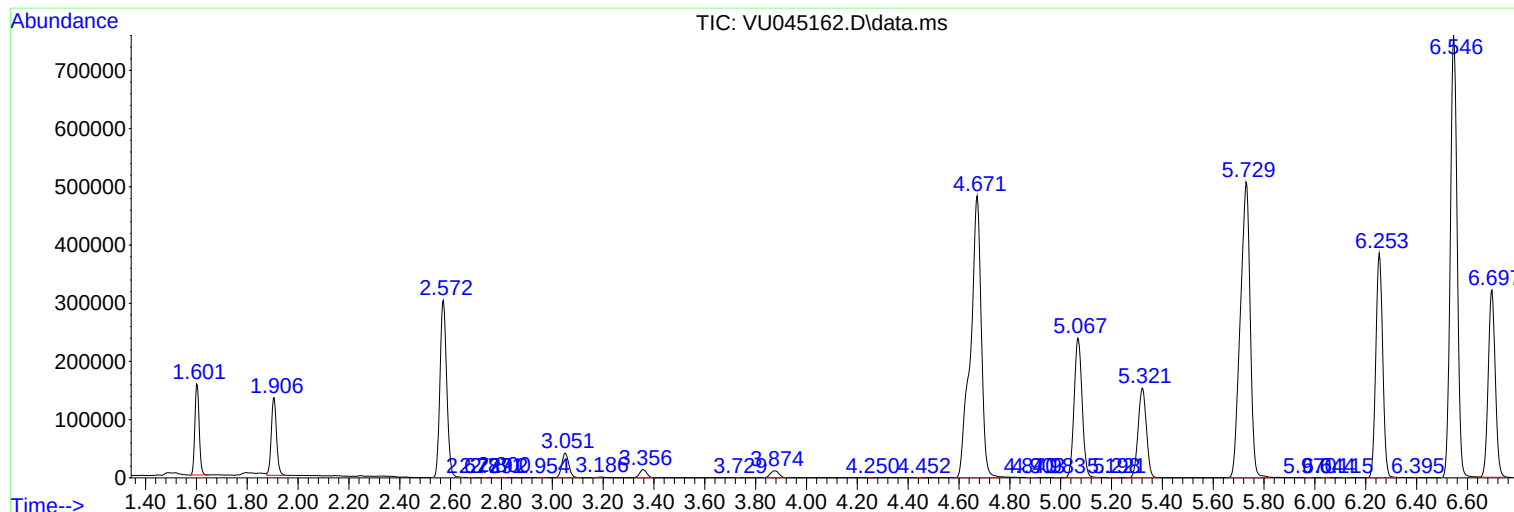

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045162.D
Acq On : 05 Oct 2021 22:23
Operator : SY/MD
Sample : M4023-12 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045162.D
Acq On : 05 Oct 2021 22:23
Operator : SY/MD
Sample : M4023-12 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
