

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045164.D
 Acq On : 05 Oct 2021 23:10
 Operator : SY/MD
 Sample : M4023-04 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045164.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	97	rVB	155057	177947	13.54%	1.536%
2	1.912	170	178	194	rVB	132306	179421	13.66%	1.549%
3	2.571	370	383	407	rBV2	284322	505183	38.45%	4.361%
4	2.925	487	493	495	rBV2	202	273	0.02%	0.002%
5	3.051	521	532	553	rVB	33088	63464	4.83%	0.548%
6	3.153	561	564	567	rBV	157	135	0.01%	0.001%
7	3.189	567	575	578	rBV2	967	1362	0.10%	0.012%
8	3.279	598	603	606	rBV	181	196	0.01%	0.002%
9	3.356	621	627	630	rBV	331	356	0.03%	0.003%
10	3.378	631	634	637	rVB	195	130	0.01%	0.001%
11	3.404	637	642	646	rBV	197	195	0.01%	0.002%
12	3.452	655	657	658	rBV	153	83	0.01%	0.001%
13	3.533	679	682	685	rBV2	185	152	0.01%	0.001%
14	3.549	685	687	689	rBV	132	97	0.01%	0.001%
15	3.629	709	712	714	rBV	152	93	0.01%	0.001%
16	3.681	724	728	730	rBV	132	91	0.01%	0.001%
17	3.706	734	736	739	rBV	138	112	0.01%	0.001%
18	3.745	747	748	754	rBV2	139	108	0.01%	0.001%
19	3.800	762	765	769	rBV	169	170	0.01%	0.001%
20	3.838	775	777	779	rBV2	174	96	0.01%	0.001%
21	3.951	807	812	815	rBV2	223	208	0.02%	0.002%
22	3.996	823	826	830	rBV	196	121	0.01%	0.001%
23	4.038	832	839	842	rBV2	168	206	0.02%	0.002%
24	4.105	857	860	863	rBV2	211	151	0.01%	0.001%
25	4.153	872	875	879	rBV2	193	147	0.01%	0.001%
26	4.179	879	883	887	rBV2	184	258	0.02%	0.002%
27	4.234	895	900	903	rVB	175	192	0.01%	0.002%
28	4.256	903	907	910	rBV2	133	135	0.01%	0.001%
29	4.304	918	922	925	rVB2	180	163	0.01%	0.001%
30	4.443	962	965	969	rVB	221	175	0.01%	0.002%
31	4.472	971	974	977	rBV2	208	196	0.01%	0.002%
32	4.507	982	985	988	rBV	110	83	0.01%	0.001%
33	4.536	991	994	1001	rBV2	198	311	0.02%	0.003%
34	4.632	1008	1024	1062	rBV	145928	453477	34.52%	3.914%
35	4.986	1127	1134	1138	rBV3	241	253	0.02%	0.002%
36	5.070	1142	1160	1189	rVV	231112	509180	38.76%	4.395%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045164.D
 Acq On : 05 Oct 2021 23:10
 Operator : SY/MD
 Sample : M4023-04 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.198	1194	1200	1203	rBV3	371	404	0.03%	0.003%
38	5.266	1215	1221	1224	rBV2	340	365	0.03%	0.003%
39	5.321	1224	1238	1261	rVB	64921	146044	11.12%	1.261%
40	5.417	1265	1268	1271	rBV2	159	135	0.01%	0.001%
41	5.452	1275	1279	1282	rBV	204	217	0.02%	0.002%
42	5.542	1304	1307	1310	rBV	146	115	0.01%	0.001%
43	5.639	1334	1337	1341	rVB2	204	153	0.01%	0.001%
44	5.729	1341	1365	1393	rBV2	481185	1313808	100.00%	11.341%
45	6.253	1514	1528	1553	rBV	384940	723969	55.10%	6.249%
46	6.546	1604	1619	1640	rBV	692427	1297491	98.76%	11.200%
47	6.697	1652	1666	1683	rVB	305716	597012	45.44%	5.153%
48	7.054	1769	1777	1784	rVB3	711	1146	0.09%	0.010%
49	7.089	1784	1788	1792	rVB2	265	251	0.02%	0.002%
50	7.121	1792	1798	1800	rBV2	216	217	0.02%	0.002%
51	7.182	1811	1817	1829	rVB4	1912	3081	0.23%	0.027%
52	7.291	1849	1851	1854	rVB	181	102	0.01%	0.001%
53	7.333	1858	1864	1867	rBV2	173	175	0.01%	0.002%
54	7.382	1875	1879	1880	rBV	186	117	0.01%	0.001%
55	7.507	1914	1918	1922	rBV	240	236	0.02%	0.002%
56	7.571	1924	1938	1954	rBV	164910	290990	22.15%	2.512%
57	7.690	1966	1975	1987	rVB4	1369	2528	0.19%	0.022%
58	7.902	2027	2041	2056	rBV	587019	1008515	76.76%	8.705%
59	8.182	2115	2128	2149	rBV	115486	195980	14.92%	1.692%
60	8.369	2181	2186	2190	rBV2	193	181	0.01%	0.002%
61	8.398	2190	2195	2196	rBV2	540	378	0.03%	0.003%
62	8.500	2224	2227	2233	rBV2	202	216	0.02%	0.002%
63	8.639	2257	2270	2318	rBV	460754	801078	60.97%	6.915%
64	8.867	2339	2341	2343	rBV	165	105	0.01%	0.001%
65	8.909	2350	2354	2356	rBV	221	186	0.01%	0.002%
66	8.992	2372	2380	2382	rBV2	306	353	0.03%	0.003%
67	9.021	2387	2389	2393	rVB	187	110	0.01%	0.001%
68	9.060	2399	2401	2403	rBV	181	103	0.01%	0.001%
69	9.156	2426	2431	2435	rBV	239	202	0.02%	0.002%
70	9.179	2435	2438	2440	rBV	202	134	0.01%	0.001%
71	9.227	2448	2453	2454	rBV2	177	172	0.01%	0.001%
72	9.288	2470	2472	2474	rBV	137	99	0.01%	0.001%
73	9.365	2493	2496	2499	rBV	146	112	0.01%	0.001%
74	9.420	2499	2513	2542	rBV	537878	890221	67.76%	7.684%
75	9.571	2553	2560	2569	rBV2	2231	3241	0.25%	0.028%
76	9.693	2588	2598	2612	rBV2	10046	15808	1.20%	0.136%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045164.D
 Acq On : 05 Oct 2021 23:10
 Operator : SY/MD
 Sample : M4023-04 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

77	9.767	2618	2621	2623	rBV	145	108	0.01%	0.001%
78	9.796	2627	2630	2634	rVB2	218	172	0.01%	0.001%
79	9.909	2660	2665	2668	rBV2	189	202	0.02%	0.002%
80	9.928	2668	2671	2673	rVV2	175	138	0.01%	0.001%
81	9.957	2677	2680	2684	rBV	129	130	0.01%	0.001%
82	10.053	2705	2710	2713	rBV2	193	167	0.01%	0.001%
83	10.105	2716	2726	2738	rVV2	5027	7340	0.56%	0.063%
84	10.198	2753	2755	2758	rVB2	227	131	0.01%	0.001%
85	10.221	2758	2762	2764	rBV2	261	249	0.02%	0.002%
86	10.613	2882	2884	2887	rBV	140	122	0.01%	0.001%
87	10.674	2896	2903	2911	rVB2	2519	3805	0.29%	0.033%
88	10.761	2917	2930	2952	rBV	429573	682590	51.96%	5.892%
89	10.873	2958	2965	2969	rBV2	636	706	0.05%	0.006%
90	10.983	2993	2999	3001	rBV2	242	282	0.02%	0.002%
91	11.031	3012	3014	3019	rVB	264	158	0.01%	0.001%
92	11.121	3038	3042	3047	rVB4	594	544	0.04%	0.005%
93	11.314	3099	3102	3104	rBV2	158	110	0.01%	0.001%
94	11.462	3139	3148	3157	rBV5	1723	3347	0.25%	0.029%
95	11.700	3217	3222	3237	rVB4	1159	1473	0.11%	0.013%
96	11.815	3245	3258	3274	rBV	509764	813690	61.93%	7.024%
97	12.195	3363	3376	3394	rBV	544661	877996	66.83%	7.579%
98	12.841	3572	3577	3579	rBV2	260	257	0.02%	0.002%
99	13.565	3797	3802	3806	rVB2	302	321	0.02%	0.003%
100	13.593	3806	3811	3816	rBV2	291	357	0.03%	0.003%




Sum of corrected areas: 11585065

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045164.D
Acq On : 05 Oct 2021 23:10
Operator : SY/MD
Sample : M4023-04 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

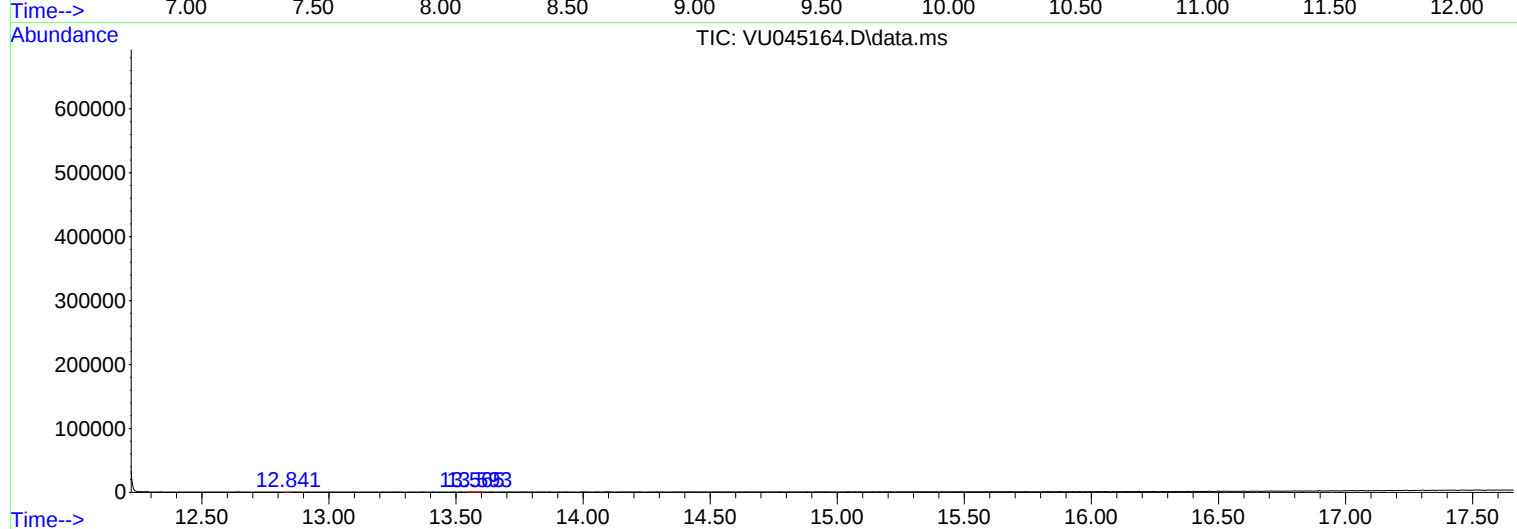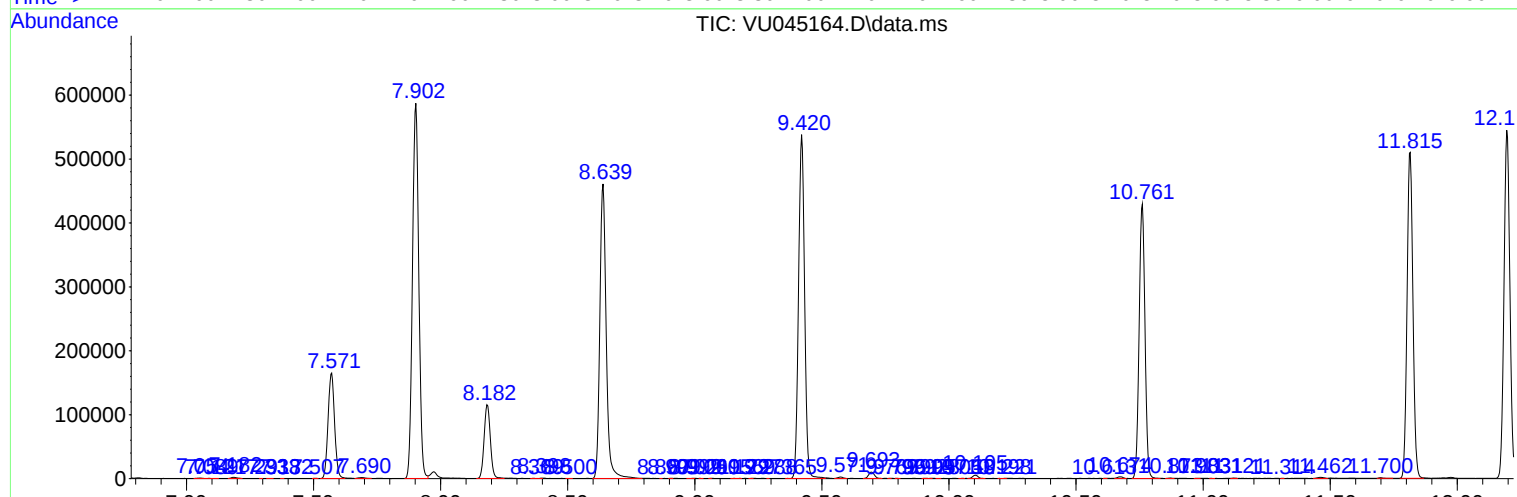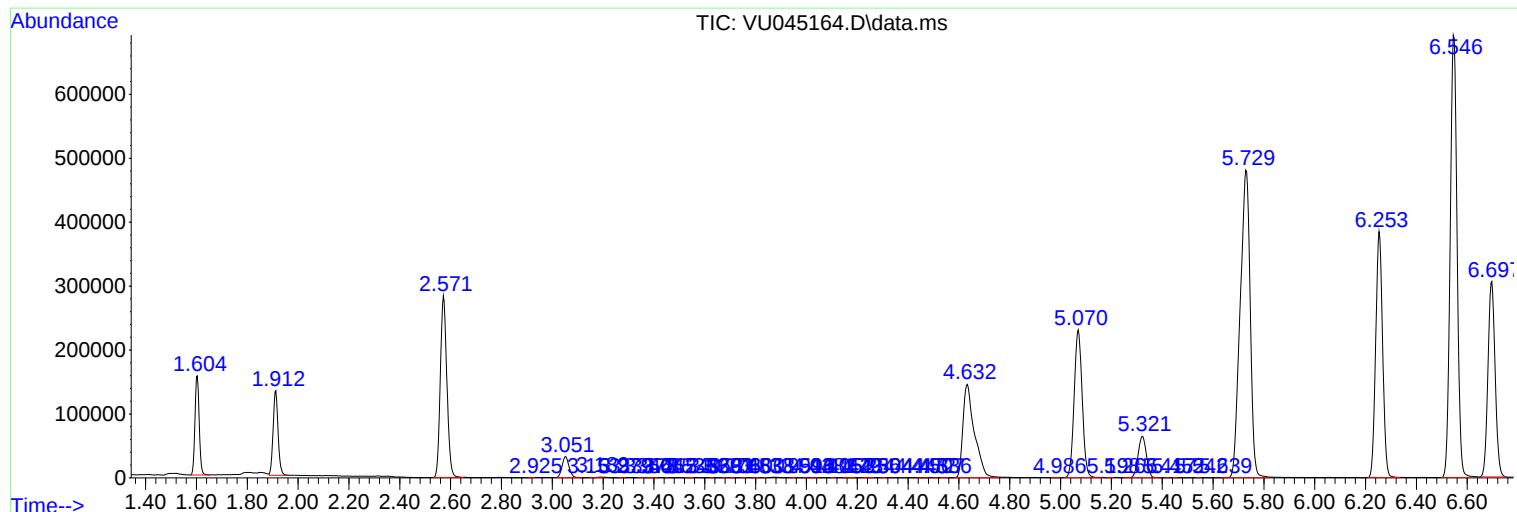

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045164.D
Acq On : 05 Oct 2021 23:10
Operator : SY/MD
Sample : M4023-04 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045164.D
Acq On : 05 Oct 2021 23:10
Operator : SY/MD
Sample : M4023-04 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
