

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045165.D
 Acq On : 05 Oct 2021 23:33
 Operator : SY/MD
 Sample : M3996-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.909	171	177	194	rVB	148045	198346	14.92%	1.857%
2	2.568	370	382	399	rBV	262735	442506	33.29%	4.144%
3	3.761	750	753	754	rBV	157	93	0.01%	0.001%
4	3.806	764	767	772	rVB	222	204	0.02%	0.002%
5	3.841	775	778	782	rBV2	183	188	0.01%	0.002%
6	3.886	789	792	795	rBV	143	145	0.01%	0.001%
7	3.986	821	823	827	rVB2	214	164	0.01%	0.002%
8	4.012	827	831	832	rBV	140	87	0.01%	0.001%
9	4.022	832	834	839	rVB	215	141	0.01%	0.001%
10	4.047	839	842	845	rBV2	162	101	0.01%	0.001%
11	4.063	845	847	850	rBV	156	115	0.01%	0.001%
12	4.112	859	862	865	rBV2	153	87	0.01%	0.001%
13	4.124	865	866	870	rVB	127	90	0.01%	0.001%
14	4.163	874	878	880	rBV2	198	168	0.01%	0.002%
15	4.237	896	901	905	rBV2	159	198	0.01%	0.002%
16	4.308	915	923	925	rBV2	222	323	0.02%	0.003%
17	4.337	929	932	934	rVB	132	96	0.01%	0.001%
18	4.359	934	939	941	rBV	191	206	0.02%	0.002%
19	4.475	970	975	977	rBV2	188	210	0.02%	0.002%
20	4.636	1009	1025	1067	rBV	140387	401221	30.18%	3.757%
21	4.986	1132	1134	1136	rBV2	235	126	0.01%	0.001%
22	5.070	1142	1160	1183	rBV	234648	514756	38.72%	4.820%
23	5.288	1224	1228	1229	rBV	423	284	0.02%	0.003%
24	5.369	1249	1253	1256	rBV	152	141	0.01%	0.001%
25	5.407	1262	1265	1268	rBV	199	146	0.01%	0.001%
26	5.475	1283	1286	1288	rBV	172	115	0.01%	0.001%
27	5.597	1317	1324	1327	rBV	206	301	0.02%	0.003%
28	5.729	1343	1365	1388	rBV2	491937	1329400	100.00%	12.448%
29	6.108	1481	1483	1484	rBV	256	113	0.01%	0.001%
30	6.156	1494	1498	1500	rBV2	145	107	0.01%	0.001%
31	6.189	1506	1508	1511	rBV2	111	90	0.01%	0.001%
32	6.253	1512	1528	1547	rBV	395565	738737	55.57%	6.917%
33	6.546	1608	1619	1632	rVB5	8292	15589	1.17%	0.146%
34	6.597	1632	1635	1640	rBV3	240	213	0.02%	0.002%
35	6.697	1651	1666	1691	rBV	312809	610685	45.94%	5.718%
36	7.009	1760	1763	1766	rVB2	243	188	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045165.D
 Acq On : 05 Oct 2021 23:33
 Operator : SY/MD
 Sample : M3996-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.050	1766	1776	1782	rBV4	737	1341	0.10%	0.013%
38	7.111	1786	1795	1803	rVV4	2028	3125	0.24%	0.029%
39	7.189	1811	1819	1829	rVB4	1963	3284	0.25%	0.031%
40	7.369	1867	1875	1877	rBV	187	209	0.02%	0.002%
41	7.388	1878	1881	1884	rBV	200	126	0.01%	0.001%
42	7.478	1905	1909	1911	rBV	174	110	0.01%	0.001%
43	7.504	1914	1917	1922	rVB2	196	137	0.01%	0.001%
44	7.571	1924	1938	1957	rBV	165538	293435	22.07%	2.748%
45	7.693	1969	1976	1984	rVB3	1489	2319	0.17%	0.022%
46	7.758	1995	1996	1999	rBV	142	92	0.01%	0.001%
47	7.771	1999	2000	2003	rVB	230	97	0.01%	0.001%
48	7.800	2003	2009	2014	rBV3	503	528	0.04%	0.005%
49	7.902	2023	2041	2056	rBV	592573	1020878	76.79%	9.559%
50	8.182	2116	2128	2146	rBV	114061	196015	14.74%	1.835%
51	8.317	2165	2170	2174	rVB2	288	218	0.02%	0.002%
52	8.362	2179	2184	2186	rBV2	219	239	0.02%	0.002%
53	8.433	2203	2206	2209	rVB2	144	92	0.01%	0.001%
54	8.459	2211	2214	2216	rVB2	192	111	0.01%	0.001%
55	8.481	2216	2221	2223	rBV	310	366	0.03%	0.003%
56	8.510	2227	2230	2232	rBV2	177	126	0.01%	0.001%
57	8.555	2232	2244	2258	rVV	449771	752060	56.57%	7.042%
58	8.639	2259	2270	2316	rVB	461263	812891	61.15%	7.612%
59	8.899	2348	2351	2354	rVB	235	130	0.01%	0.001%
60	8.944	2362	2365	2369	rBV2	153	185	0.01%	0.002%
61	8.996	2378	2381	2383	rBV	225	150	0.01%	0.001%
62	9.063	2399	2402	2404	rBV2	194	138	0.01%	0.001%
63	9.092	2409	2411	2414	rBV2	194	132	0.01%	0.001%
64	9.121	2416	2420	2422	rBV2	117	90	0.01%	0.001%
65	9.144	2422	2427	2431	rVB2	226	254	0.02%	0.002%
66	9.253	2458	2461	2468	rVB	228	235	0.02%	0.002%
67	9.288	2468	2472	2474	rBV	175	150	0.01%	0.001%
68	9.353	2489	2492	2495	rBV2	207	132	0.01%	0.001%
69	9.420	2500	2513	2546	rBV	552772	904956	68.07%	8.474%
70	9.571	2556	2560	2566	rVV2	461	515	0.04%	0.005%
71	9.600	2566	2569	2575	rVB2	240	225	0.02%	0.002%
72	9.748	2611	2615	2618	rBV2	184	177	0.01%	0.002%
73	9.819	2634	2637	2642	rBV	157	156	0.01%	0.001%
74	9.931	2669	2672	2677	rVB	238	149	0.01%	0.001%
75	9.957	2677	2680	2682	rBV2	220	141	0.01%	0.001%
76	9.996	2688	2692	2696	rBV	174	137	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045165.D
 Acq On : 05 Oct 2021 23:33
 Operator : SY/MD
 Sample : M3996-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.102	2721	2725	2726	rBV	486	345	0.03%	0.003%
78	10.169	2743	2746	2748	rVB	227	118	0.01%	0.001%
79	10.195	2748	2754	2756	rBV2	195	222	0.02%	0.002%
80	10.237	2763	2767	2768	rBV2	249	173	0.01%	0.002%
81	10.311	2788	2790	2793	rBV2	164	95	0.01%	0.001%
82	10.397	2815	2817	2820	rVB	191	87	0.01%	0.001%
83	10.423	2822	2825	2834	rVB	241	217	0.02%	0.002%
84	10.465	2836	2838	2841	rVB2	166	95	0.01%	0.001%
85	10.488	2842	2845	2850	rVB	168	123	0.01%	0.001%
86	10.674	2893	2903	2911	rBV3	2862	4334	0.33%	0.041%
87	10.761	2916	2930	2946	rBV	442923	706121	53.12%	6.612%
88	11.124	3039	3043	3049	rBV3	550	618	0.05%	0.006%
89	11.208	3065	3069	3070	rBV	314	229	0.02%	0.002%
90	11.336	3106	3109	3112	rVB2	277	203	0.02%	0.002%
91	11.462	3141	3148	3159	rVB5	2070	3434	0.26%	0.032%
92	11.520	3161	3166	3169	rBV2	164	143	0.01%	0.001%
93	11.545	3169	3174	3178	rVB2	218	244	0.02%	0.002%
94	11.574	3179	3183	3184	rBV	182	113	0.01%	0.001%
95	11.642	3202	3204	3208	rBV2	154	144	0.01%	0.001%
96	11.703	3216	3223	3231	rVB5	1014	1495	0.11%	0.014%
97	11.815	3245	3258	3280	rBV	526314	820892	61.75%	7.687%
98	11.950	3291	3300	3303	rBV5	1073	1684	0.13%	0.016%
99	12.195	3363	3376	3397	rBV	558999	886460	66.68%	8.301%
100	12.687	3525	3529	3533	rBV2	214	201	0.02%	0.002%




Sum of corrected areas: 10679321

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045165.D
Acq On : 05 Oct 2021 23:33
Operator : SY/MD
Sample : M3996-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

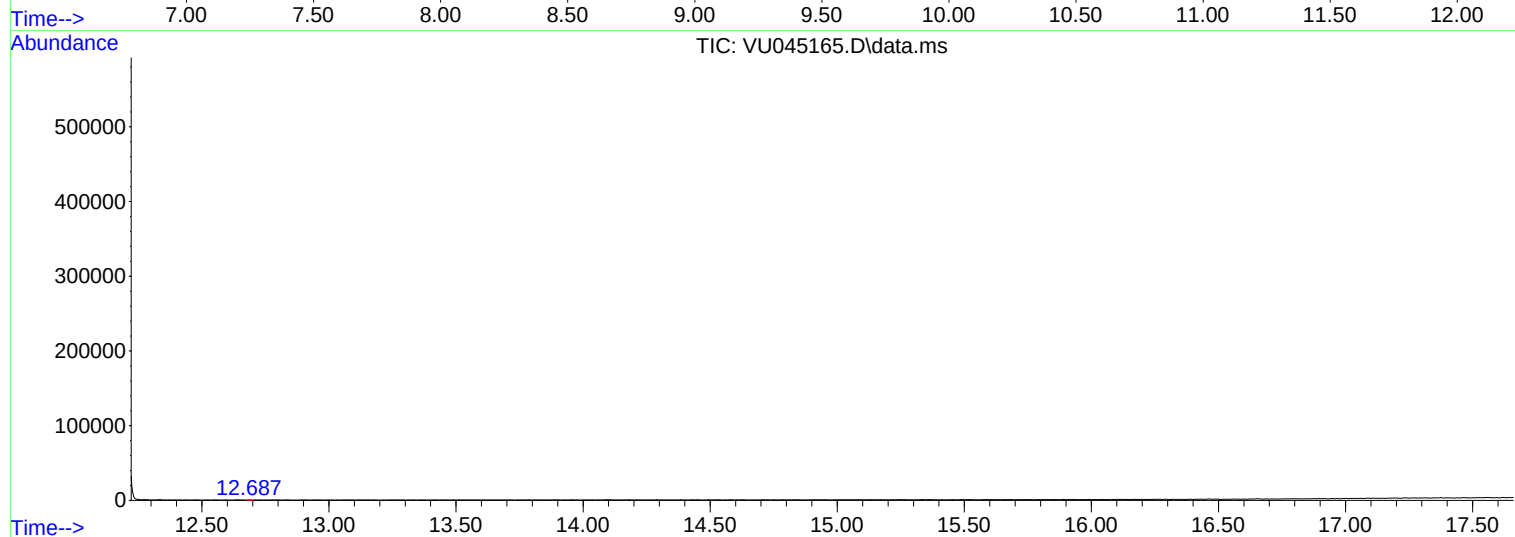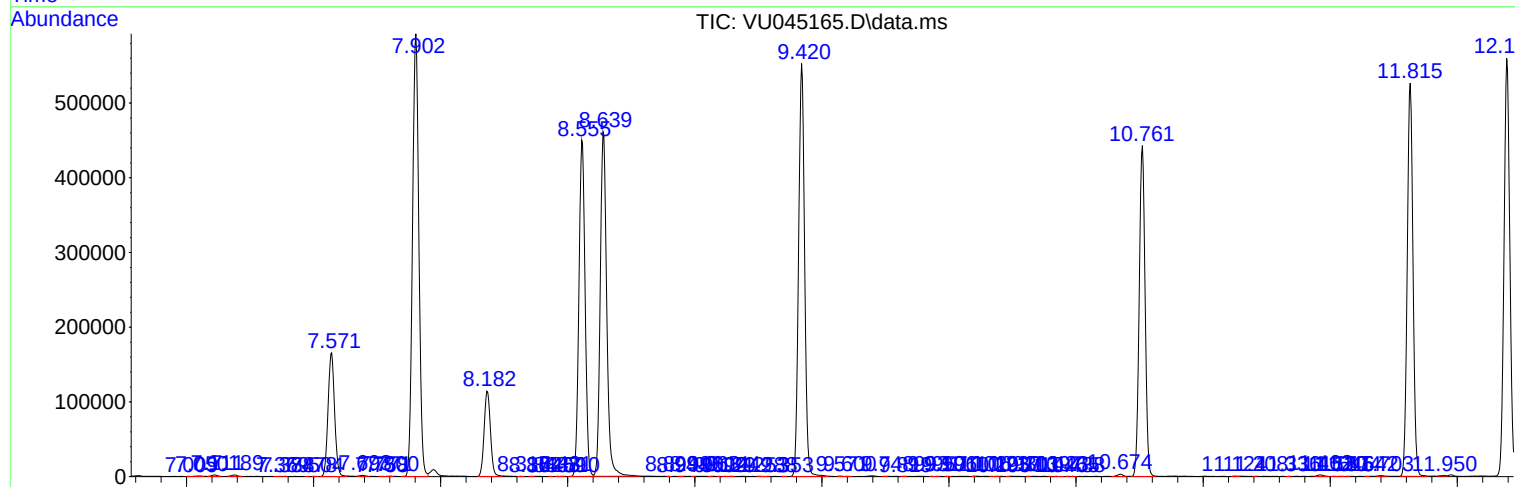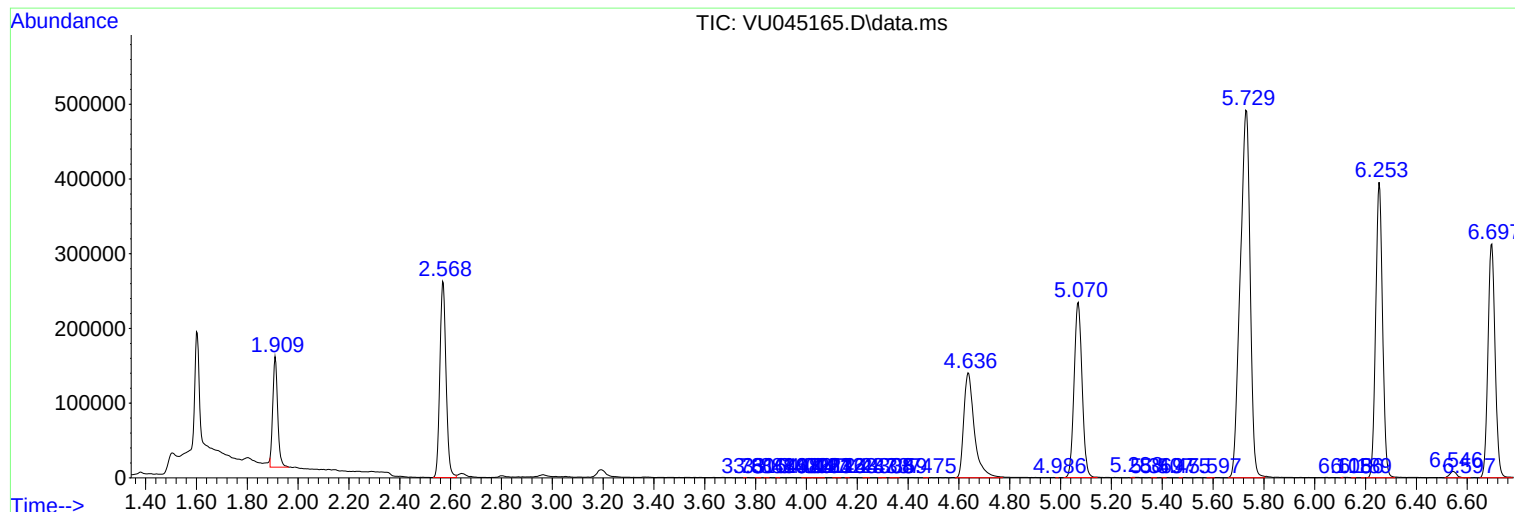

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045165.D
Acq On : 05 Oct 2021 23:33
Operator : SY/MD
Sample : M3996-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045165.D
Acq On : 05 Oct 2021 23:33
Operator : SY/MD
Sample : M3996-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
