

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045169.D
 Acq On : 06 Oct 2021 01:06
 Operator : SY/MD
 Sample : M3996-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU045169.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	76	82	97	rVB	146030	165687	9.61%	1.444%
2	1.916	171	179	193	rVB	130179	178399	10.35%	1.555%
3	2.572	371	383	401	rBV	257443	427395	24.79%	3.725%
4	2.700	420	423	426	rVB2	212	123	0.01%	0.001%
5	2.723	426	430	433	rBV	168	173	0.01%	0.002%
6	2.964	499	505	510	rVB3	444	674	0.04%	0.006%
7	2.990	510	513	517	rVB2	215	180	0.01%	0.002%
8	3.028	518	525	527	rBV	233	253	0.01%	0.002%
9	3.047	529	531	539	rVB3	368	304	0.02%	0.003%
10	3.083	539	542	545	rBV2	169	133	0.01%	0.001%
11	3.141	557	560	562	rBV2	196	121	0.01%	0.001%
12	3.192	562	576	595	rVV2	11004	25789	1.50%	0.225%
13	3.369	621	631	648	rBV2	2537	5582	0.32%	0.049%
14	3.469	659	662	665	rVB	153	135	0.01%	0.001%
15	3.527	675	680	682	rBV2	178	173	0.01%	0.002%
16	3.543	682	685	689	rBV2	133	138	0.01%	0.001%
17	3.665	718	723	727	rBV2	155	187	0.01%	0.002%
18	3.732	741	744	752	rVB2	161	198	0.01%	0.002%
19	3.764	752	754	758	rVB2	153	109	0.01%	0.001%
20	3.816	766	770	773	rBV2	159	193	0.01%	0.002%
21	3.867	785	786	790	rVB	201	133	0.01%	0.001%
22	3.909	795	799	803	rVB	190	218	0.01%	0.002%
23	3.932	803	806	812	rBV2	171	236	0.01%	0.002%
24	3.996	821	826	829	rBV	195	190	0.01%	0.002%
25	4.057	842	845	848	rVB2	197	138	0.01%	0.001%
26	4.205	885	891	895	rBV2	247	277	0.02%	0.002%
27	4.250	903	905	911	rVB2	234	224	0.01%	0.002%
28	4.375	941	944	947	rBV2	188	182	0.01%	0.002%
29	4.633	1009	1024	1063	rBV	148182	406675	23.59%	3.544%
30	4.996	1134	1137	1139	rBV2	250	169	0.01%	0.001%
31	5.070	1142	1160	1186	rVV	228034	496539	28.80%	4.327%
32	5.189	1194	1197	1202	rBV2	328	374	0.02%	0.003%
33	5.231	1208	1210	1211	rBV	260	121	0.01%	0.001%
34	5.272	1220	1223	1226	rBV3	249	249	0.01%	0.002%
35	5.424	1267	1270	1274	rBV	127	130	0.01%	0.001%
36	5.485	1285	1289	1294	rBV2	171	217	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045169.D
 Acq On : 06 Oct 2021 01:06
 Operator : SY/MD
 Sample : M3996-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.555	1307	1311	1314	rBV2	181	187	0.01%	0.002%
38	5.591	1319	1322	1325	rBV	169	157	0.01%	0.001%
39	5.732	1343	1366	1396	rBV2	473141	1280672	74.27%	11.161%
40	6.099	1474	1480	1481	rBV3	260	291	0.02%	0.003%
41	6.253	1513	1528	1553	rBV	370440	701445	40.68%	6.113%
42	6.539	1607	1617	1629	rVB9	4552	8764	0.51%	0.076%
43	6.697	1651	1666	1686	rBV	301681	585750	33.97%	5.105%
44	6.845	1710	1712	1716	rVB2	305	181	0.01%	0.002%
45	6.887	1723	1725	1729	rVB	265	161	0.01%	0.001%
46	7.009	1760	1763	1765	rBV2	167	116	0.01%	0.001%
47	7.047	1768	1775	1782	rBV2	605	1034	0.06%	0.009%
48	7.131	1797	1801	1806	rBV2	104	117	0.01%	0.001%
49	7.186	1811	1818	1829	rVV4	1823	3104	0.18%	0.027%
50	7.327	1859	1862	1864	rBV	175	145	0.01%	0.001%
51	7.388	1877	1881	1887	rBV2	228	343	0.02%	0.003%
52	7.446	1895	1899	1902	rBV2	229	245	0.01%	0.002%
53	7.478	1906	1909	1912	rBV	146	129	0.01%	0.001%
54	7.497	1912	1915	1918	rBV2	171	160	0.01%	0.001%
55	7.568	1924	1937	1953	rBV	159166	278168	16.13%	2.424%
56	7.690	1968	1975	1988	rVB5	1168	2236	0.13%	0.019%
57	7.806	2006	2011	2016	rBV2	221	285	0.02%	0.002%
58	7.903	2027	2041	2056	rBV	578971	987015	57.24%	8.602%
59	8.182	2116	2128	2150	rBV	111306	187862	10.90%	1.637%
60	8.311	2166	2168	2171	rBV2	275	182	0.01%	0.002%
61	8.430	2202	2205	2208	rBV2	149	130	0.01%	0.001%
62	8.555	2230	2244	2259	rBV	1019547	1724239	100.00%	15.027%
63	8.639	2259	2270	2315	rVB	459209	814465	47.24%	7.098%
64	8.848	2332	2335	2338	rBV2	231	157	0.01%	0.001%
65	9.176	2432	2437	2440	rBV2	226	235	0.01%	0.002%
66	9.340	2485	2488	2492	rVB2	152	117	0.01%	0.001%
67	9.420	2498	2513	2532	rBV	523653	862569	50.03%	7.517%
68	9.681	2592	2594	2595	rBV	335	132	0.01%	0.001%
69	9.726	2606	2608	2612	rBV2	188	119	0.01%	0.001%
70	9.925	2666	2670	2673	rBV	146	118	0.01%	0.001%
71	9.951	2675	2678	2682	rBV	125	119	0.01%	0.001%
72	10.025	2696	2701	2704	rBV2	223	243	0.01%	0.002%
73	10.095	2719	2723	2728	rVB3	370	327	0.02%	0.003%
74	10.156	2738	2742	2745	rBV2	214	172	0.01%	0.001%
75	10.279	2775	2780	2783	rBV	236	209	0.01%	0.002%
76	10.333	2794	2797	2803	rBV2	187	176	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045169.D
 Acq On : 06 Oct 2021 01:06
 Operator : SY/MD
 Sample : M3996-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A31

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.362	2803	2806	2809	rVB2	188	132	0.01%	0.001%
78	10.382	2809	2812	2815	rVB2	180	149	0.01%	0.001%
79	10.401	2815	2818	2820	rBV	180	111	0.01%	0.001%
80	10.523	2854	2856	2859	rBV	187	132	0.01%	0.001%
81	10.562	2865	2868	2874	rVB	246	183	0.01%	0.002%
82	10.671	2894	2902	2913	rBV5	2016	3082	0.18%	0.027%
83	10.758	2917	2929	2950	rVB	411408	671836	38.96%	5.855%
84	10.896	2967	2972	2974	rBV	331	278	0.02%	0.002%
85	10.931	2980	2983	2986	rVB	296	223	0.01%	0.002%
86	11.002	3001	3005	3009	rBV	204	242	0.01%	0.002%
87	11.044	3014	3018	3022	rBV2	264	202	0.01%	0.002%
88	11.066	3023	3025	3028	rBV2	195	119	0.01%	0.001%
89	11.115	3038	3040	3043	rBV	219	175	0.01%	0.002%
90	11.436	3136	3140	3141	rBV	172	115	0.01%	0.001%
91	11.465	3144	3149	3155	rVB5	1212	1532	0.09%	0.013%
92	11.513	3161	3164	3166	rBV	249	182	0.01%	0.002%
93	11.645	3203	3205	3209	rBV2	164	108	0.01%	0.001%
94	11.700	3216	3222	3228	rBV4	842	1105	0.06%	0.010%
95	11.816	3245	3258	3280	rBV	496662	782971	45.41%	6.823%
96	12.028	3320	3324	3326	rBV2	267	212	0.01%	0.002%
97	12.195	3359	3376	3393	rBV	533343	856848	49.69%	7.467%
98	12.353	3422	3425	3428	rBV2	201	143	0.01%	0.001%
99	12.488	3465	3467	3471	rBV	160	119	0.01%	0.001%
100	13.221	3692	3695	3699	rBV	222	135	0.01%	0.001%




Sum of corrected areas: 11474628

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045169.D
Acq On : 06 Oct 2021 01:06
Operator : SY/MD
Sample : M3996-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

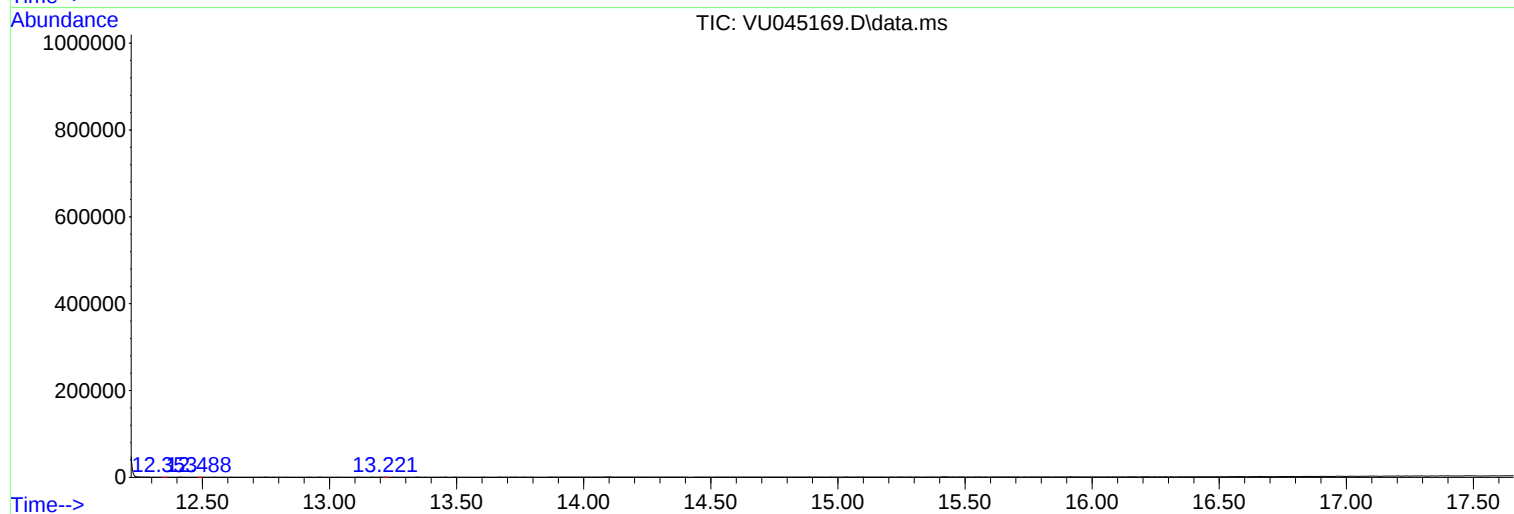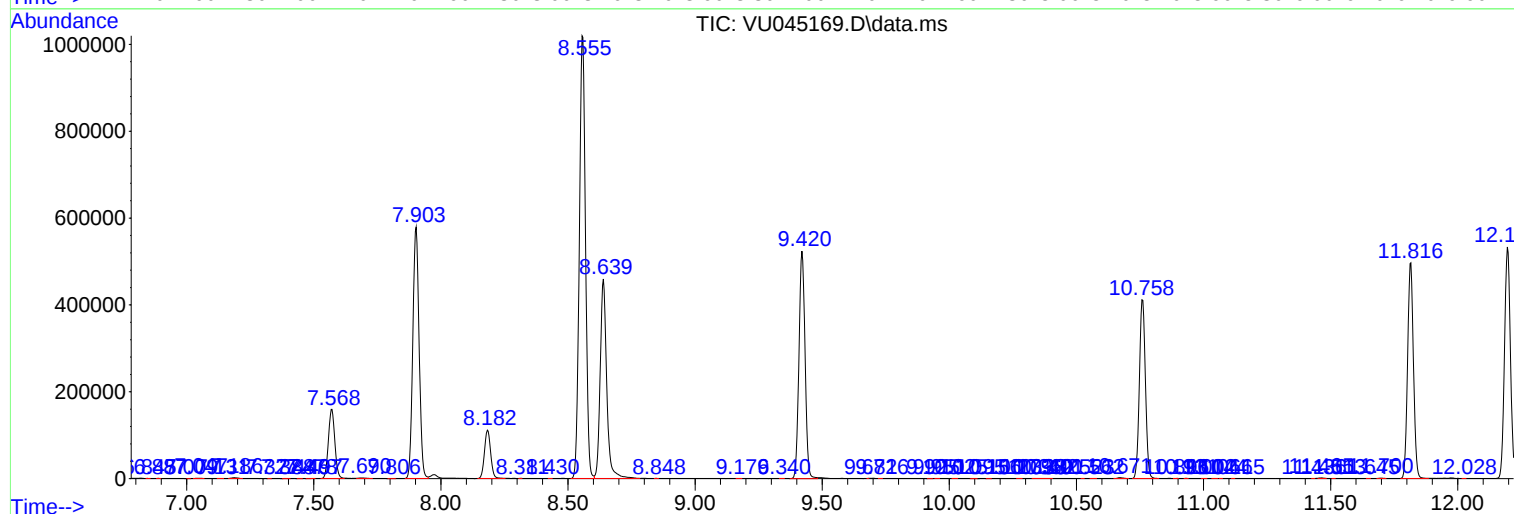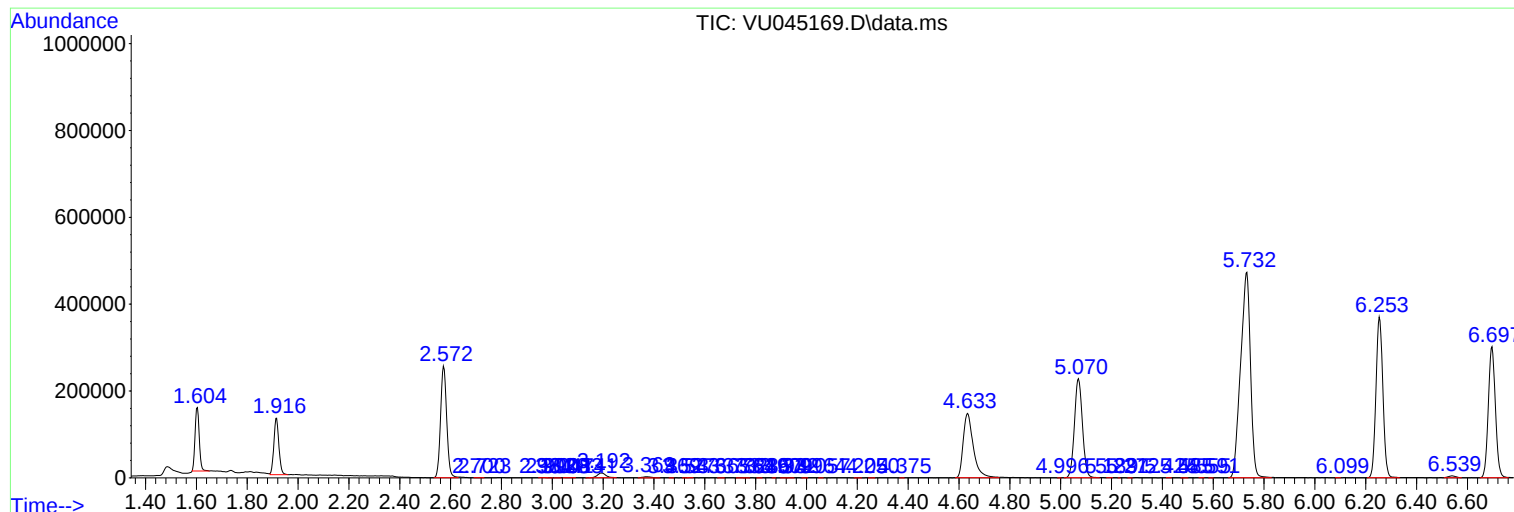

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045169.D
Acq On : 06 Oct 2021 01:06
Operator : SY/MD
Sample : M3996-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045169.D
Acq On : 06 Oct 2021 01:06
Operator : SY/MD
Sample : M3996-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------