

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045170.D
 Acq On : 06 Oct 2021 01:29
 Operator : SY/MD
 Sample : M3996-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU045170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	75	81	93	rBV	142731	162511	6.03%	1.312%
2	1.912	171	178	202	rVB	127292	173383	6.43%	1.400%
3	2.572	371	383	412	rBV	252311	422621	15.68%	3.413%
4	2.874	474	477	481	rBV2	206	177	0.01%	0.001%
5	3.047	528	531	532	rBV	200	113	0.00%	0.001%
6	3.112	548	551	553	rBV	169	108	0.00%	0.001%
7	3.192	562	576	609	rVB	27847	70147	2.60%	0.566%
8	3.327	614	618	619	rVV2	232	187	0.01%	0.002%
9	3.369	621	631	649	rVV4	5703	13659	0.51%	0.110%
10	3.449	653	656	659	rVV	233	161	0.01%	0.001%
11	3.469	659	662	665	rVB2	178	121	0.00%	0.001%
12	3.507	671	674	676	rBV	166	127	0.00%	0.001%
13	3.665	720	723	726	rBV2	176	143	0.01%	0.001%
14	3.716	733	739	744	rBB	250	277	0.01%	0.002%
15	3.768	752	755	757	rBV2	141	101	0.00%	0.001%
16	3.806	764	767	769	rBV2	163	111	0.00%	0.001%
17	3.867	782	786	788	rVB	153	136	0.01%	0.001%
18	3.893	788	794	796	rBV	203	188	0.01%	0.002%
19	3.922	800	803	806	rBV2	230	200	0.01%	0.002%
20	3.957	809	814	815	rBV	168	157	0.01%	0.001%
21	4.038	833	839	841	rBV	148	176	0.01%	0.001%
22	4.057	841	845	849	rVB2	173	126	0.00%	0.001%
23	4.083	849	853	856	rBV2	176	189	0.01%	0.002%
24	4.234	895	900	903	rBV2	160	151	0.01%	0.001%
25	4.269	908	911	914	rBB	161	116	0.00%	0.001%
26	4.292	914	918	922	rBV2	184	154	0.01%	0.001%
27	4.314	922	925	927	rBV	140	110	0.00%	0.001%
28	4.398	945	951	954	rBV2	226	274	0.01%	0.002%
29	4.427	958	960	962	rBV	173	109	0.00%	0.001%
30	4.575	999	1006	1007	rBV	201	250	0.01%	0.002%
31	4.633	1009	1024	1063	rBV2	156511	432108	16.04%	3.489%
32	5.070	1143	1160	1186	rBV	222284	489785	18.18%	3.955%
33	5.211	1201	1204	1206	rBV2	271	220	0.01%	0.002%
34	5.285	1225	1227	1229	rBV	303	202	0.01%	0.002%
35	5.346	1244	1246	1249	rVB	182	108	0.00%	0.001%
36	5.372	1249	1254	1257	rBV2	339	341	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045170.D
 Acq On : 06 Oct 2021 01:29
 Operator : SY/MD
 Sample : M3996-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.581	1316	1319	1325	rBV2	184	259	0.01%	0.002%
38	5.729	1343	1365	1397	rBV2	467650	1266904	47.02%	10.230%
39	6.176	1500	1504	1506	rBV	220	170	0.01%	0.001%
40	6.253	1514	1528	1550	rBV	364484	679201	25.21%	5.485%
41	6.546	1606	1619	1631	rBV4	17366	33019	1.23%	0.267%
42	6.697	1651	1666	1690	rBV	295643	577686	21.44%	4.665%
43	6.948	1738	1744	1748	rBV2	192	251	0.01%	0.002%
44	7.047	1770	1775	1778	rBV2	547	644	0.02%	0.005%
45	7.108	1785	1794	1799	rVB	235	380	0.01%	0.003%
46	7.131	1799	1801	1807	rBV2	158	178	0.01%	0.001%
47	7.189	1809	1819	1827	rVV3	1737	2984	0.11%	0.024%
48	7.269	1835	1844	1849	rBV2	251	450	0.02%	0.004%
49	7.401	1878	1885	1891	rBV2	237	364	0.01%	0.003%
50	7.497	1913	1915	1919	rBV2	142	115	0.00%	0.001%
51	7.571	1924	1938	1962	rVV	157329	277203	10.29%	2.238%
52	7.813	2009	2013	2014	rBV	177	130	0.00%	0.001%
53	7.903	2024	2041	2056	rBV	568012	970407	36.01%	7.836%
54	8.182	2115	2128	2149	rBV	109466	186402	6.92%	1.505%
55	8.369	2182	2186	2190	rVB	169	193	0.01%	0.002%
56	8.555	2230	2244	2259	rBV	1601677	2694645	100.00%	21.760%
57	8.639	2260	2270	2322	rVB	442498	794727	29.49%	6.418%
58	9.044	2390	2396	2399	rBV2	204	235	0.01%	0.002%
59	9.060	2399	2401	2403	rBV	160	112	0.00%	0.001%
60	9.102	2411	2414	2417	rBV2	180	126	0.00%	0.001%
61	9.121	2418	2420	2423	rVB2	162	96	0.00%	0.001%
62	9.140	2423	2426	2428	rBV	176	110	0.00%	0.001%
63	9.224	2447	2452	2456	rBV	177	180	0.01%	0.001%
64	9.285	2468	2471	2473	rBV2	199	162	0.01%	0.001%
65	9.317	2479	2481	2484	rBV2	151	106	0.00%	0.001%
66	9.420	2500	2513	2549	rBV	512330	839987	31.17%	6.783%
67	9.546	2550	2552	2558	rVB2	220	138	0.01%	0.001%
68	9.694	2595	2598	2604	rVB3	660	857	0.03%	0.007%
69	9.732	2606	2610	2612	rBV2	203	178	0.01%	0.001%
70	9.784	2622	2626	2628	rBV	161	127	0.00%	0.001%
71	9.867	2647	2652	2653	rBV	206	146	0.01%	0.001%
72	9.912	2664	2666	2670	rBV2	175	148	0.01%	0.001%
73	9.964	2678	2682	2685	rBV2	217	174	0.01%	0.001%
74	10.009	2693	2696	2698	rVB2	165	98	0.00%	0.001%
75	10.025	2698	2701	2706	rBV2	222	202	0.01%	0.002%
76	10.224	2759	2763	2766	rBV	189	120	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
 Data File : VU045170.D
 Acq On : 06 Oct 2021 01:29
 Operator : SY/MD
 Sample : M3996-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F4A32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.247	2766	2770	2775	rVB2	209	206	0.01%	0.002%
78	10.272	2775	2778	2781	rBV	162	145	0.01%	0.001%
79	10.465	2835	2838	2842	rVB2	219	180	0.01%	0.001%
80	10.507	2847	2851	2854	rBV2	214	198	0.01%	0.002%
81	10.677	2894	2904	2914	rBV5	2216	3196	0.12%	0.026%
82	10.761	2917	2930	2951	rBV	413306	664606	24.66%	5.367%
83	10.838	2951	2954	2959	rBV	184	171	0.01%	0.001%
84	10.867	2959	2963	2965	rBV2	439	383	0.01%	0.003%
85	11.063	3021	3024	3031	rVB	256	180	0.01%	0.001%
86	11.118	3039	3041	3042	rBV	340	129	0.00%	0.001%
87	11.230	3071	3076	3078	rBV2	273	251	0.01%	0.002%
88	11.365	3115	3118	3121	rBV	234	190	0.01%	0.002%
89	11.404	3127	3130	3133	rVB2	217	152	0.01%	0.001%
90	11.465	3142	3149	3152	rBV3	1179	1578	0.06%	0.013%
91	11.581	3183	3185	3190	rBV	317	289	0.01%	0.002%
92	11.619	3195	3197	3201	rBV	146	105	0.00%	0.001%
93	11.700	3215	3222	3231	rBV3	806	1227	0.05%	0.010%
94	11.816	3245	3258	3276	rBV	483180	764819	28.38%	6.176%
95	11.902	3282	3285	3287	rBV2	360	199	0.01%	0.002%
96	12.057	3330	3333	3336	rBV	227	125	0.00%	0.001%
97	12.195	3362	3376	3398	rBV	525709	845982	31.39%	6.831%
98	12.591	3496	3499	3501	rBV	198	142	0.01%	0.001%
99	12.619	3505	3508	3515	rBV2	235	296	0.01%	0.002%
100	12.854	3578	3581	3585	rBV	210	201	0.01%	0.002%




Sum of corrected areas: 12383611

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045170.D
Acq On : 06 Oct 2021 01:29
Operator : SY/MD
Sample : M3996-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

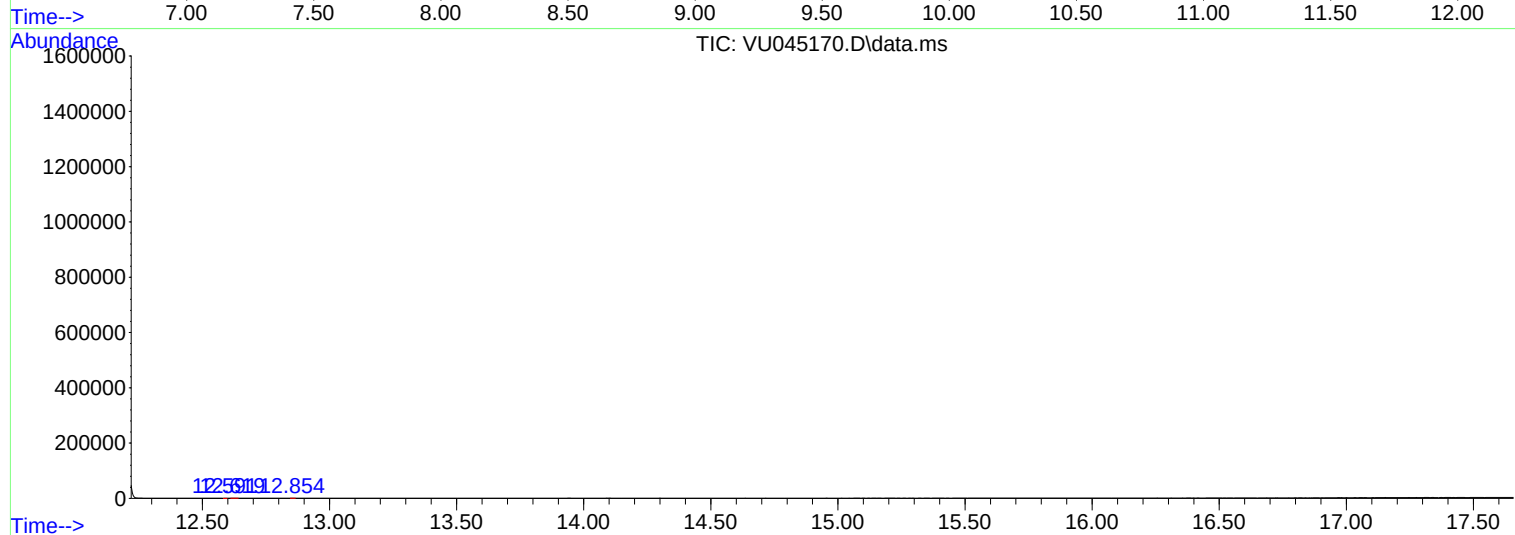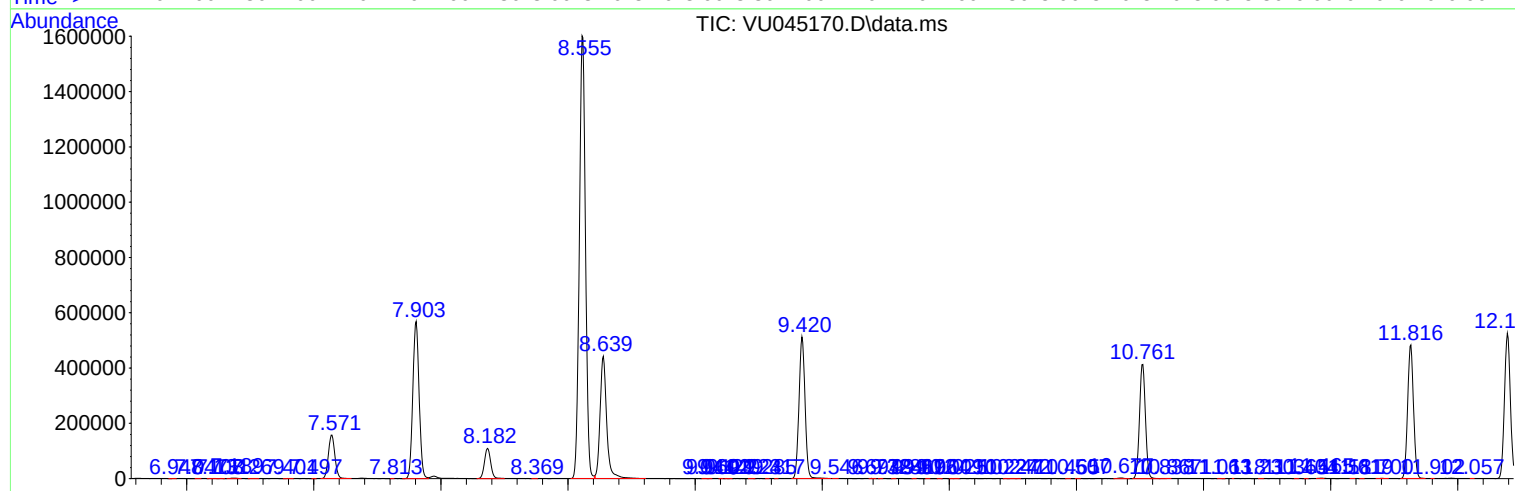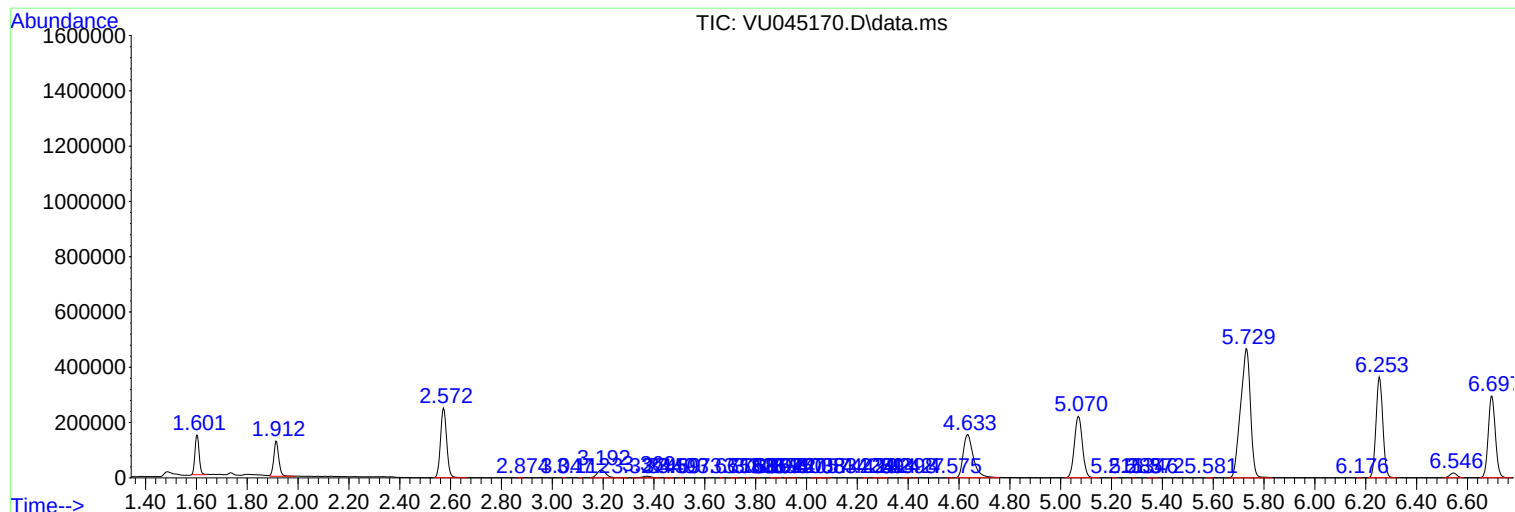

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045170.D
Acq On : 06 Oct 2021 01:29
Operator : SY/MD
Sample : M3996-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045170.D
Acq On : 06 Oct 2021 01:29
Operator : SY/MD
Sample : M3996-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F4A32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
