


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100521\
Data File : VU045133.D
Acq On : 05 Oct 2021 10:18
Operator : SY/MD
Sample : BFB006
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB006

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Title : VOC Analysis
Last Update : Mon Oct 11 01:47:08 2021

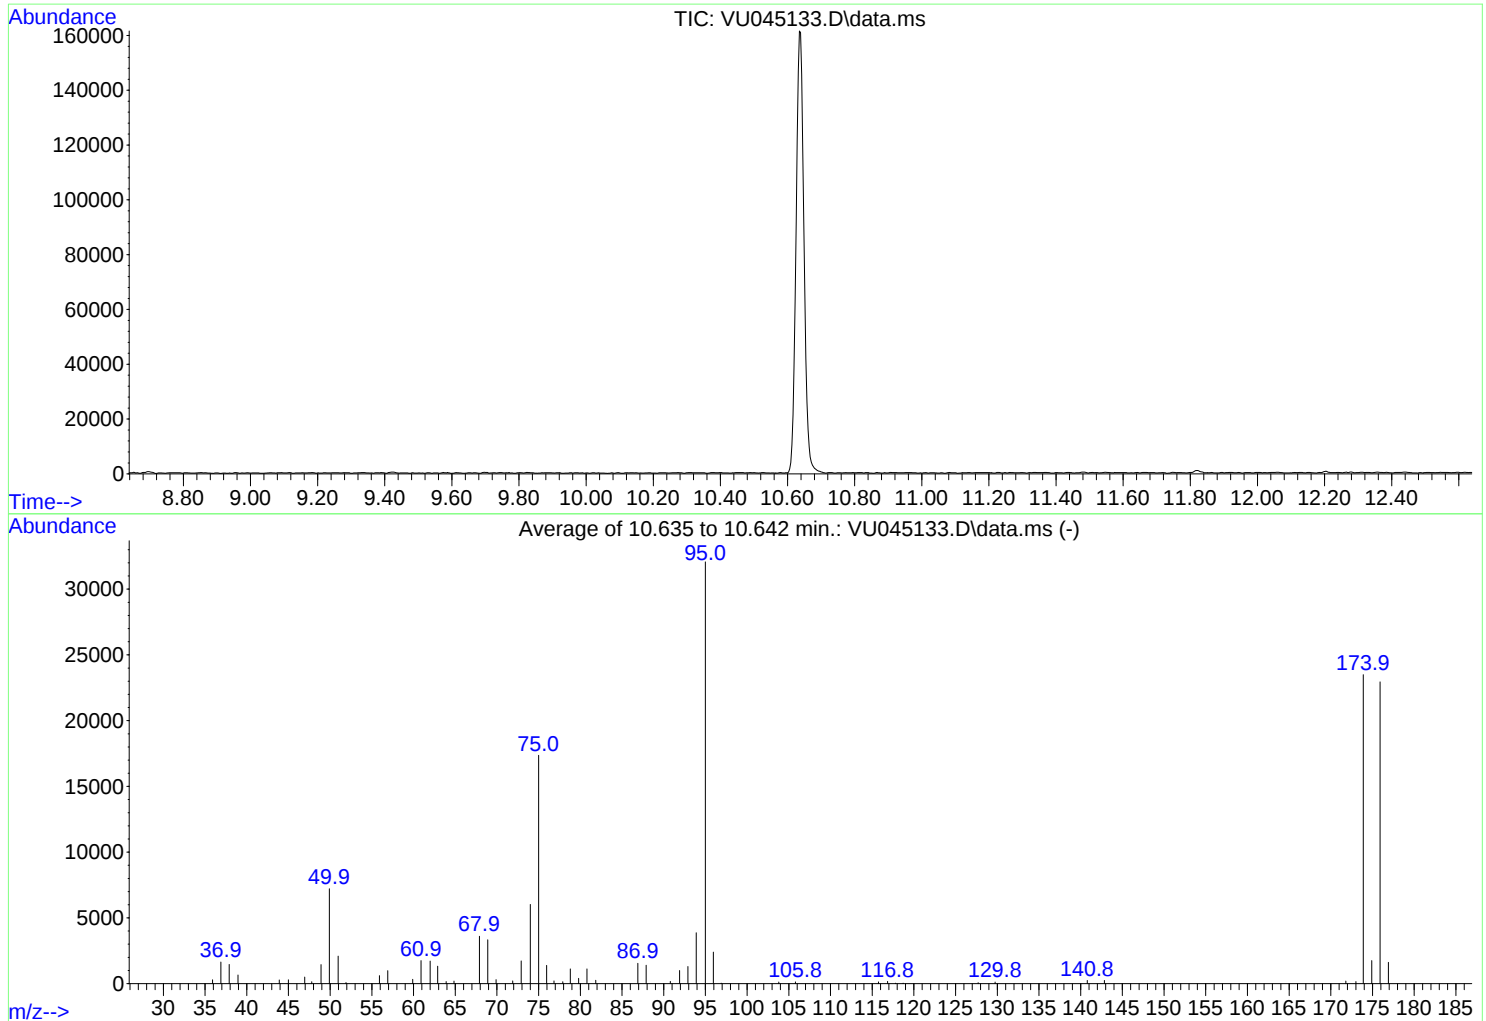

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.5	7211	PASS
75	95	30	80	54.1	17360	PASS
95	95	100	100	100.0	32077	PASS
96	95	5	9	7.5	2403	PASS
173	174	0.00	2	0.7	165	PASS
174	95	50	120	73.2	23496	PASS
175	174	5	9	7.5	1756	PASS
176	174	95	101	97.7	22949	PASS
177	176	5	9	7.1	1621	PASS

Scan 2879 (10.597 min): VU045133.D\data.ms
BFB006

m/z	Abundance
39.90	144.0
43.90	265.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006

m/z	Abundance
36.00	357.0
36.90	1605.0
37.90	1501.0
39.00	725.0
39.90	107.0
44.00	524.0
45.00	302.0
46.90	453.0
47.80	183.0
48.90	1506.0
49.90	7498.0
51.00	2150.0
51.90	144.0
55.90	673.0
56.90	1012.0
59.90	352.0
60.90	1817.0
62.00	1878.0
62.90	1424.0
63.90	159.0
64.80	238.0
67.90	3903.0
68.90	3589.0
69.90	332.0
71.90	201.0
72.90	1854.0
74.00	6290.0
75.00	18448.0
75.90	1523.0
76.80	191.0
77.90	180.0
78.80	1187.0
79.80	411.0
80.80	1149.0
81.80	265.0
86.90	1569.0
87.90	1400.0
90.80	179.0
91.90	975.0
92.90	1393.0
93.90	3912.0
95.00	33056.0
96.00	2552.0
96.90	110.0
103.80	136.0
105.80	150.0
115.80	154.0
116.80	184.0
117.80	107.0
118.70	102.0
127.70	111.0
129.70	127.0
140.80	280.0
142.90	251.0
171.80	224.0
173.00	237.0
173.90	23816.0
174.90	1865.0
175.90	22952.0
176.90	1606.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006

m/z	Abundance
35.90	299.0
36.90	1693.0
37.90	1499.0
38.90	659.0
39.90	118.0
44.00	553.0
45.00	291.0
46.90	533.0
47.80	157.0
48.90	1500.0
49.90	7462.0
50.90	2136.0
51.90	111.0
55.90	620.0
56.90	980.0
59.90	331.0
60.90	1801.0
62.00	1773.0
62.90	1371.0
63.90	161.0
64.90	193.0
67.90	3720.0
68.90	3442.0
69.90	311.0
71.90	216.0
72.90	1792.0
74.00	6188.0
75.00	17880.0
76.00	1427.0
76.90	209.0
77.90	159.0
78.80	1143.0
79.80	410.0
80.80	1152.0
81.90	256.0
86.90	1614.0
87.90	1441.0
90.80	178.0
91.90	1032.0
92.90	1325.0
93.90	3981.0
95.00	33120.0
95.90	2484.0
103.80	126.0
105.80	151.0
115.70	130.0
116.90	165.0
127.70	117.0
129.80	123.0
140.80	240.0
142.90	235.0
171.80	196.0
173.00	257.0
173.90	24328.0
174.90	1808.0
175.90	23704.0
176.90	1682.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006

m/z	Abundance
35.90	241.0
36.90	1635.0
37.90	1392.0
38.90	582.0
39.90	124.0
43.90	555.0
45.00	289.0
47.00	514.0
47.80	118.0
48.90	1351.0
49.90	6672.0
50.90	1984.0
55.90	522.0
56.90	952.0
59.90	294.0
60.90	1660.0
62.00	1514.0
62.90	1188.0
63.90	170.0
64.90	150.0
67.90	3198.0
68.90	2986.0
69.90	280.0
71.90	213.0
72.90	1526.0
74.00	5604.0
75.00	15751.0
76.00	1227.0
76.90	208.0
77.90	117.0
78.80	1017.0
79.80	369.0
80.80	1057.0
81.90	228.0
86.90	1468.0
87.90	1365.0
90.80	168.0
91.90	980.0
92.90	1190.0
93.90	3710.0
95.00	30056.0
95.90	2174.0
103.80	117.0
105.80	122.0
115.80	116.0
116.90	152.0
129.80	119.0
140.80	198.0
142.80	227.0
171.80	161.0
173.90	22344.0
174.90	1596.0
175.90	22192.0
176.90	1575.0

Instrument :
MSVOA_U
ClientSampleId :
BFB006