
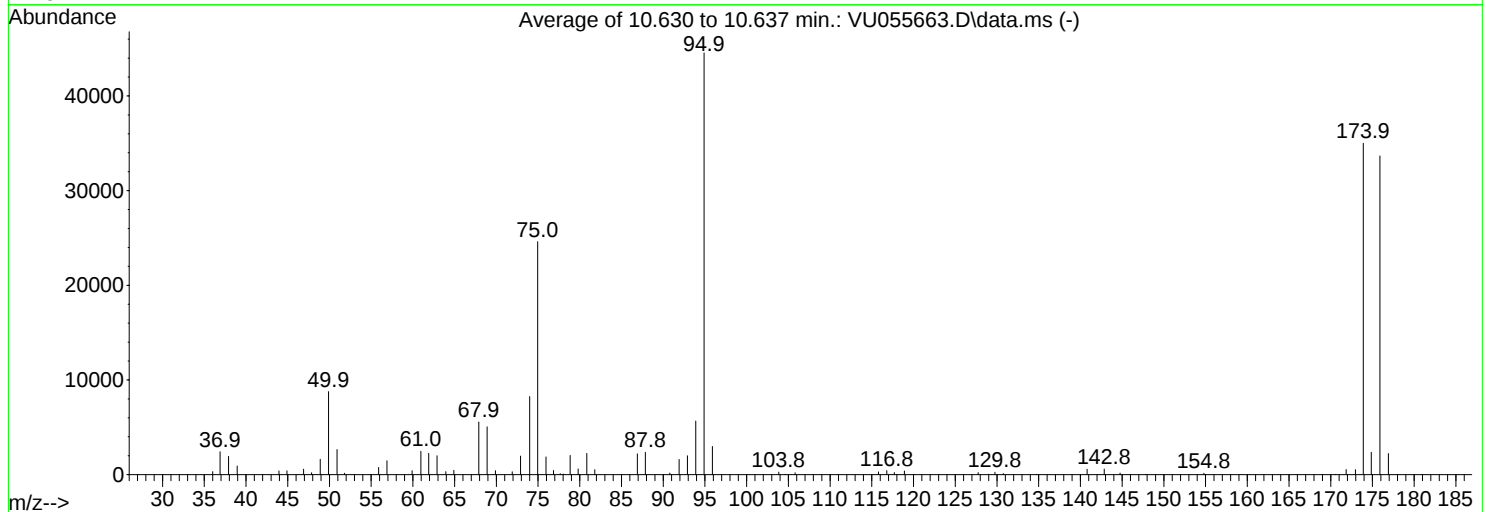


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100523\
Data File : VU055663.D
Acq On : 05 Oct 2023 08:53
Operator : MD/SY
Sample : BFB040
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB040

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM100523.M
Title : TRACE VOA SOM01.0
Last Update : Fri Oct 06 19:09:35 2023

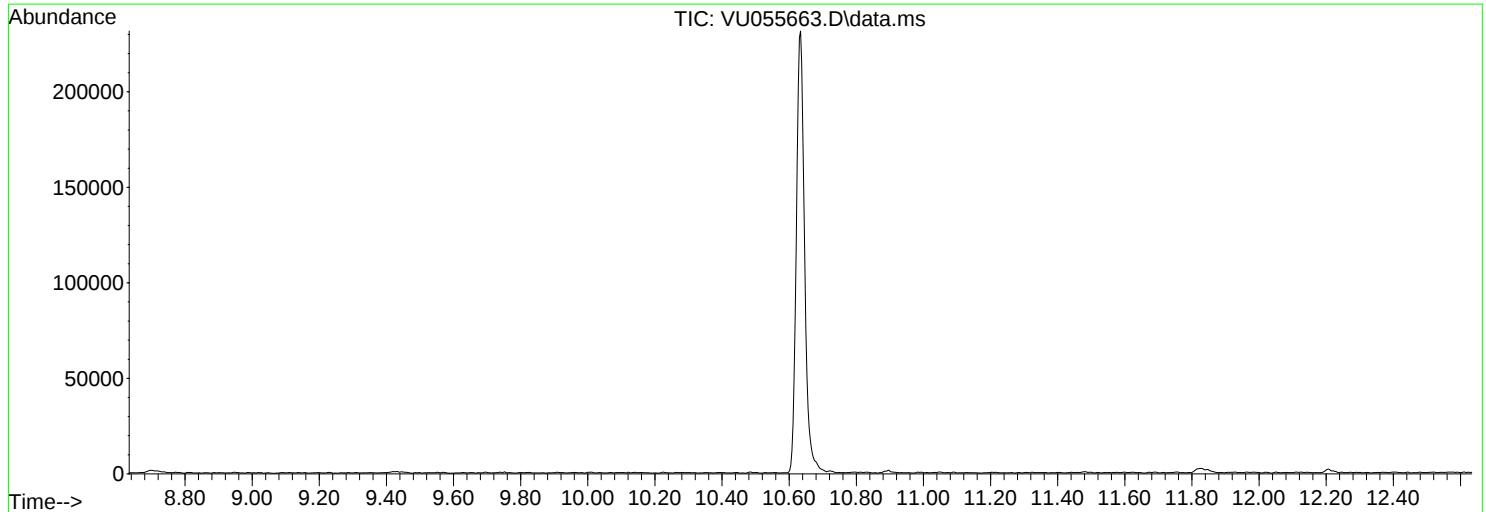

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	8772	PASS
75	95	30	80	55.2	24608	PASS
95	95	100	100	100.0	44552	PASS
96	95	5	9	6.7	2970	PASS
173	174	0.00	2	1.5	520	PASS
174	95	50	120	78.6	35005	PASS
175	174	5	9	6.7	2361	PASS
176	174	95	101	96.2	33667	PASS
177	176	5	9	6.6	2235	PASS

m/z	Abundance
39.90	187.0
43.90	367.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
36.00	369.0
36.90	2404.0
37.90	2045.0
39.00	987.0
39.90	192.0
44.00	694.0
44.90	361.0
46.80	776.0
47.90	213.0
48.90	1752.0
49.90	9033.0
50.90	3022.0
51.80	219.0
54.90	103.0
55.90	787.0
56.90	1600.0
59.90	383.0
61.00	2469.0
61.90	2347.0
62.90	2091.0
64.00	312.0
64.90	468.0
67.90	5603.0
68.90	5248.0
69.90	482.0
71.90	357.0
72.90	2031.0
74.00	8419.0
74.90	24864.0
76.00	1815.0
76.80	467.0
77.70	174.0
78.00	179.0
78.90	2083.0
79.80	660.0
80.90	2222.0
81.80	550.0
86.90	2182.0
87.90	2433.0
90.90	179.0
91.90	1539.0
92.90	2075.0
93.90	5832.0
94.90	45080.0
95.90	2976.0
103.90	315.0
104.60	104.0
105.80	220.0
115.80	270.0
116.80	499.0
117.70	222.0
118.90	445.0
127.80	234.0
129.00	151.0
129.70	267.0
130.90	103.0
134.70	111.0
140.80	508.0
142.80	511.0
144.70	159.0
147.80	126.0
154.80	180.0
171.90	594.0
172.90	574.0
173.90	34936.0
174.80	2348.0
175.90	33232.0
176.90	2202.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
36.00	316.0
36.90	2528.0
37.90	1983.0
39.00	954.0
39.90	160.0
44.00	783.0
44.90	426.0
46.90	571.0
47.90	188.0
48.90	1656.0
49.90	9009.0
50.90	2691.0
51.80	162.0
55.90	768.0
56.90	1496.0
59.90	436.0
60.90	2530.0
61.90	2279.0
62.90	2035.0
64.00	304.0
64.90	473.0
67.90	5734.0
68.90	5188.0
69.90	440.0
71.90	322.0
72.90	2032.0
74.00	8582.0
75.00	25272.0
75.90	1886.0
76.80	445.0
77.60	148.0
78.80	2001.0
79.80	628.0
80.80	2333.0
81.80	543.0
86.90	2316.0
87.90	2439.0
90.80	166.0
91.90	1639.0
92.90	2046.0
93.90	5814.0
94.90	46112.0
95.90	3048.0
103.90	298.0
105.80	211.0
115.80	295.0
116.80	436.0
117.70	232.0
118.90	396.0
127.80	232.0
129.80	283.0
130.70	130.0
140.80	601.0
142.90	603.0
144.80	172.0
154.80	169.0
170.60	100.0
171.80	555.0
173.00	535.0
173.90	36008.0
174.80	2401.0
175.90	34944.0
176.90	2299.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040

m/z	Abundance
36.00	304.0
36.90	2299.0
37.90	1746.0
38.90	782.0
39.90	121.0
44.00	797.0
44.90	410.0
47.00	400.0
47.80	191.0
48.90	1471.0
49.90	8274.0
50.90	2277.0
51.90	103.0
55.90	715.0
56.90	1329.0
59.90	470.0
60.90	2415.0
61.90	2107.0
62.90	1866.0
63.90	343.0
64.90	441.0
67.90	5340.0
68.90	4746.0
69.90	344.0
71.90	215.0
72.90	1806.0
74.00	7756.0
75.00	23688.0
75.90	1952.0
76.90	395.0
78.80	1989.0
79.80	528.0
80.80	2193.0
81.80	462.0
86.90	2121.0
87.80	2224.0
90.70	168.0
91.90	1630.0
92.90	1846.0
93.90	5367.0
94.90	42464.0
95.90	2886.0
103.80	219.0
105.80	193.0
115.80	283.0
116.80	347.0
117.70	206.0
118.90	344.0
127.70	204.0
129.70	240.0
130.70	147.0
140.80	596.0
142.90	646.0
144.80	162.0
154.80	135.0
171.80	488.0
173.00	451.0
173.90	34072.0
174.90	2333.0
175.90	32824.0
176.90	2205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB040