

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100620\
 Data File : VU040530.D
 Acq On : 06 Oct 2020 16:01
 Operator : SY/MD
 Sample : VU1006WBL03
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK203

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	91	rBV	168012	181263	15.06%	1.919%
2	1.919	172	180	193	rVB	125981	163824	13.61%	1.734%
3	2.173	257	259	261	rBV3	742	391	0.03%	0.004%
4	2.578	372	385	402	rBV	275665	454613	37.78%	4.813%
5	2.697	418	422	424	rBV2	621	471	0.04%	0.005%
6	2.761	436	442	445	rBV3	272	349	0.03%	0.004%
7	2.810	445	457	466	rVB3	2369	4318	0.36%	0.046%
8	2.954	499	502	504	rBV2	432	294	0.02%	0.003%
9	3.035	522	527	528	rBV3	312	254	0.02%	0.003%
10	3.054	528	533	534	rBV3	1637	1202	0.10%	0.013%
11	3.112	549	551	556	rVB	284	208	0.02%	0.002%
12	3.154	559	564	569	rBV2	285	415	0.03%	0.004%
13	3.199	574	578	585	rVB3	623	704	0.06%	0.007%
14	3.237	585	590	592	rBV	241	255	0.02%	0.003%
15	3.379	623	634	641	rBV7	1384	2632	0.22%	0.028%
16	3.713	728	738	739	rBV2	456	463	0.04%	0.005%
17	3.797	761	764	768	rVB	502	395	0.03%	0.004%
18	3.819	768	771	774	rBV2	383	285	0.02%	0.003%
19	3.851	778	781	784	rBV	340	277	0.02%	0.003%
20	4.433	959	962	965	rBV2	220	215	0.02%	0.002%
21	4.636	1008	1025	1047	rBV	121883	285469	23.72%	3.022%
22	4.986	1131	1134	1138	rVV4	493	350	0.03%	0.004%
23	5.080	1146	1163	1187	rVV	213588	473372	39.34%	5.012%
24	5.301	1226	1232	1238	rBV4	609	883	0.07%	0.009%
25	5.391	1253	1260	1262	rBV4	829	1052	0.09%	0.011%
26	5.526	1298	1302	1304	rBV2	379	253	0.02%	0.003%
27	5.546	1306	1308	1316	rVB3	400	268	0.02%	0.003%
28	5.739	1346	1368	1392	rBV2	447480	1203400	100.00%	12.741%
29	6.044	1460	1463	1466	rBV3	310	234	0.02%	0.002%
30	6.112	1480	1484	1488	rVB3	279	260	0.02%	0.003%
31	6.137	1488	1492	1494	rBV2	296	254	0.02%	0.003%
32	6.260	1515	1530	1550	rBV	380329	709050	58.92%	7.507%
33	6.372	1563	1565	1569	rVB3	478	255	0.02%	0.003%
34	6.420	1577	1580	1583	rBV3	285	210	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100620\
 Data File : VU040530.D
 Acq On : 06 Oct 2020 16:01
 Operator : SY/MD
 Sample : VU1006WBL03
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK203

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
 Title : VOC Analysis

35	6.542	1607	1618	1629	rBV8	4809	9104	0.76%	0.096%
36	6.607	1635	1638	1642	rVB2	344	259	0.02%	0.003%
37	6.700	1652	1667	1686	rBV	280871	549261	45.64%	5.815%
38	6.980	1751	1754	1759	rVB	500	401	0.03%	0.004%
39	7.067	1775	1781	1783	rBV2	346	336	0.03%	0.004%
40	7.186	1810	1818	1820	rBV2	447	498	0.04%	0.005%
41	7.571	1925	1938	1958	rBV	161380	281296	23.38%	2.978%
42	7.800	1998	2009	2021	rBV5	3764	7270	0.60%	0.077%
43	7.906	2027	2042	2060	rBV	547524	935176	77.71%	9.901%
44	8.185	2116	2129	2148	rBV	117635	200735	16.68%	2.125%
45	8.317	2164	2170	2178	rVB4	425	595	0.05%	0.006%
46	8.382	2188	2190	2193	rVV	377	257	0.02%	0.003%
47	8.411	2194	2199	2202	rVV4	858	818	0.07%	0.009%
48	8.436	2204	2207	2211	rVB2	338	237	0.02%	0.003%
49	8.468	2215	2217	2221	rVB	500	229	0.02%	0.002%
50	8.494	2221	2225	2228	rBV2	286	273	0.02%	0.003%
51	8.552	2240	2243	2244	rVV	827	523	0.04%	0.006%
52	8.562	2244	2246	2250	rVB3	1109	713	0.06%	0.008%
53	8.636	2255	2269	2314	rBV	343536	635100	52.78%	6.724%
54	8.816	2321	2325	2333	rVB4	817	773	0.06%	0.008%
55	8.925	2354	2359	2361	rBV3	443	441	0.04%	0.005%
56	9.243	2450	2458	2459	rBV2	305	382	0.03%	0.004%
57	9.272	2463	2467	2471	rBV2	200	210	0.02%	0.002%
58	9.420	2499	2513	2534	rBV	549017	908869	75.53%	9.623%
59	9.575	2553	2561	2566	rVB	2170	2654	0.22%	0.028%
60	9.700	2591	2600	2610	rVB3	1766	3014	0.25%	0.032%
61	9.812	2629	2635	2641	rBV2	594	752	0.06%	0.008%
62	9.902	2660	2663	2667	rBV2	248	233	0.02%	0.002%
63	9.999	2689	2693	2696	rBV2	348	348	0.03%	0.004%
64	10.050	2704	2709	2711	rBV2	264	308	0.03%	0.003%
65	10.108	2718	2727	2736	rBV7	3126	5978	0.50%	0.063%
66	10.259	2768	2774	2777	rBV2	267	246	0.02%	0.003%
67	10.288	2781	2783	2794	rVB	629	509	0.04%	0.005%
68	10.333	2794	2797	2801	rBV2	343	246	0.02%	0.003%
69	10.436	2826	2829	2833	rVB	369	281	0.02%	0.003%
70	10.484	2833	2844	2849	rBV3	2768	3871	0.32%	0.041%
71	10.597	2872	2879	2882	rBV2	301	399	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100620\
 Data File : VU040530.D
 Acq On : 06 Oct 2020 16:01
 Operator : SY/MD
 Sample : VU1006WBL03
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK203

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
 Title : VOC Analysis

72	10.693	2904	2909	2915	rBV	303	396	0.03%	0.004%
73	10.758	2915	2929	2944	rVV	345806	578145	48.04%	6.121%
74	10.819	2944	2948	2958	rVB5	2755	3767	0.31%	0.040%
75	11.005	3001	3006	3010	rBV2	385	374	0.03%	0.004%
76	11.031	3010	3014	3016	rBV	399	273	0.02%	0.003%
77	11.089	3024	3032	3045	rBV4	2023	3429	0.28%	0.036%
78	11.140	3045	3048	3050	rBV	343	236	0.02%	0.002%
79	11.330	3104	3107	3112	rBV2	364	297	0.02%	0.003%
80	11.462	3142	3148	3157	rVB4	3009	3877	0.32%	0.041%
81	11.693	3216	3220	3223	rBV	441	385	0.03%	0.004%
82	11.742	3227	3235	3244	rVV3	4783	6954	0.58%	0.074%
83	11.809	3244	3256	3277	rVV	540164	857325	71.24%	9.077%
84	12.189	3360	3374	3393	rBV	531202	858830	71.37%	9.093%
85	12.870	3583	3586	3589	rBV2	307	220	0.02%	0.002%
86	12.992	3616	3624	3630	rBV2	2561	3233	0.27%	0.034%
87	13.214	3683	3693	3701	rBV3	7461	10371	0.86%	0.110%
88	13.568	3799	3803	3810	rBV2	463	581	0.05%	0.006%
89	13.777	3864	3868	3871	rVB	514	359	0.03%	0.004%
90	13.832	3877	3885	3896	rVB3	11785	17349	1.44%	0.184%
91	14.079	3953	3962	3975	rVB	20053	32854	2.73%	0.348%
92	14.172	3988	3991	3993	rBV2	293	213	0.02%	0.002%
93	14.324	4026	4038	4049	rBV3	14472	22716	1.89%	0.241%
94	14.375	4051	4054	4055	rBV2	472	283	0.02%	0.003%
95	14.639	4132	4136	4138	rBV3	320	289	0.02%	0.003%
96	14.677	4146	4148	4149	rBV3	410	208	0.02%	0.002%
97	14.922	4221	4224	4227	rBV2	501	369	0.03%	0.004%
98	15.561	4421	4423	4426	rBV2	485	255	0.02%	0.003%
99	15.819	4500	4503	4507	rBV3	562	410	0.03%	0.004%
100	15.983	4552	4554	4556	rVB2	715	319	0.03%	0.003%


Sum of corrected areas: 9445050

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100620\
Data File : VU040530.D
Acq On : 06 Oct 2020 16:01
Operator : SY/MD
Sample : VU1006WBL03
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK203

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

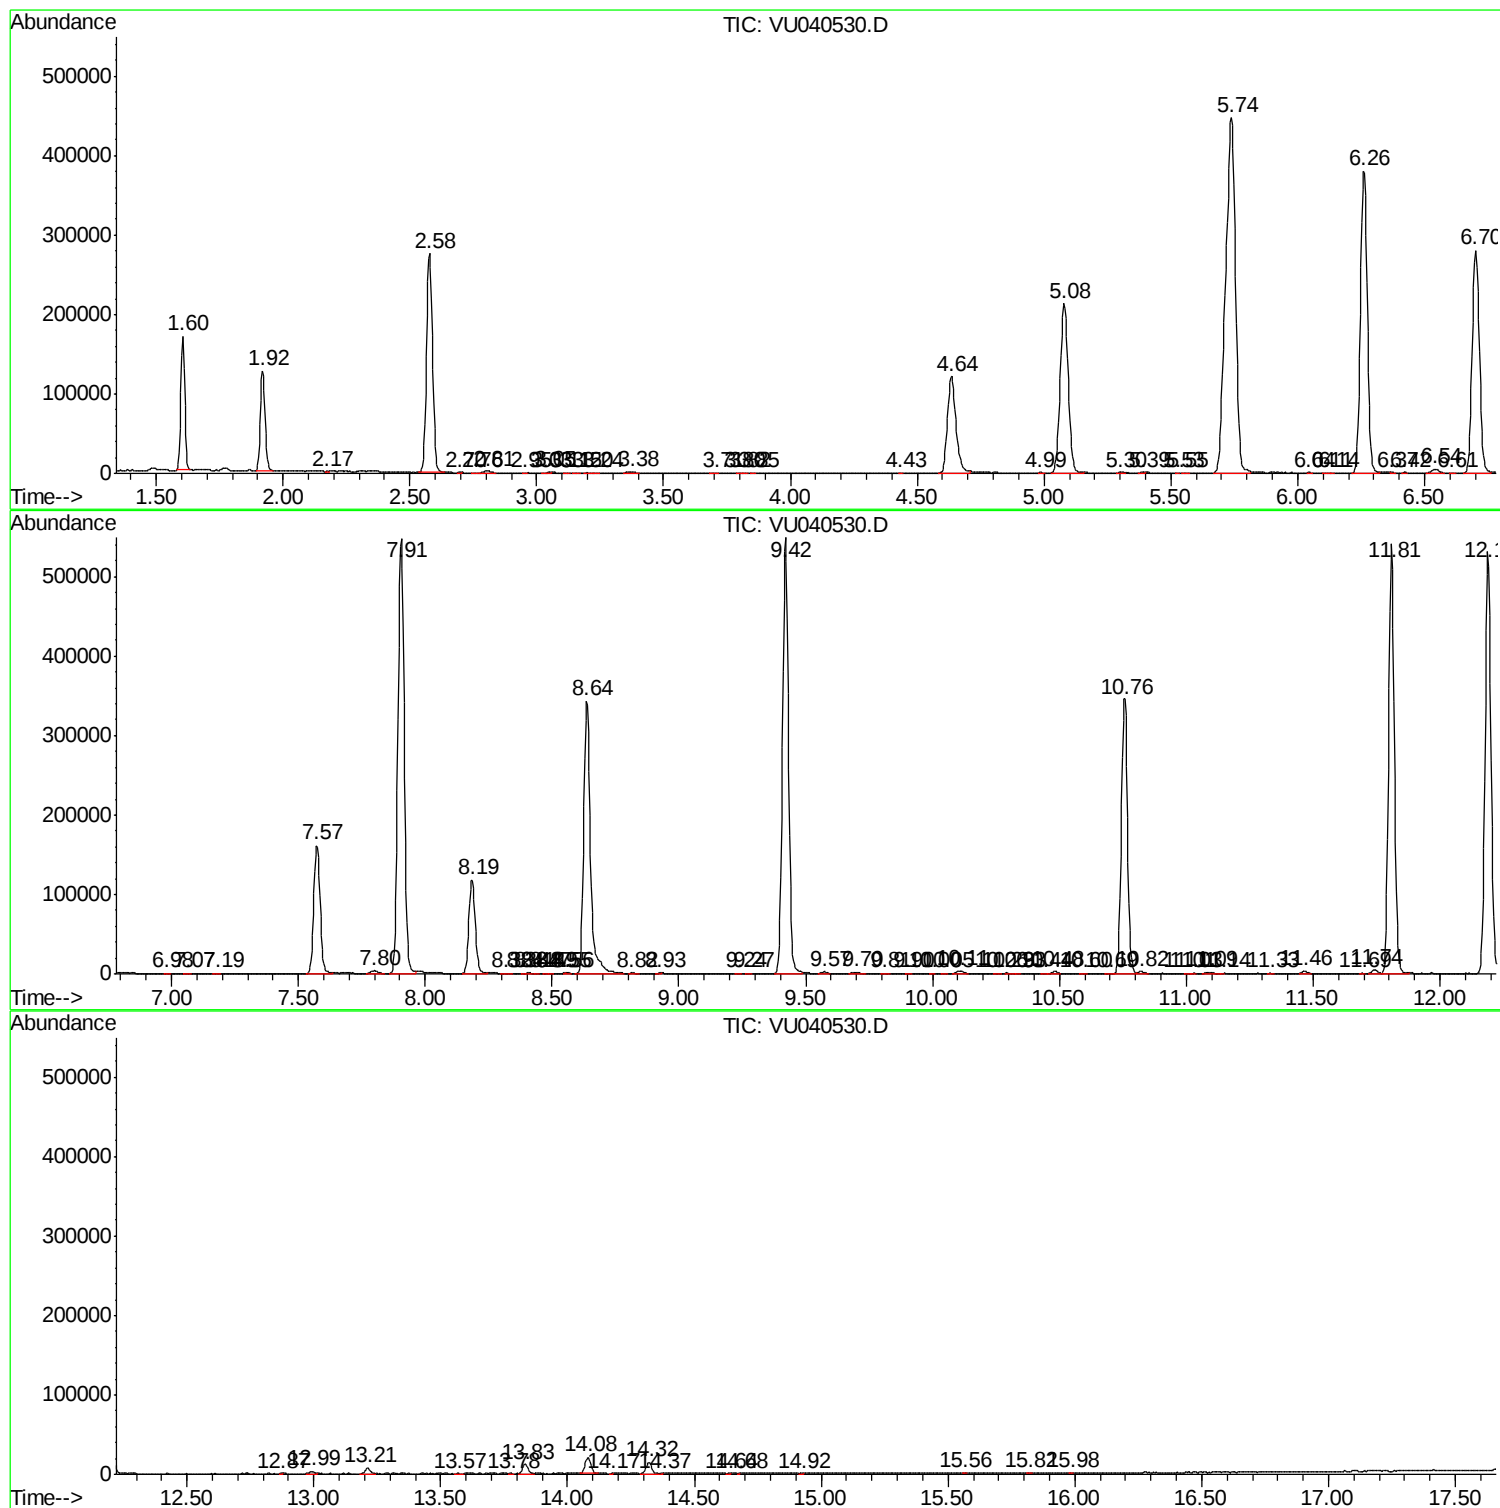

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU100620\
Data File : VU040530.D
Acq On : 06 Oct 2020 16:01
Operator : SY/MD
Sample : VU1006WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK203

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU100620\
Data File : VU040530.D
Acq On : 06 Oct 2020 16:01
Operator : SY/MD
Sample : VU1006WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK203

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc