

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100620\
 Data File : VU040533.D
 Acq On : 06 Oct 2020 17:52
 Operator : SY/MD
 Sample : TEST
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TEST

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
 Title : VOC Analysis

Signal : TIC: VU040534.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.607	74	83	99	rVB2	309367	359339	28.45%	2.692%
2	1.916	171	179	196	rVB	126939	166614	13.19%	1.248%
3	2.581	372	386	402	rBV3	325482	601764	47.65%	4.508%
4	2.710	423	426	430	rBV3	328	220	0.02%	0.002%
5	2.797	450	453	454	rBV	475	275	0.02%	0.002%
6	2.883	475	480	482	rBV2	227	233	0.02%	0.002%
7	2.999	513	516	519	rVV	384	226	0.02%	0.002%
8	3.060	522	535	550	rVV	58735	110550	8.75%	0.828%
9	3.202	566	579	592	rVV	6182	13769	1.09%	0.103%
10	3.279	601	603	608	rBV2	275	200	0.02%	0.001%
11	3.369	617	631	649	rVB	75826	147370	11.67%	1.104%
12	3.674	722	726	732	rBV2	398	426	0.03%	0.003%
13	3.713	732	738	739	rBV3	1397	1313	0.10%	0.010%
14	3.771	752	756	760	rBV2	332	357	0.03%	0.003%
15	3.793	761	763	768	rVB	399	290	0.02%	0.002%
16	4.006	825	829	833	rVB2	251	205	0.02%	0.002%
17	4.083	849	853	857	rBV	306	256	0.02%	0.002%
18	4.642	1011	1027	1037	rBV	139597	345007	27.32%	2.584%
19	4.935	1116	1118	1123	rVB3	305	215	0.02%	0.002%
20	4.954	1123	1124	1131	rVB2	209	198	0.02%	0.001%
21	5.083	1146	1164	1185	rBV	226408	498751	39.49%	3.736%
22	5.333	1227	1242	1259	rBV2	48510	105830	8.38%	0.793%
23	5.462	1279	1282	1286	rVB	277	215	0.02%	0.002%
24	5.539	1289	1306	1325	rVB2	52552	114646	9.08%	0.859%
25	5.616	1327	1330	1333	rVB2	293	231	0.02%	0.002%
26	5.742	1346	1369	1379	rBV2	470980	1262932	100.00%	9.460%
27	5.899	1415	1418	1420	rBV	487	310	0.02%	0.002%
28	6.102	1476	1481	1484	rBV2	268	254	0.02%	0.002%
29	6.263	1515	1531	1548	rBV	375541	701718	55.56%	5.256%
30	6.372	1562	1565	1569	rVB2	420	297	0.02%	0.002%
31	6.555	1607	1622	1636	rVB	81519	152951	12.11%	1.146%
32	6.703	1653	1668	1685	rBV	299858	571574	45.26%	4.282%
33	6.803	1686	1699	1719	rVB2	124967	239045	18.93%	1.791%
34	6.964	1747	1749	1754	rVB	425	365	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100620\
 Data File : VU040533.D
 Acq On : 06 Oct 2020 17:52
 Operator : SY/MD
 Sample : TEST
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TEST

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
 Title : VOC Analysis

35	6.993	1754	1758	1763	rBV2	332	416	0.03%	0.003%
36	7.185	1810	1818	1819	rBV3	603	536	0.04%	0.004%
37	7.221	1825	1829	1832	rBV2	230	213	0.02%	0.002%
38	7.501	1910	1916	1918	rBV2	193	202	0.02%	0.002%
39	7.529	1918	1925	1926	rBV	259	280	0.02%	0.002%
40	7.575	1926	1939	1955	rBV	167892	287520	22.77%	2.154%
41	7.677	1967	1971	1979	rBV5	551	746	0.06%	0.006%
42	7.800	2001	2009	2011	rBV2	931	910	0.07%	0.007%
43	7.906	2028	2042	2054	rBV	568718	955618	75.67%	7.158%
44	7.976	2054	2064	2079	rVB	150149	253982	20.11%	1.903%
45	8.121	2103	2109	2114	rBV3	362	463	0.04%	0.003%
46	8.185	2115	2129	2145	rVV	123877	205827	16.30%	1.542%
47	8.247	2145	2148	2153	rVB4	435	377	0.03%	0.003%
48	8.337	2173	2176	2182	rBV4	499	488	0.04%	0.004%
49	8.407	2186	2198	2215	rBV	133633	228239	18.07%	1.710%
50	8.558	2233	2245	2257	rBV	115754	190307	15.07%	1.426%
51	8.639	2257	2270	2295	rBV	403639	689752	54.62%	5.167%
52	8.870	2339	2342	2349	rBV2	318	282	0.02%	0.002%
53	8.915	2349	2356	2370	rBV4	1587	3186	0.25%	0.024%
54	9.034	2389	2393	2396	rBV3	306	271	0.02%	0.002%
55	9.073	2403	2405	2411	rVB2	401	377	0.03%	0.003%
56	9.166	2432	2434	2439	rBV	276	204	0.02%	0.002%
57	9.211	2446	2448	2456	rVB3	338	323	0.03%	0.002%
58	9.259	2461	2463	2466	rVB	362	209	0.02%	0.002%
59	9.291	2470	2473	2477	rBV	335	286	0.02%	0.002%
60	9.420	2500	2513	2537	rBV2	546317	1057355	83.72%	7.920%
61	9.571	2548	2560	2573	rBV	123841	194495	15.40%	1.457%
62	9.697	2586	2599	2613	rVV	139238	228018	18.05%	1.708%
63	9.774	2618	2623	2627	rBV3	404	358	0.03%	0.003%
64	9.922	2666	2669	2678	rVB	235	283	0.02%	0.002%
65	10.105	2713	2726	2748	rBV4	244869	492694	39.01%	3.691%
66	10.488	2840	2845	2846	rBV2	320	278	0.02%	0.002%
67	10.642	2890	2893	2898	rBV	324	349	0.03%	0.003%
68	10.754	2916	2928	2946	rVV	382066	614371	48.65%	4.602%
69	10.819	2946	2948	2953	rVB2	528	409	0.03%	0.003%
70	10.880	2963	2967	2969	rBV2	458	291	0.02%	0.002%
71	11.089	3030	3032	3036	rVB2	511	315	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100620\
 Data File : VU040533.D
 Acq On : 06 Oct 2020 17:52
 Operator : SY/MD
 Sample : TEST
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TEST

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
 Title : VOC Analysis

72	11.275	3086	3090	3092	rBV2	291	249	0.02%	0.002%
73	11.462	3143	3148	3154	rBV3	520	619	0.05%	0.005%
74	11.539	3165	3172	3178	rVB2	397	641	0.05%	0.005%
75	11.568	3178	3181	3184	rBV2	283	237	0.02%	0.002%
76	11.661	3205	3210	3216	rVB2	363	378	0.03%	0.003%
77	11.735	3230	3233	3235	rBV3	701	424	0.03%	0.003%
78	11.809	3243	3256	3276	rBV2	566787	1127408	89.27%	8.445%
79	11.931	3290	3294	3296	rBV3	584	424	0.03%	0.003%
80	12.063	3331	3335	3341	rBV2	355	427	0.03%	0.003%
81	12.188	3361	3374	3393	rBV2	605132	1178230	93.29%	8.826%
82	12.269	3396	3399	3403	rVB2	373	226	0.02%	0.002%
83	12.369	3428	3430	3437	rVB3	360	306	0.02%	0.002%
84	12.606	3500	3504	3506	rBV	276	239	0.02%	0.002%
85	12.697	3528	3532	3537	rVB2	299	335	0.03%	0.003%
86	12.761	3547	3552	3554	rBV3	483	486	0.04%	0.004%
87	12.992	3622	3624	3632	rVB2	385	306	0.02%	0.002%
88	13.092	3649	3655	3659	rBV	551	574	0.05%	0.004%
89	13.169	3676	3679	3682	rBV2	381	307	0.02%	0.002%
90	13.211	3688	3692	3698	rBV3	771	855	0.07%	0.006%
91	13.574	3802	3805	3810	rBV	371	226	0.02%	0.002%
92	13.832	3873	3885	3903	rBV	142251	220830	17.49%	1.654%
93	13.928	3913	3915	3918	rBV	292	202	0.02%	0.002%
94	14.076	3955	3961	3967	rVB4	2037	2178	0.17%	0.016%
95	14.176	3988	3992	3995	rBV2	383	340	0.03%	0.003%
96	14.317	4031	4036	4050	rBV6	1799	3053	0.24%	0.023%
97	15.114	4281	4284	4288	rVB	540	421	0.03%	0.003%
98	15.137	4288	4291	4293	rBV	519	406	0.03%	0.003%
99	15.799	4495	4497	4501	rBV2	500	287	0.02%	0.002%
100	15.838	4505	4509	4513	rBV2	1000	965	0.08%	0.007%


Sum of corrected areas: 13349755

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100620\
Data File : VU040533.D
Acq On : 06 Oct 2020 17:52
Operator : SY/MD
Sample : TEST
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TEST

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

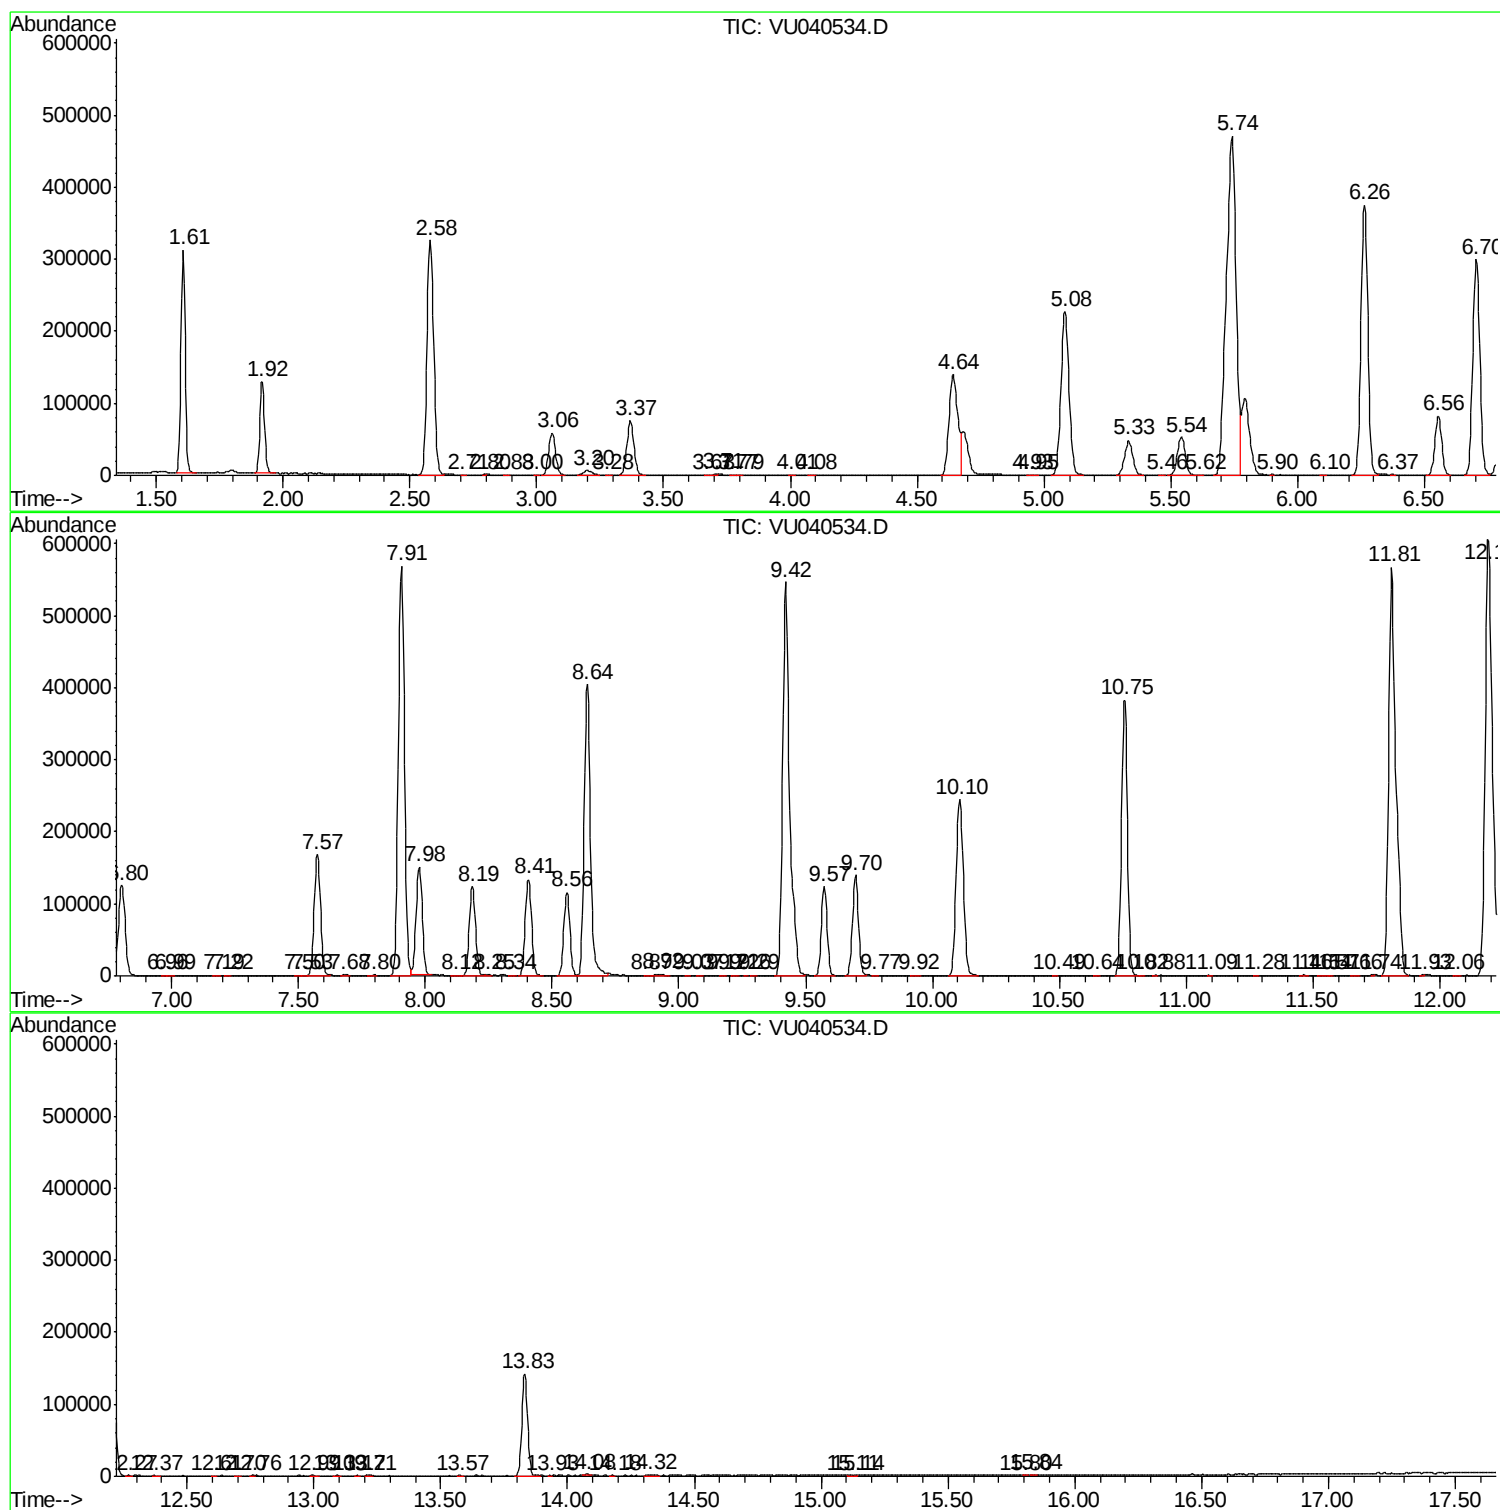

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU100620\
Data File : VU040533.D
Acq On : 06 Oct 2020 17:52
Operator : SY/MD
Sample : TEST
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TEST

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU100620\
Data File : VU040533.D
Acq On : 06 Oct 2020 17:52
Operator : SY/MD
Sample : TEST
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TEST

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc