


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU100620\
 Data File : VU040521.D
 Acq On : 06 Oct 2020 12:24
 Operator : SY/MD
 Sample : BFB32
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB201

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
 Title : VOC Analysis
 Last Update : Wed Oct 07 08:04:20 2020

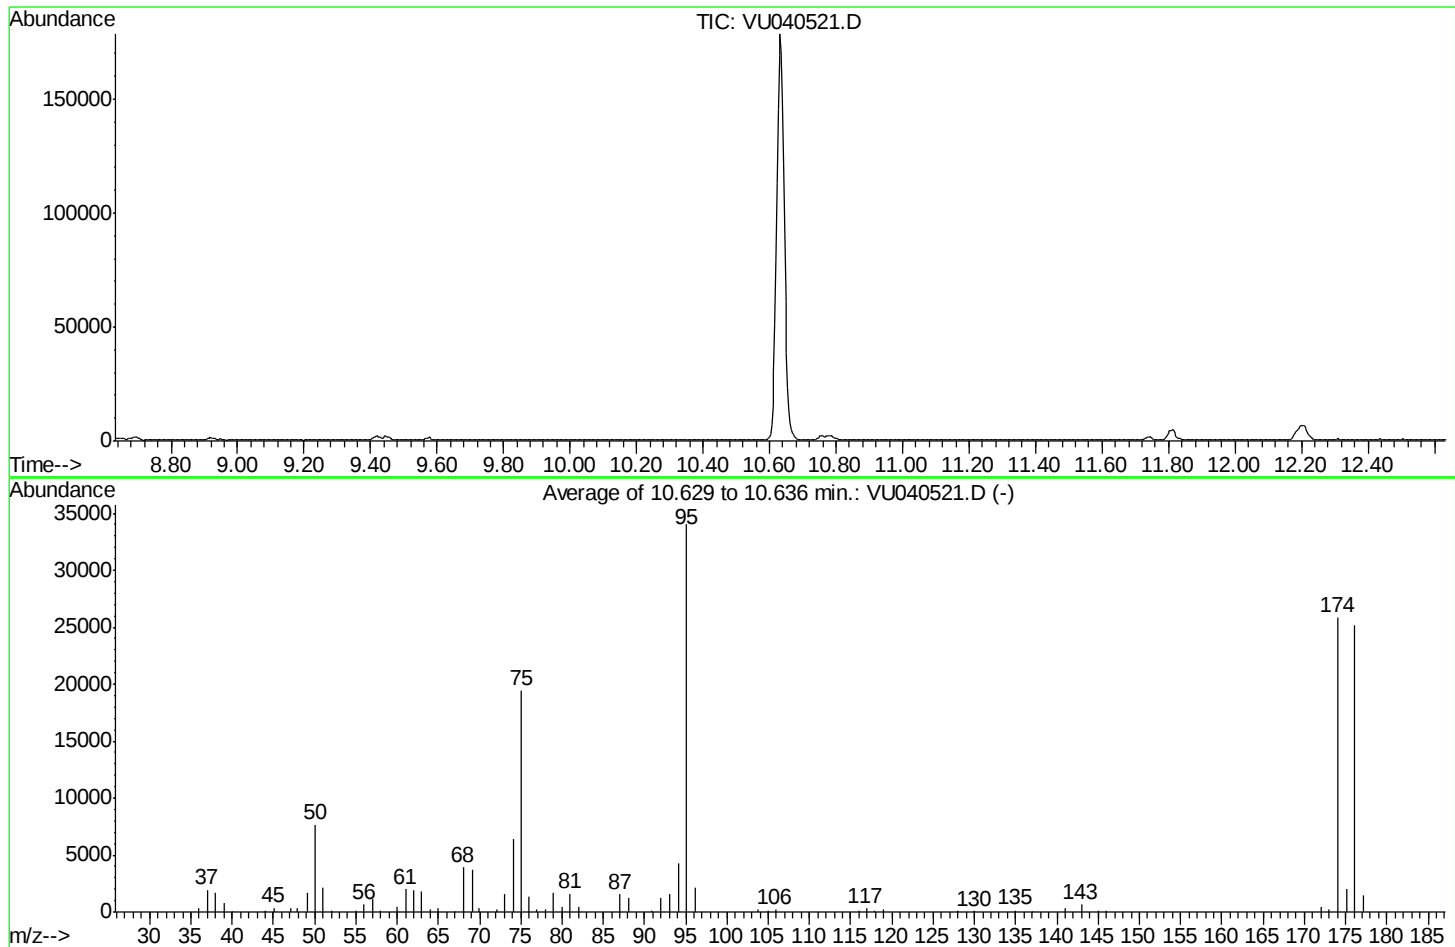

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	7675	PASS
75	95	30	80	57.0	19402	PASS
95	95	100	100	100.0	34029	PASS
96	95	5	9	6.4	2180	PASS
173	174	0.00	2	0.9	244	PASS
174	95	50	120	75.8	25792	PASS
175	174	5	9	7.7	1983	PASS
176	174	95	101	97.8	25218	PASS
177	176	5	9	6.0	1509	PASS

m/z	Abundance
35.90	291.0
37.00	1863.0
38.00	1649.0
39.00	851.0
39.90	233.0
44.00	736.0
45.00	396.0
47.10	422.0
47.90	282.0
49.10	1753.0
50.10	7686.0
51.00	2082.0
52.00	130.0
55.10	135.0
56.00	677.0
57.00	1185.0
60.10	338.0
61.00	2057.0
62.10	2087.0
63.00	1785.0
64.10	310.0
65.00	316.0
67.00	108.0
68.00	4000.0
69.10	3667.0
70.00	362.0
72.00	207.0
73.00	1627.0
74.10	6418.0
75.10	18728.0
76.00	1293.0
76.90	233.0
78.00	142.0
78.90	1734.0
80.00	446.0
80.90	1525.0
81.90	443.0
87.10	1527.0
88.10	1191.0
90.90	106.0
92.00	1290.0
93.00	1517.0
94.10	4008.0
95.10	33128.0
96.10	2211.0
103.80	256.0
105.00	164.0
105.90	181.0
116.00	160.0
116.90	296.0
117.90	112.0
119.00	248.0
128.00	110.0
130.00	101.0
135.10	114.0
137.00	101.0
141.00	344.0
143.00	602.0
145.00	121.0
145.90	119.0
172.00	450.0
174.10	24912.0
175.10	1869.0
176.10	24392.0
177.10	1433.0

Instrument :
MSVOA_U
ClientSampleId :
BFB201

m/z	Abundance
35.00	325.0
37.00	1973.0
38.00	1680.0
39.00	884.0
39.00	237.0
44.00	632.0
45.10	417.0
47.10	399.0
47.90	340.0
49.10	1692.0
50.10	7942.0
51.00	2193.0
52.00	146.0
55.00	129.0
56.00	650.0
57.00	1227.0
57.90	113.0
60.10	428.0
61.10	2073.0
62.10	2001.0
63.00	1832.0
64.00	292.0
65.00	326.0
68.00	4105.0
69.10	3757.0
69.90	363.0
72.00	244.0
73.10	1531.0
74.10	6644.0
75.10	19896.0
76.00	1379.0
76.90	190.0
78.00	181.0
78.90	1729.0
80.00	482.0
81.00	1690.0
82.00	485.0
87.10	1593.0
88.10	1315.0
90.90	136.0
92.00	1242.0
93.00	1613.0
94.10	4396.0
95.10	35032.0
96.10	2257.0
103.80	235.0
105.00	134.0
105.90	229.0
115.90	163.0
116.90	315.0
118.00	131.0
119.00	240.0
127.90	100.0
130.00	118.0
135.00	152.0
141.00	418.0
143.00	656.0
145.00	157.0
146.00	134.0
172.10	498.0
173.00	380.0
174.10	26672.0
175.10	2048.0
176.10	26064.0
177.10	1550.0

Instrument :
MSVOA_U
ClientSampleId :
BFB201

m/z	Abundance
35.90	337.0
37.00	1925.0
38.00	1579.0
39.10	806.0
40.00	217.0
44.00	561.0
45.10	370.0
47.00	358.0
47.90	328.0
49.10	1515.0
50.10	7399.0
51.00	2164.0
52.00	131.0
54.90	130.0
56.00	610.0
57.00	1100.0
57.90	102.0
60.00	506.0
61.00	1856.0
62.00	1790.0
63.00	1635.0
64.00	235.0
65.00	324.0
68.10	3694.0
69.10	3586.0
69.90	309.0
72.10	272.0
73.10	1508.0
74.10	6222.0
75.10	19584.0
76.00	1427.0
77.00	153.0
78.00	220.0
78.90	1492.0
80.00	484.0
81.00	1650.0
82.00	460.0
87.00	1513.0
88.00	1377.0
90.90	122.0
92.00	1085.0
93.00	1562.0
94.10	4423.0
95.10	33928.0
96.10	2072.0
103.90	153.0
105.90	250.0
115.90	151.0
116.90	302.0
118.00	140.0
119.00	212.0
127.90	107.0
130.10	117.0
134.90	122.0
141.00	430.0
143.00	685.0
145.00	159.0
146.00	119.0
172.00	431.0
173.00	353.0
174.10	25792.0
175.10	2033.0
176.10	25200.0
177.10	1546.0

Instrument :
MSVOA_U
ClientSampleId :
BFB201

Scan 2877 (10.591 min): VU040521.D
BFB32

m/z	Abundance
39.90	208.0
44.00	569.0

Instrument :
MSVOA_U
ClientSampleId :
BFB201