

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
 Data File : VU045176.D
 Acq On : 06 Oct 2021 11:28
 Operator : SY/MD
 Sample : M4024-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU0451176.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	36	42	53	rBV	7595	12831	1.01%	0.130%
2	1.600	74	81	93	rBV	160816	175159	13.75%	1.781%
3	1.909	168	177	194	rVB	122370	173463	13.61%	1.763%
4	2.568	367	382	399	rBV	252512	426043	33.44%	4.331%
5	2.684	415	418	421	rVB	225	152	0.01%	0.002%
6	2.777	442	447	450	rBV2	624	771	0.06%	0.008%
7	3.047	529	531	536	rVB2	437	344	0.03%	0.003%
8	3.198	567	578	586	rVV2	822	1702	0.13%	0.017%
9	3.356	624	627	632	rBV	269	291	0.02%	0.003%
10	3.404	639	642	645	rBV	207	186	0.01%	0.002%
11	3.514	672	676	678	rBV2	245	218	0.02%	0.002%
12	3.571	689	694	695	rBV	185	157	0.01%	0.002%
13	3.626	706	711	714	rBV2	217	258	0.02%	0.003%
14	3.694	729	732	737	rVB2	174	161	0.01%	0.002%
15	3.722	737	741	747	rBV2	206	297	0.02%	0.003%
16	3.755	750	751	757	rVB	251	233	0.02%	0.002%
17	3.838	774	777	782	rVB2	234	196	0.02%	0.002%
18	3.864	782	785	787	rBV2	331	257	0.02%	0.003%
19	4.038	836	839	843	rVB2	236	201	0.02%	0.002%
20	4.070	843	849	853	rBV	267	266	0.02%	0.003%
21	4.282	912	915	921	rVB2	216	246	0.02%	0.003%
22	4.488	975	979	983	rBV2	213	246	0.02%	0.003%
23	4.626	1007	1022	1053	rVV	139766	360533	28.30%	3.665%
24	4.861	1092	1095	1100	rBV2	195	194	0.02%	0.002%
25	4.954	1120	1124	1128	rVB	239	219	0.02%	0.002%
26	5.070	1142	1160	1182	rBV	225981	493874	38.76%	5.020%
27	5.195	1196	1199	1203	rVB2	225	189	0.01%	0.002%
28	5.218	1203	1206	1214	rVB4	475	595	0.05%	0.006%
29	5.253	1214	1217	1221	rBV	248	205	0.02%	0.002%
30	5.321	1223	1238	1252	rVB6	5986	13980	1.10%	0.142%
31	5.449	1273	1278	1280	rBV2	222	191	0.01%	0.002%
32	5.607	1320	1327	1331	rBV2	197	221	0.02%	0.002%
33	5.729	1341	1365	1386	rBV2	472059	1274119	100.00%	12.952%
34	6.031	1454	1459	1462	rBV2	255	292	0.02%	0.003%
35	6.253	1513	1528	1549	rBV	378261	712293	55.90%	7.241%
36	6.410	1575	1577	1580	rVB3	285	167	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
 Data File : VU045176.D
 Acq On : 06 Oct 2021 11:28
 Operator : SY/MD
 Sample : M4024-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COAH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.546	1606	1619	1641	rBV3	137631	261905	20.56%	2.662%
38	6.697	1652	1666	1685	rBV	302148	583455	45.79%	5.931%
39	6.883	1723	1724	1728	rVB	403	217	0.02%	0.002%
40	7.018	1763	1766	1769	rBV2	214	174	0.01%	0.002%
41	7.044	1769	1774	1776	rBV	391	355	0.03%	0.004%
42	7.189	1810	1819	1826	rVB3	1862	2886	0.23%	0.029%
43	7.436	1889	1896	1900	rBV2	157	242	0.02%	0.002%
44	7.568	1924	1937	1960	rVV	155985	270596	21.24%	2.751%
45	7.687	1967	1974	1983	rBV3	1340	2013	0.16%	0.020%
46	7.751	1992	1994	1997	rVB	302	172	0.01%	0.002%
47	7.774	1997	2001	2003	rBV2	178	171	0.01%	0.002%
48	7.902	2022	2041	2057	rBV	579901	989067	77.63%	10.054%
49	7.976	2057	2064	2073	rVB	8346	14226	1.12%	0.145%
50	8.182	2116	2128	2150	rVV	109105	180903	14.20%	1.839%
51	8.423	2199	2203	2205	rBV2	278	231	0.02%	0.002%
52	8.471	2215	2218	2223	rBV2	193	217	0.02%	0.002%
53	8.555	2240	2244	2248	rBV2	274	241	0.02%	0.002%
54	8.635	2254	2269	2299	rBV	389646	703137	55.19%	7.148%
55	8.812	2322	2324	2330	rVB2	294	215	0.02%	0.002%
56	8.841	2330	2333	2336	rBV2	345	240	0.02%	0.002%
57	8.906	2350	2353	2359	rVB2	202	240	0.02%	0.002%
58	8.992	2374	2380	2383	rBV2	216	231	0.02%	0.002%
59	9.041	2392	2395	2399	rBV2	233	218	0.02%	0.002%
60	9.182	2434	2439	2441	rBV2	180	173	0.01%	0.002%
61	9.201	2441	2445	2448	rVV	245	220	0.02%	0.002%
62	9.336	2483	2487	2490	rBV	256	247	0.02%	0.003%
63	9.420	2500	2513	2552	rBV	543300	884964	69.46%	8.996%
64	9.571	2555	2560	2566	rVB3	331	367	0.03%	0.004%
65	9.697	2592	2599	2607	rVB2	1096	1436	0.11%	0.015%
66	9.790	2624	2628	2631	rBV	205	202	0.02%	0.002%
67	10.102	2721	2725	2730	rVB2	250	249	0.02%	0.003%
68	10.179	2743	2749	2754	rBV	231	294	0.02%	0.003%
69	10.217	2759	2761	2767	rBV2	162	155	0.01%	0.002%
70	10.320	2789	2793	2797	rBV2	184	192	0.02%	0.002%
71	10.674	2895	2903	2912	rBV3	1644	2159	0.17%	0.022%
72	10.761	2917	2930	2952	rVB	405371	646506	50.74%	6.572%
73	10.899	2969	2973	2977	rBV	261	218	0.02%	0.002%
74	10.944	2984	2987	2990	rBV2	206	175	0.01%	0.002%
75	11.002	3000	3005	3008	rBV	343	315	0.02%	0.003%
76	11.041	3014	3017	3020	rVB	275	173	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
 Data File : VU045176.D
 Acq On : 06 Oct 2021 11:28
 Operator : SY/MD
 Sample : M4024-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.459	3141	3147	3148	rBV4	586	471	0.04%	0.005%
78	11.468	3148	3150	3152	rVB	589	331	0.03%	0.003%
79	11.635	3193	3202	3204	rBV2	725	887	0.07%	0.009%
80	11.696	3215	3221	3225	rBV3	614	611	0.05%	0.006%
81	11.815	3246	3258	3277	rBV	491548	782803	61.44%	7.958%
82	11.979	3304	3309	3314	rVB2	725	851	0.07%	0.009%
83	12.198	3361	3377	3392	rBV	520733	841797	66.07%	8.557%
84	12.362	3422	3428	3435	rBV2	283	370	0.03%	0.004%
85	12.722	3534	3540	3541	rBV2	276	325	0.03%	0.003%
86	12.825	3569	3572	3577	rBV2	259	246	0.02%	0.003%
87	12.944	3607	3609	3615	rVB2	229	191	0.01%	0.002%
88	12.973	3615	3618	3620	rBV2	223	185	0.01%	0.002%
89	13.034	3634	3637	3639	rBV2	272	187	0.01%	0.002%
90	13.105	3655	3659	3661	rBV	264	216	0.02%	0.002%
91	13.175	3678	3681	3684	rBV2	215	204	0.02%	0.002%
92	13.847	3887	3890	3902	rVB3	853	1204	0.09%	0.012%
93	13.893	3902	3904	3907	rBV	219	170	0.01%	0.002%
94	14.095	3957	3967	3978	rBV	2305	3662	0.29%	0.037%
95	14.336	4036	4042	4043	rBV2	561	576	0.05%	0.006%
96	14.825	4190	4194	4198	rBV2	320	370	0.03%	0.004%
97	14.880	4205	4211	4216	rBV	411	624	0.05%	0.006%
98	14.925	4222	4225	4227	rBV2	398	297	0.02%	0.003%
99	16.236	4631	4633	4635	rBV2	400	244	0.02%	0.002%
100	16.632	4754	4756	4758	rBV3	467	260	0.02%	0.003%




Sum of corrected areas: 9837229

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
Data File : VU045176.D
Acq On : 06 Oct 2021 11:28
Operator : SY/MD
Sample : M4024-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

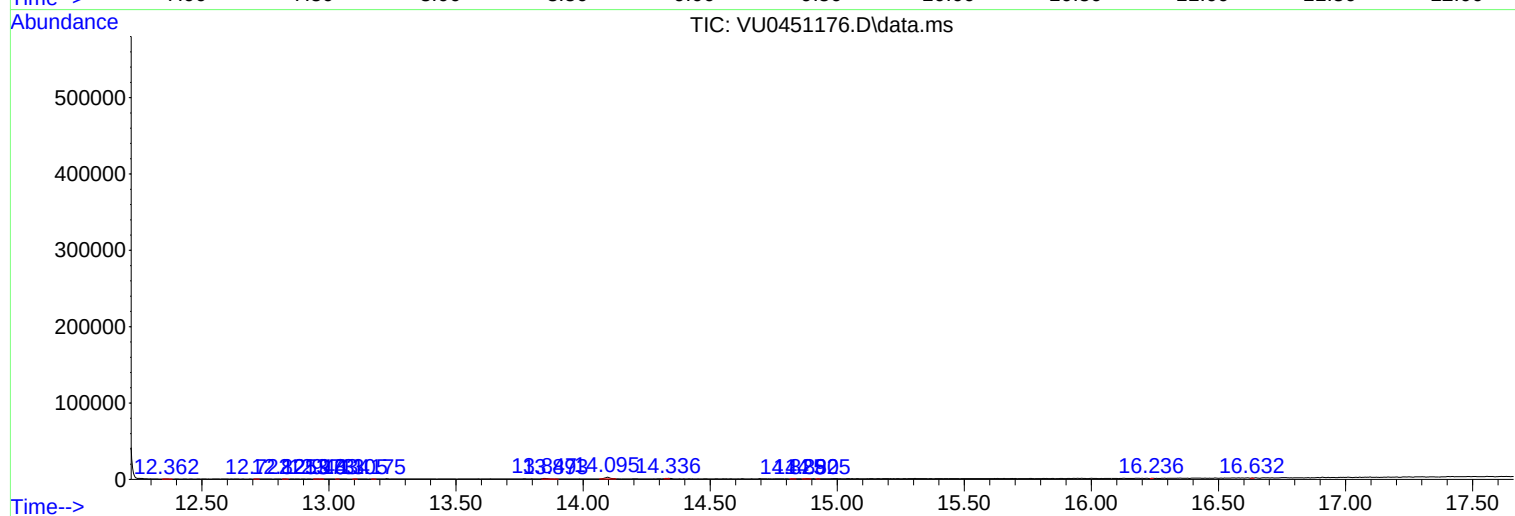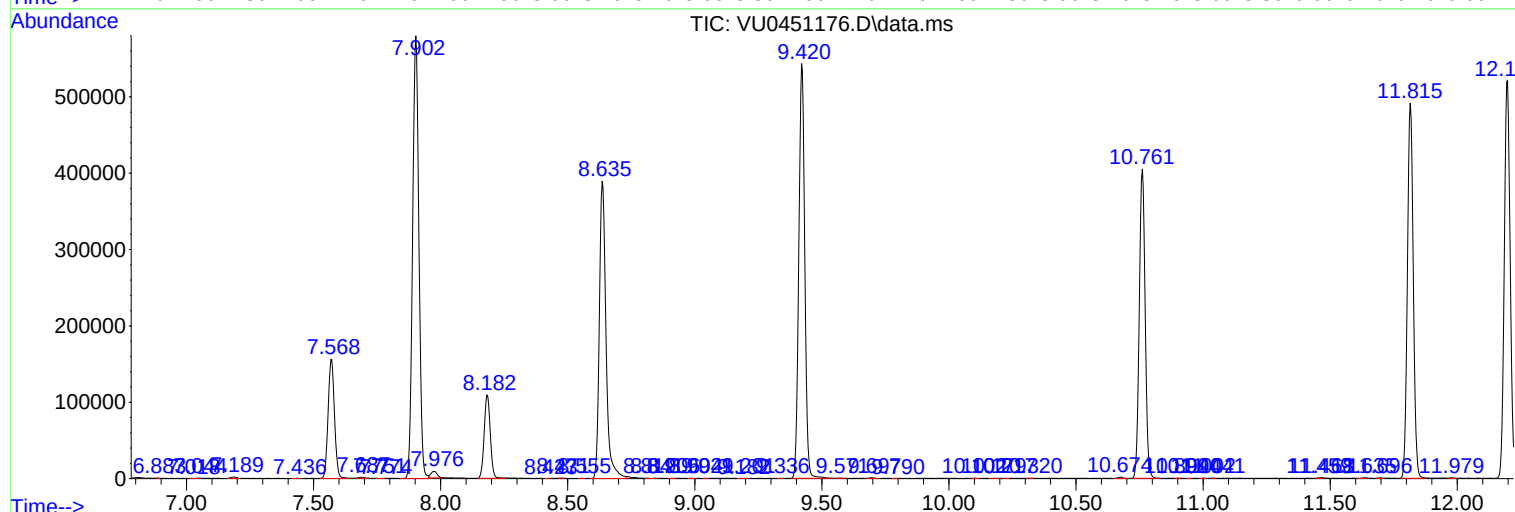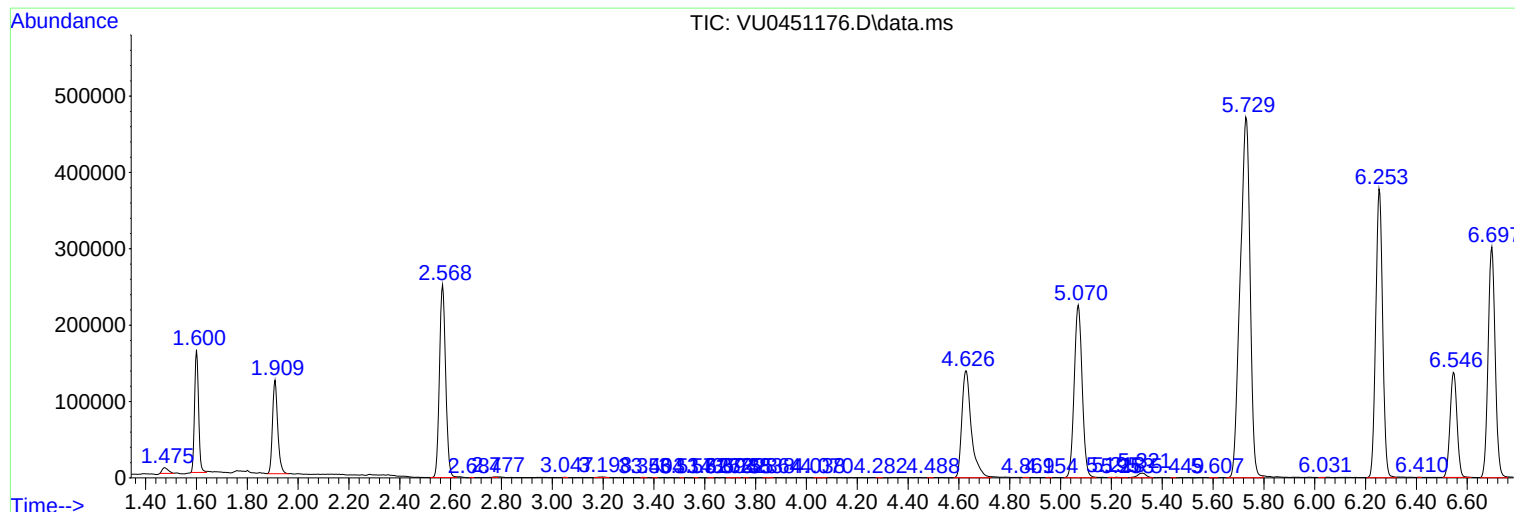

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
Data File : VU045176.D
Acq On : 06 Oct 2021 11:28
Operator : SY/MD
Sample : M4024-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
Data File : VU045176.D
Acq On : 06 Oct 2021 11:28
Operator : SY/MD
Sample : M4024-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
