

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
 Data File : VU045177.D
 Acq On : 06 Oct 2021 11:51
 Operator : SY/MD
 Sample : M4024-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU0451177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.472	35	41	53	rBV	8378	15541	1.21%	0.162%
2	1.601	74	81	99	rVB	163441	177357	13.82%	1.848%
3	1.906	168	176	195	rVB	125473	176018	13.72%	1.834%
4	2.568	369	382	397	rBV	244988	411870	32.10%	4.292%
5	2.768	431	444	458	rBV3	2565	5508	0.43%	0.057%
6	2.993	511	514	521	rVB2	224	306	0.02%	0.003%
7	3.025	521	524	526	rBV	239	194	0.02%	0.002%
8	3.047	526	531	538	rVV3	737	934	0.07%	0.010%
9	3.083	538	542	546	rVB2	263	224	0.02%	0.002%
10	3.115	546	552	553	rBV2	211	214	0.02%	0.002%
11	3.128	553	556	560	rVV	238	201	0.02%	0.002%
12	3.189	564	575	592	rVV2	2622	6446	0.50%	0.067%
13	3.327	614	618	620	rBV	186	166	0.01%	0.002%
14	3.420	644	647	651	rVV	139	145	0.01%	0.002%
15	3.443	651	654	658	rVB	155	145	0.01%	0.002%
16	3.562	682	691	694	rBV2	234	369	0.03%	0.004%
17	3.581	694	697	698	rVV	295	192	0.01%	0.002%
18	3.591	698	700	707	rVB3	415	454	0.04%	0.005%
19	3.674	722	726	734	rVB	336	517	0.04%	0.005%
20	3.736	740	745	749	rBV	200	261	0.02%	0.003%
21	3.816	765	770	775	rVB2	211	290	0.02%	0.003%
22	3.861	780	784	785	rBV	330	191	0.01%	0.002%
23	3.877	785	789	791	rBV	295	250	0.02%	0.003%
24	3.916	798	801	804	rBV2	192	143	0.01%	0.001%
25	3.951	809	812	816	rVB2	221	160	0.01%	0.002%
26	3.996	823	826	829	rBV2	187	161	0.01%	0.002%
27	4.337	927	932	935	rBV	171	216	0.02%	0.002%
28	4.382	940	946	948	rBV2	200	244	0.02%	0.003%
29	4.446	963	966	968	rBV2	217	177	0.01%	0.002%
30	4.530	983	992	995	rBV2	250	422	0.03%	0.004%
31	4.552	995	999	1003	rVV2	158	156	0.01%	0.002%
32	4.626	1008	1022	1048	rBV	146102	354136	27.60%	3.690%
33	4.967	1124	1128	1131	rBV	286	200	0.02%	0.002%
34	5.067	1143	1159	1183	rBV	225950	495303	38.61%	5.161%
35	5.224	1204	1208	1210	rVB3	376	245	0.02%	0.003%
36	5.244	1211	1214	1219	rVB2	270	232	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
 Data File : VU045177.D
 Acq On : 06 Oct 2021 11:51
 Operator : SY/MD
 Sample : M4024-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.295	1221	1230	1233	rBV3	709	1073	0.08%	0.011%
38	5.379	1251	1256	1259	rBV3	431	381	0.03%	0.004%
39	5.443	1274	1276	1280	rVV2	215	197	0.02%	0.002%
40	5.536	1298	1305	1307	rBV2	179	205	0.02%	0.002%
41	5.613	1326	1329	1334	rBV2	153	156	0.01%	0.002%
42	5.729	1343	1365	1390	rBV2	474833	1282952	100.00%	13.369%
43	6.157	1494	1498	1504	rVB2	205	265	0.02%	0.003%
44	6.186	1504	1507	1511	rVB2	249	219	0.02%	0.002%
45	6.253	1511	1528	1551	rBV	373464	697518	54.37%	7.268%
46	6.417	1576	1579	1580	rBV2	245	143	0.01%	0.001%
47	6.472	1593	1596	1602	rVB2	324	297	0.02%	0.003%
48	6.546	1602	1619	1633	rBV4	51724	100433	7.83%	1.047%
49	6.697	1650	1666	1688	rBV	303779	591217	46.08%	6.161%
50	6.845	1709	1712	1715	rBV3	291	174	0.01%	0.002%
51	6.915	1732	1734	1742	rVB2	235	282	0.02%	0.003%
52	6.954	1742	1746	1748	rVB2	280	224	0.02%	0.002%
53	6.993	1753	1758	1764	rBV2	194	290	0.02%	0.003%
54	7.034	1767	1771	1773	rVV	246	228	0.02%	0.002%
55	7.047	1773	1775	1786	rVB2	409	509	0.04%	0.005%
56	7.182	1810	1817	1829	rVV3	1920	3265	0.25%	0.034%
57	7.568	1921	1937	1960	rVV	155940	268268	20.91%	2.795%
58	7.687	1964	1974	1982	rVB3	1255	2463	0.19%	0.026%
59	7.903	2026	2041	2056	rVV	569952	983754	76.68%	10.251%
60	7.973	2056	2063	2081	rVB	10545	19038	1.48%	0.198%
61	8.182	2116	2128	2147	rBV	109613	182275	14.21%	1.899%
62	8.346	2174	2179	2181	rBV	340	334	0.03%	0.003%
63	8.558	2240	2245	2252	rBV3	458	455	0.04%	0.005%
64	8.636	2255	2269	2311	rBV	397795	721532	56.24%	7.519%
65	8.777	2311	2313	2314	rBV	581	216	0.02%	0.002%
66	9.321	2479	2482	2489	rBV2	207	280	0.02%	0.003%
67	9.420	2498	2513	2532	rBV	520345	857124	66.81%	8.932%
68	9.693	2590	2598	2607	rBV2	1675	2863	0.22%	0.030%
69	9.816	2633	2636	2640	rBV	184	148	0.01%	0.002%
70	9.935	2670	2673	2675	rBV	204	152	0.01%	0.002%
71	10.050	2706	2709	2712	rVB	201	147	0.01%	0.002%
72	10.140	2732	2737	2739	rBV2	272	274	0.02%	0.003%
73	10.179	2745	2749	2751	rBV2	151	153	0.01%	0.002%
74	10.327	2791	2795	2799	rBV2	253	320	0.02%	0.003%
75	10.436	2824	2829	2838	rBV2	239	407	0.03%	0.004%
76	10.616	2882	2885	2888	rBV	249	206	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
 Data File : VU045177.D
 Acq On : 06 Oct 2021 11:51
 Operator : SY/MD
 Sample : M4024-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.677	2897	2904	2911	rVB4	1808	2638	0.21%	0.027%
78	10.761	2917	2930	2951	rVB	404625	650732	50.72%	6.781%
79	10.999	3001	3004	3010	rVB3	430	539	0.04%	0.006%
80	11.034	3010	3015	3019	rBV2	245	311	0.02%	0.003%
81	11.111	3037	3039	3043	rVB2	315	171	0.01%	0.002%
82	11.134	3043	3046	3050	rBV2	165	177	0.01%	0.002%
83	11.275	3087	3090	3092	rBV2	199	161	0.01%	0.002%
84	11.391	3123	3126	3129	rBV2	183	160	0.01%	0.002%
85	11.436	3137	3140	3141	rBV	260	159	0.01%	0.002%
86	11.462	3141	3148	3157	rVB3	1340	1908	0.15%	0.020%
87	11.513	3162	3164	3168	rVB	245	175	0.01%	0.002%
88	11.697	3217	3221	3227	rVB4	697	709	0.06%	0.007%
89	11.816	3245	3258	3281	rBV	472236	739372	57.63%	7.705%
90	11.902	3281	3285	3289	rBV4	391	420	0.03%	0.004%
91	11.980	3305	3309	3314	rVB5	1060	1036	0.08%	0.011%
92	12.012	3314	3319	3325	rBV2	176	222	0.02%	0.002%
93	12.076	3333	3339	3343	rBV3	414	590	0.05%	0.006%
94	12.195	3363	3376	3397	rBV	511101	825245	64.32%	8.599%
95	12.497	3467	3470	3474	rBV	224	178	0.01%	0.002%
96	12.578	3491	3495	3497	rBV	239	218	0.02%	0.002%
97	13.902	3902	3907	3910	rBV	308	353	0.03%	0.004%
98	14.266	4018	4020	4024	rBV	210	174	0.01%	0.002%
99	14.336	4039	4042	4049	rBV2	415	462	0.04%	0.005%
100	15.182	4301	4305	4307	rBV3	409	359	0.03%	0.004%




Sum of corrected areas: 9596494

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
Data File : VU045177.D
Acq On : 06 Oct 2021 11:51
Operator : SY/MD
Sample : M4024-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COAL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

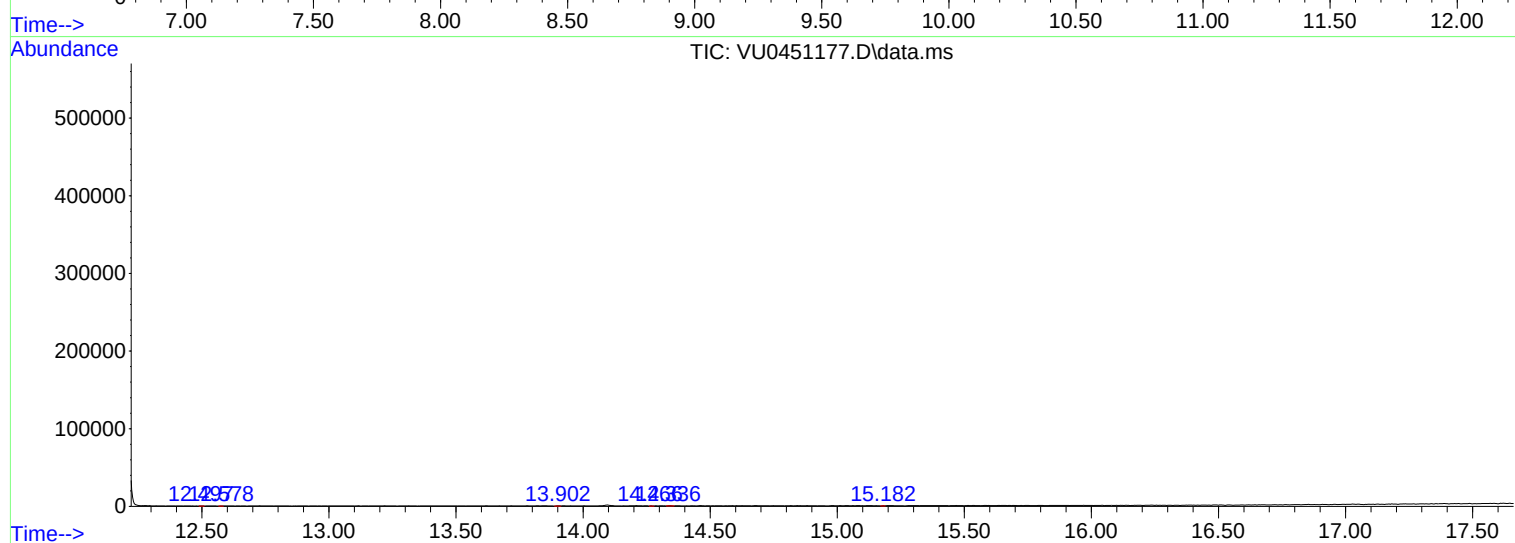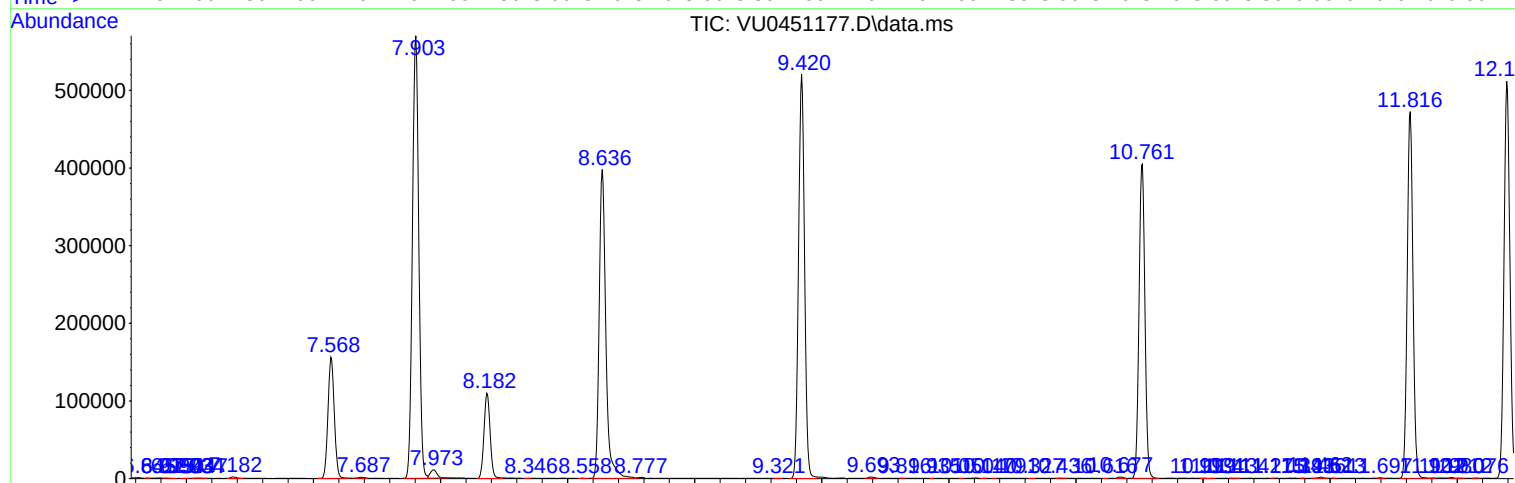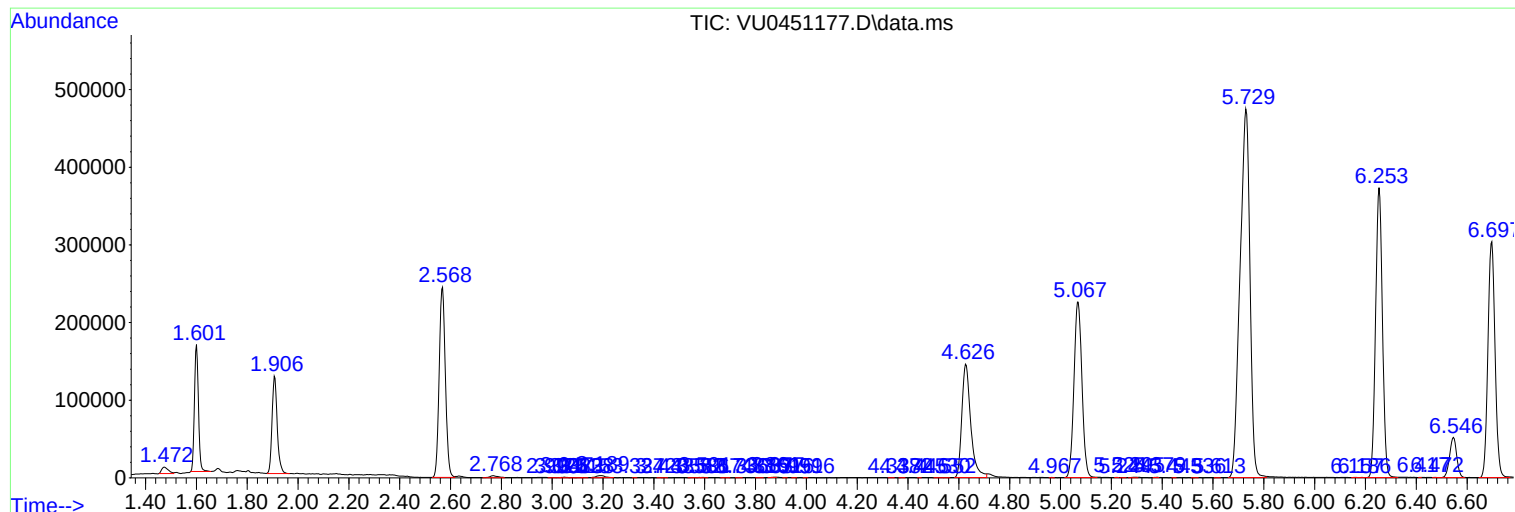

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
Data File : VU045177.D
Acq On : 06 Oct 2021 11:51
Operator : SY/MD
Sample : M4024-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
Data File : VU045177.D
Acq On : 06 Oct 2021 11:51
Operator : SY/MD
Sample : M4024-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
