

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
 Data File : VU045178.D
 Acq On : 06 Oct 2021 12:15
 Operator : SY/MD
 Sample : M4024-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU0451178.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	36	42	54	rVB	8331	14041	1.09%	0.141%
2	1.601	73	81	97	rBV	167255	186889	14.52%	1.880%
3	1.906	168	176	193	rVB	127471	176613	13.72%	1.776%
4	2.565	369	381	397	rBV	257101	434751	33.77%	4.373%
5	2.768	436	444	451	rBV2	1178	2252	0.17%	0.023%
6	2.954	498	502	504	rBV	264	236	0.02%	0.002%
7	2.996	512	515	519	rBV	220	183	0.01%	0.002%
8	3.048	529	531	532	rBV	323	146	0.01%	0.001%
9	3.086	539	543	549	rBV2	212	233	0.02%	0.002%
10	3.186	564	574	576	rBV	2066	2560	0.20%	0.026%
11	3.250	590	594	596	rBV	190	177	0.01%	0.002%
12	3.292	601	607	611	rBV2	307	379	0.03%	0.004%
13	3.311	611	613	618	rVV	179	151	0.01%	0.002%
14	3.392	637	638	645	rVB2	235	288	0.02%	0.003%
15	3.424	645	648	651	rBV	228	193	0.01%	0.002%
16	3.559	685	690	693	rBV	233	233	0.02%	0.002%
17	3.659	715	721	723	rBV	262	233	0.02%	0.002%
18	3.733	741	744	749	rVB	211	203	0.02%	0.002%
19	3.842	774	778	780	rBV	231	202	0.02%	0.002%
20	3.868	783	786	789	rBV2	431	327	0.03%	0.003%
21	3.964	813	816	820	rBV2	177	144	0.01%	0.001%
22	4.462	968	971	974	rBV2	151	143	0.01%	0.001%
23	4.565	999	1003	1007	rBV	277	308	0.02%	0.003%
24	4.626	1007	1022	1061	rVV	144020	406430	31.57%	4.088%
25	4.925	1110	1115	1118	rBV2	180	192	0.01%	0.002%
26	5.067	1143	1159	1187	rBV	227933	498994	38.76%	5.019%
27	5.289	1223	1228	1238	rBV5	702	1227	0.10%	0.012%
28	5.729	1343	1365	1387	rBV2	478244	1287556	100.00%	12.951%
29	5.896	1415	1417	1421	rVB4	238	164	0.01%	0.002%
30	6.150	1493	1496	1500	rBV2	262	213	0.02%	0.002%
31	6.253	1512	1528	1547	rBV	376096	700059	54.37%	7.042%
32	6.546	1605	1619	1635	rBV	138726	261389	20.30%	2.629%
33	6.633	1643	1646	1647	rVB	293	134	0.01%	0.001%
34	6.694	1650	1665	1688	rBV	304636	594043	46.14%	5.975%
35	6.999	1757	1760	1764	rVV	209	195	0.02%	0.002%
36	7.041	1769	1773	1782	rVB2	335	518	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
 Data File : VU045178.D
 Acq On : 06 Oct 2021 12:15
 Operator : SY/MD
 Sample : M4024-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.186	1810	1818	1826	rBV3	1889	2764	0.21%	0.028%
38	7.250	1834	1838	1844	rBV2	196	274	0.02%	0.003%
39	7.568	1924	1937	1954	rBV2	155708	272258	21.15%	2.739%
40	7.687	1967	1974	1982	rVV3	1164	1803	0.14%	0.018%
41	7.716	1982	1983	1986	rVB	315	143	0.01%	0.001%
42	7.842	2018	2022	2027	rBV	186	222	0.02%	0.002%
43	7.903	2027	2041	2056	rBV	580800	997227	77.45%	10.031%
44	7.974	2058	2063	2078	rVB	8708	13244	1.03%	0.133%
45	8.183	2116	2128	2144	rBV	110557	181748	14.12%	1.828%
46	8.398	2190	2195	2202	rVB	351	456	0.04%	0.005%
47	8.433	2202	2206	2209	rBV	319	283	0.02%	0.003%
48	8.469	2214	2217	2223	rBV3	237	304	0.02%	0.003%
49	8.556	2240	2244	2246	rBV3	394	295	0.02%	0.003%
50	8.636	2256	2269	2314	rBV	409737	725071	56.31%	7.293%
51	8.999	2376	2382	2384	rBV2	209	224	0.02%	0.002%
52	9.076	2401	2406	2410	rBV2	213	284	0.02%	0.003%
53	9.192	2437	2442	2444	rBV2	204	206	0.02%	0.002%
54	9.215	2444	2449	2451	rBV2	178	188	0.01%	0.002%
55	9.273	2464	2467	2470	rVB	164	137	0.01%	0.001%
56	9.301	2470	2476	2480	rBV2	229	286	0.02%	0.003%
57	9.359	2491	2494	2497	rBV	279	227	0.02%	0.002%
58	9.420	2499	2513	2537	rBV	535444	876023	68.04%	8.812%
59	9.572	2555	2560	2562	rBV2	243	273	0.02%	0.003%
60	9.700	2593	2600	2606	rBV	781	1069	0.08%	0.011%
61	9.832	2638	2641	2645	rVB2	248	235	0.02%	0.002%
62	9.986	2686	2689	2692	rVB	215	134	0.01%	0.001%
63	10.192	2750	2753	2756	rBV	228	165	0.01%	0.002%
64	10.321	2790	2793	2797	rBV2	171	146	0.01%	0.001%
65	10.617	2878	2885	2889	rBV2	223	299	0.02%	0.003%
66	10.674	2897	2903	2909	rBV4	1901	2589	0.20%	0.026%
67	10.761	2916	2930	2951	rVB	412964	667628	51.85%	6.715%
68	10.867	2960	2963	2966	rBV2	331	235	0.02%	0.002%
69	10.922	2977	2980	2983	rBV2	335	256	0.02%	0.003%
70	11.009	3003	3007	3011	rVV3	228	244	0.02%	0.002%
71	11.089	3027	3032	3035	rBV	309	273	0.02%	0.003%
72	11.154	3044	3052	3056	rVB2	217	364	0.03%	0.004%
73	11.182	3056	3061	3065	rBV	200	274	0.02%	0.003%
74	11.205	3065	3068	3071	rVB3	405	296	0.02%	0.003%
75	11.244	3075	3080	3082	rBV2	147	140	0.01%	0.001%
76	11.459	3135	3147	3148	rBV4	1284	1376	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
 Data File : VU045178.D
 Acq On : 06 Oct 2021 12:15
 Operator : SY/MD
 Sample : M4024-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.636	3195	3202	3204	rBV2	526	562	0.04%	0.006%
78	11.700	3217	3222	3227	rBV2	723	666	0.05%	0.007%
79	11.816	3245	3258	3276	rBV	484073	766279	59.51%	7.708%
80	11.912	3286	3288	3294	rVB3	221	155	0.01%	0.002%
81	11.944	3295	3298	3299	rBV2	351	144	0.01%	0.001%
82	11.973	3305	3307	3316	rVB4	938	900	0.07%	0.009%
83	12.195	3362	3376	3395	rBV	525680	846140	65.72%	8.511%
84	12.649	3514	3517	3521	rBV2	265	205	0.02%	0.002%
85	12.735	3537	3544	3551	rBV2	258	466	0.04%	0.005%
86	12.768	3551	3554	3557	rBV	250	171	0.01%	0.002%
87	12.809	3564	3567	3569	rBV2	214	180	0.01%	0.002%
88	12.964	3608	3615	3618	rBV2	310	346	0.03%	0.003%
89	13.067	3644	3647	3650	rBV2	183	185	0.01%	0.002%
90	13.237	3697	3700	3702	rBV	284	208	0.02%	0.002%
91	13.597	3806	3812	3815	rBV2	199	256	0.02%	0.003%
92	14.102	3960	3969	3973	rBV3	734	1112	0.09%	0.011%
93	14.333	4037	4041	4046	rVB3	571	475	0.04%	0.005%
94	14.636	4133	4135	4139	rBV2	293	200	0.02%	0.002%
95	14.674	4144	4147	4152	rBV3	309	303	0.02%	0.003%
96	14.796	4182	4185	4190	rBV2	371	316	0.02%	0.003%
97	14.819	4190	4192	4194	rBV	288	175	0.01%	0.002%
98	15.186	4304	4306	4310	rVB	317	180	0.01%	0.002%
99	15.208	4310	4313	4314	rBV2	344	192	0.01%	0.002%
100	15.677	4456	4459	4462	rBV2	275	205	0.02%	0.002%




Sum of corrected areas: 9941683

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
Data File : VU045178.D
Acq On : 06 Oct 2021 12:15
Operator : SY/MD
Sample : M4024-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

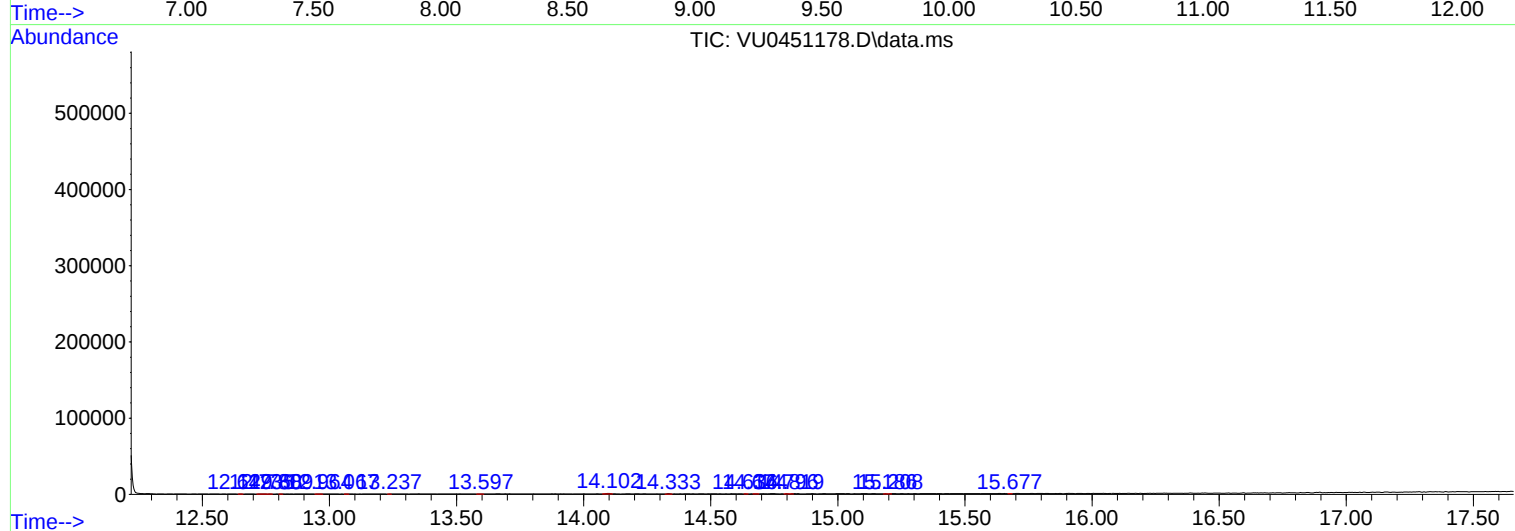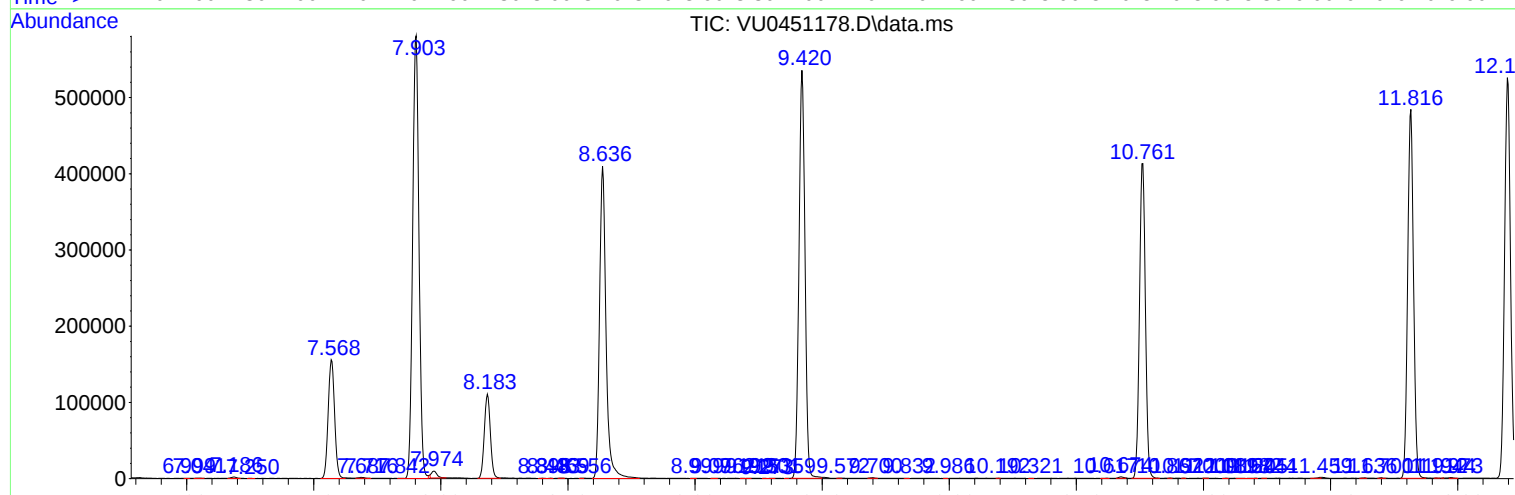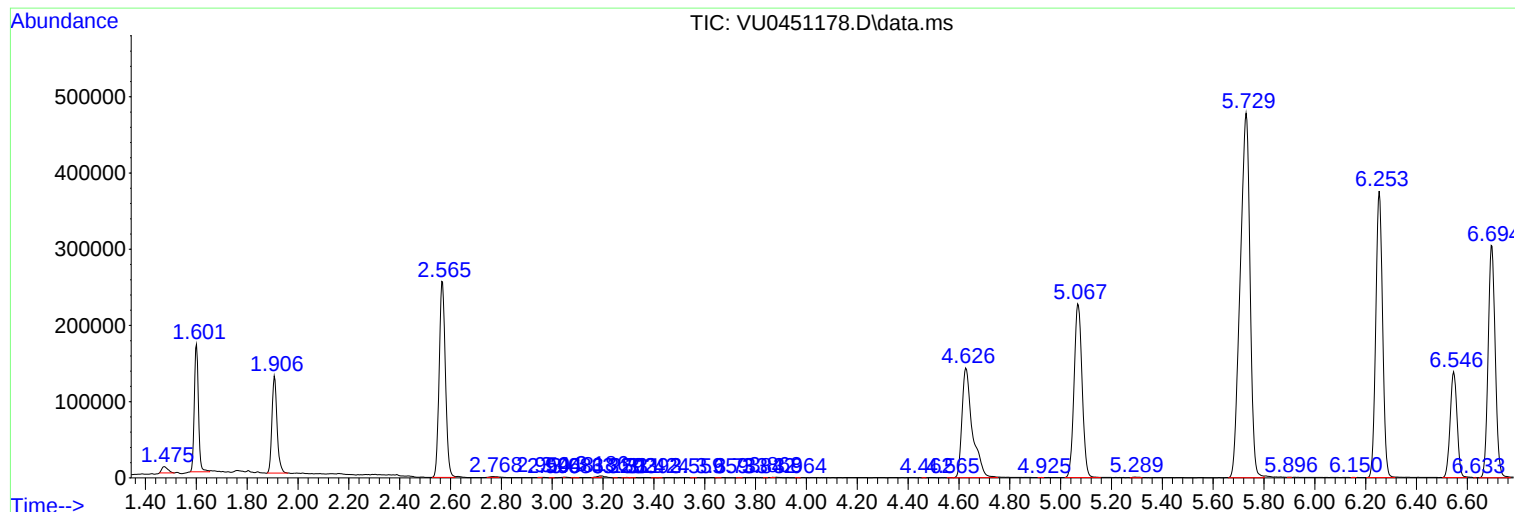

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
Data File : VU045178.D
Acq On : 06 Oct 2021 12:15
Operator : SY/MD
Sample : M4024-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
Data File : VU045178.D
Acq On : 06 Oct 2021 12:15
Operator : SY/MD
Sample : M4024-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------