

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
 Data File : VU045179.D
 Acq On : 06 Oct 2021 12:39
 Operator : SY/MD
 Sample : M4024-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU0451179.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	36	42	53	rBV3	7992	15038	0.34%	0.092%
2	1.600	74	81	95	rBV	167724	182738	4.10%	1.121%
3	1.909	169	177	196	rVB	123314	176032	3.95%	1.080%
4	2.575	369	384	400	rBV3	395268	776390	17.41%	4.764%
5	2.755	437	440	441	rBV2	356	200	0.00%	0.001%
6	2.764	441	443	447	rVB2	410	269	0.01%	0.002%
7	3.051	528	532	538	rVB	745	659	0.01%	0.004%
8	3.192	563	576	591	rBV3	6374	13886	0.31%	0.085%
9	3.359	619	628	636	rBV5	1624	3107	0.07%	0.019%
10	3.459	657	659	664	rVB2	181	174	0.00%	0.001%
11	3.620	704	709	712	rBV2	175	197	0.00%	0.001%
12	3.649	712	718	721	rBV2	137	149	0.00%	0.001%
13	3.874	773	788	803	rBV2	14777	33425	0.75%	0.205%
14	3.993	822	825	828	rVV2	293	243	0.01%	0.001%
15	4.028	832	836	838	rBV	195	158	0.00%	0.001%
16	4.083	848	853	856	rBV2	188	151	0.00%	0.001%
17	4.150	870	874	878	rBV2	245	323	0.01%	0.002%
18	4.208	889	892	897	rVB2	195	188	0.00%	0.001%
19	4.247	901	904	911	rVB2	273	348	0.01%	0.002%
20	4.285	912	916	919	rBV2	212	157	0.00%	0.001%
21	4.337	927	932	935	rBV2	181	201	0.00%	0.001%
22	4.369	939	942	945	rBV	139	149	0.00%	0.001%
23	4.671	1007	1036	1068	rBV2	867118	2262210	50.72%	13.882%
24	5.070	1143	1160	1183	rBV	226921	499842	11.21%	3.067%
25	5.256	1214	1218	1219	rBV2	429	335	0.01%	0.002%
26	5.317	1224	1237	1250	rVB5	3946	9636	0.22%	0.059%
27	5.469	1280	1284	1287	rBV2	242	210	0.00%	0.001%
28	5.600	1321	1325	1328	rBV	180	174	0.00%	0.001%
29	5.729	1338	1365	1398	rBV2	469089	1280536	28.71%	7.858%
30	6.253	1514	1528	1552	rBV	377132	706207	15.83%	4.334%
31	6.546	1603	1619	1651	rBV	2386637	4459965	100.00%	27.368%
32	6.697	1653	1666	1688	rVB	302297	593531	13.31%	3.642%
33	6.973	1750	1752	1755	rVB	300	172	0.00%	0.001%
34	7.044	1768	1774	1783	rVB2	490	1075	0.02%	0.007%
35	7.185	1808	1818	1827	rBV4	1732	3052	0.07%	0.019%
36	7.285	1845	1849	1854	rBV2	183	204	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
 Data File : VU045179.D
 Acq On : 06 Oct 2021 12:39
 Operator : SY/MD
 Sample : M4024-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.504	1914	1917	1921	rVB	332	250	0.01%	0.002%
38	7.568	1924	1937	1953	rBV	154805	268404	6.02%	1.647%
39	7.690	1967	1975	1983	rVB3	1514	2244	0.05%	0.014%
40	7.902	2026	2041	2055	rBV	577993	975914	21.88%	5.989%
41	7.970	2058	2062	2076	rVB	9339	14407	0.32%	0.088%
42	8.182	2115	2128	2146	rBV	107575	177536	3.98%	1.089%
43	8.349	2178	2180	2188	rVB	386	229	0.01%	0.001%
44	8.404	2188	2197	2206	rBV5	7523	12473	0.28%	0.077%
45	8.459	2206	2214	2216	rBV2	131	171	0.00%	0.001%
46	8.523	2230	2234	2236	rBV2	221	206	0.00%	0.001%
47	8.636	2256	2269	2303	rVV	385508	699638	15.69%	4.293%
48	8.915	2350	2356	2360	rBV2	149	209	0.00%	0.001%
49	9.131	2418	2423	2426	rVB2	197	188	0.00%	0.001%
50	9.218	2447	2450	2453	rVB2	267	178	0.00%	0.001%
51	9.246	2453	2459	2462	rVB	223	237	0.01%	0.001%
52	9.275	2462	2468	2471	rBV2	299	403	0.01%	0.002%
53	9.320	2477	2482	2487	rBV2	177	236	0.01%	0.001%
54	9.420	2499	2513	2534	rBV	529075	869645	19.50%	5.336%
55	9.700	2592	2600	2606	rBB3	783	1148	0.03%	0.007%
56	9.944	2673	2676	2679	rBV	236	174	0.00%	0.001%
57	10.099	2720	2724	2726	rBV2	324	298	0.01%	0.002%
58	10.185	2746	2751	2754	rBV	221	219	0.00%	0.001%
59	10.552	2863	2865	2869	rVB	257	159	0.00%	0.001%
60	10.571	2869	2871	2874	rBV	192	159	0.00%	0.001%
61	10.645	2890	2894	2896	rBV2	243	215	0.00%	0.001%
62	10.674	2896	2903	2912	rVB3	1526	2403	0.05%	0.015%
63	10.761	2917	2930	2946	rBV	410574	652355	14.63%	4.003%
64	11.008	3003	3007	3011	rBV2	279	201	0.00%	0.001%
65	11.028	3011	3013	3016	rBV	285	217	0.00%	0.001%
66	11.127	3040	3044	3047	rVB2	316	218	0.00%	0.001%
67	11.462	3143	3148	3159	rVB4	1124	2076	0.05%	0.013%
68	11.562	3176	3179	3184	rBV	234	217	0.00%	0.001%
69	11.603	3190	3192	3196	rBV	189	170	0.00%	0.001%
70	11.635	3196	3202	3206	rVV4	654	893	0.02%	0.005%
71	11.703	3217	3223	3228	rVB3	637	785	0.02%	0.005%
72	11.816	3245	3258	3279	rBV	479076	757312	16.98%	4.647%
73	11.938	3294	3296	3298	rBV	325	164	0.00%	0.001%
74	11.973	3302	3307	3308	rBV	706	547	0.01%	0.003%
75	12.034	3322	3326	3331	rBV2	202	199	0.00%	0.001%
76	12.195	3363	3376	3392	rBV	510349	826293	18.53%	5.070%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
 Data File : VU045179.D
 Acq On : 06 Oct 2021 12:39
 Operator : SY/MD
 Sample : M4024-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	12.475	3459	3463	3467	rBV2	318	234	0.01%	0.001%
78	12.500	3467	3471	3474	rBV2	212	203	0.00%	0.001%
79	12.812	3563	3568	3574	rBV2	192	307	0.01%	0.002%
80	12.883	3586	3590	3597	rVB	216	242	0.01%	0.001%
81	12.922	3599	3602	3608	rVB2	307	309	0.01%	0.002%
82	12.960	3612	3614	3622	rVB	297	338	0.01%	0.002%
83	12.996	3622	3625	3630	rBV2	292	244	0.01%	0.001%
84	13.024	3630	3634	3637	rBV	201	227	0.01%	0.001%
85	13.124	3662	3665	3669	rBV2	248	246	0.01%	0.002%
86	13.217	3688	3694	3695	rBV	301	283	0.01%	0.002%
87	13.420	3753	3757	3759	rBV2	265	204	0.00%	0.001%
88	13.648	3825	3828	3834	rVB2	310	330	0.01%	0.002%
89	13.677	3834	3837	3841	rBV2	218	178	0.00%	0.001%
90	13.796	3872	3874	3877	rBV	219	153	0.00%	0.001%
91	14.253	4013	4016	4020	rBV	224	169	0.00%	0.001%
92	14.352	4044	4047	4051	rBV	306	303	0.01%	0.002%
93	14.401	4060	4062	4066	rVV2	243	158	0.00%	0.001%
94	14.430	4068	4071	4075	rBV2	291	291	0.01%	0.002%
95	14.526	4098	4101	4103	rBV	312	173	0.00%	0.001%
96	14.610	4121	4127	4128	rBV2	237	192	0.00%	0.001%
97	14.706	4154	4157	4158	rBV	323	174	0.00%	0.001%
98	14.803	4184	4187	4191	rBV2	252	175	0.00%	0.001%
99	14.867	4204	4207	4211	rBV2	289	272	0.01%	0.002%
100	15.079	4269	4273	4276	rBV2	471	470	0.01%	0.003%




Sum of corrected areas: 16296196

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
Data File : VU045179.D
Acq On : 06 Oct 2021 12:39
Operator : SY/MD
Sample : M4024-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

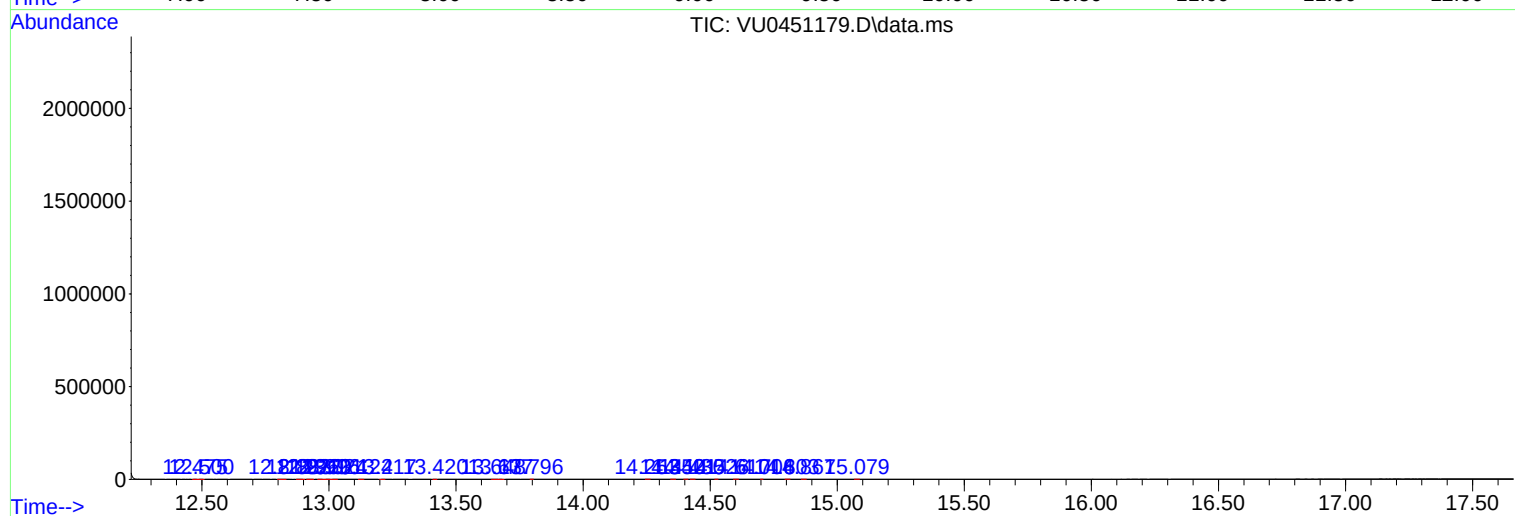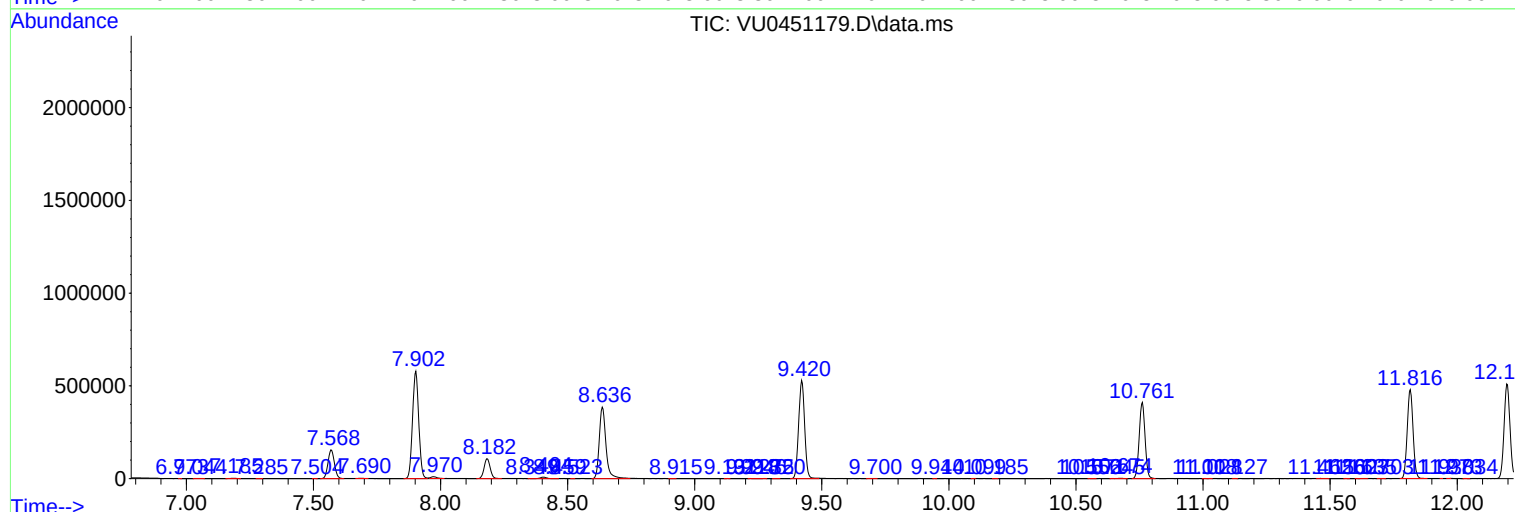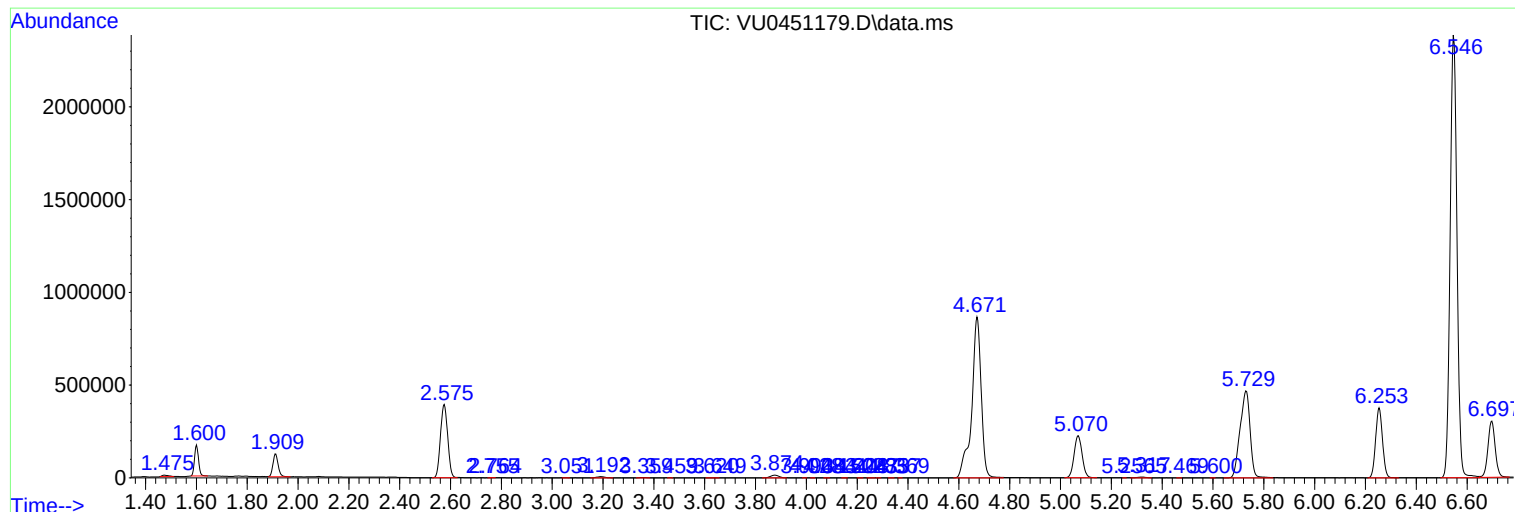

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
Data File : VU045179.D
Acq On : 06 Oct 2021 12:39
Operator : SY/MD
Sample : M4024-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
Data File : VU045179.D
Acq On : 06 Oct 2021 12:39
Operator : SY/MD
Sample : M4024-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
