


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100621\
Data File : VU045172.D
Acq On : 06 Oct 2021 09:32
Operator : SY/MD
Sample : BFB007
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB007

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Title : VOC Analysis
Last Update : Mon Oct 11 01:47:08 2021

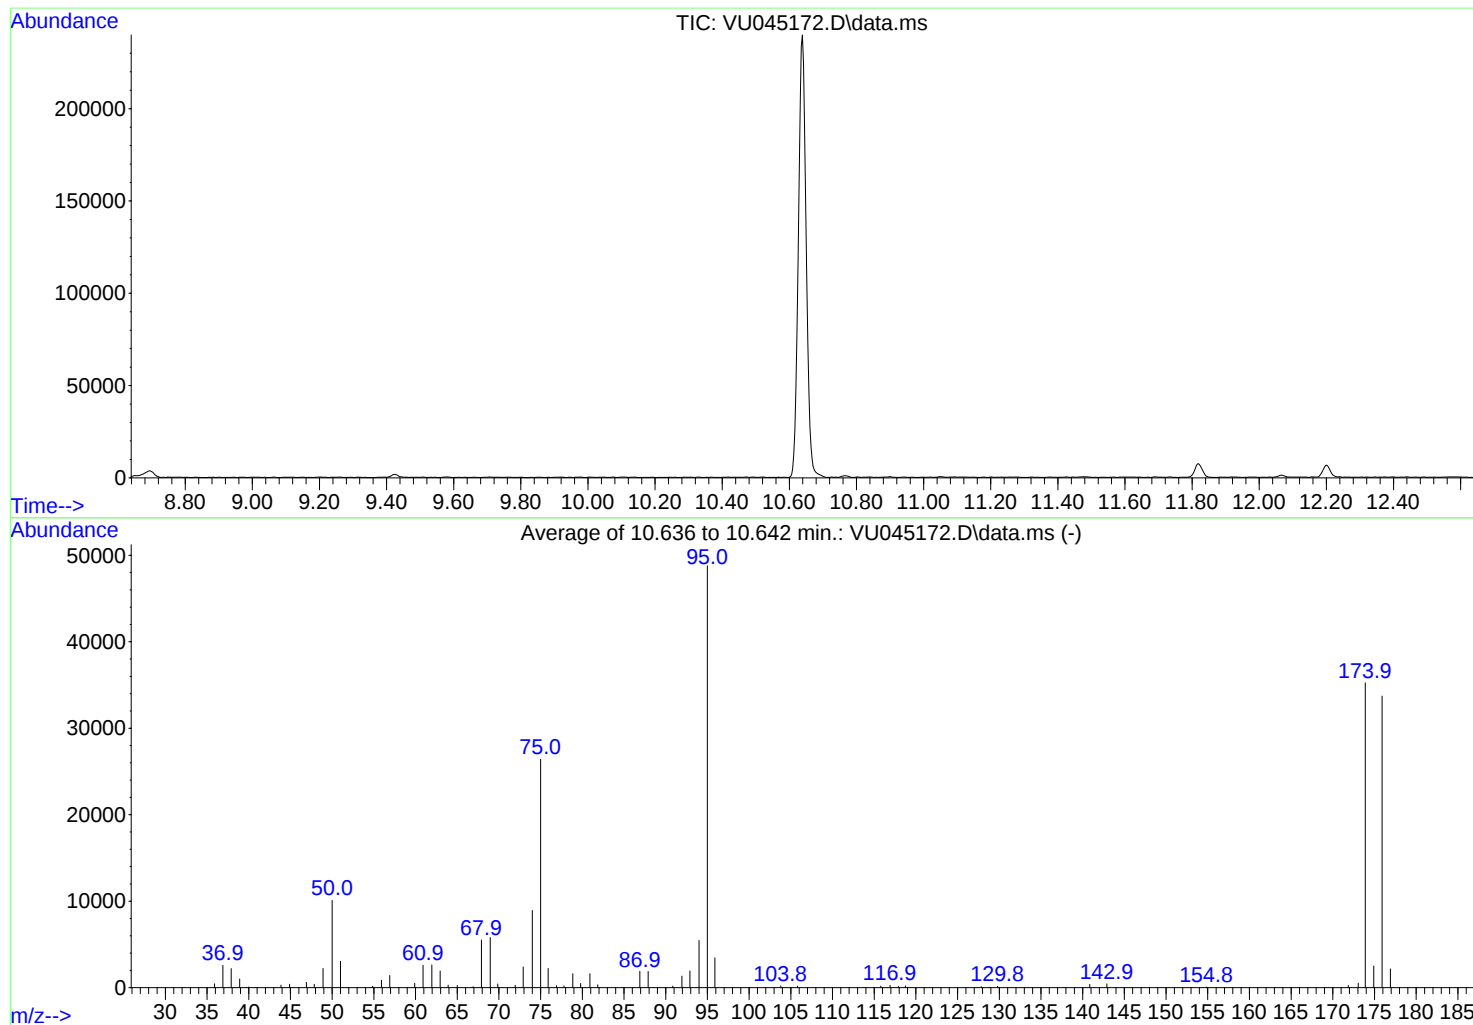

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	10093	PASS
75	95	30	80	54.1	26408	PASS
95	95	100	100	100.0	48781	PASS
96	95	5	9	7.0	3438	PASS
173	174	0.00	2	1.4	511	PASS
174	95	50	120	72.3	35248	PASS
175	174	5	9	7.1	2491	PASS
176	174	95	101	95.7	33720	PASS
177	176	5	9	6.4	2167	PASS

m/z	Abundance
43.80	300.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
35.90	420.0
36.90	2575.0
37.90	2171.0
38.90	1033.0
43.90	583.0
44.90	421.0
46.90	615.0
47.80	418.0
48.90	2175.0
50.00	10659.0
51.00	3126.0
51.90	108.0
54.80	126.0
55.90	960.0
56.90	1442.0
59.90	519.0
60.90	2741.0
62.00	2560.0
63.00	2034.0
63.90	318.0
65.00	290.0
66.90	126.0
67.90	5677.0
68.90	6000.0
69.90	412.0
71.90	308.0
72.90	2454.0
74.00	9054.0
75.00	26512.0
75.90	2302.0
76.90	246.0
77.80	227.0
78.90	1497.0
79.80	444.0
80.90	1612.0
81.90	352.0
86.90	1882.0
87.90	2009.0
90.90	156.0
91.90	1365.0
92.90	1853.0
94.00	5435.0
95.00	49256.0
95.90	3533.0
103.80	197.0
105.80	175.0
115.80	164.0
116.90	297.0
117.90	139.0
118.80	183.0
127.90	100.0
128.80	108.0
129.80	184.0
140.90	360.0
142.90	435.0
154.80	110.0
171.80	250.0
173.10	504.0
173.90	34584.0
174.90	2495.0
175.90	33088.0
176.90	2190.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
35.90	453.0
36.90	2660.0
37.90	2244.0
38.90	1023.0
40.00	106.0
43.90	617.0
44.90	389.0
46.90	638.0
47.90	391.0
48.90	2280.0
50.00	10410.0
51.00	3144.0
54.90	148.0
55.90	865.0
56.90	1467.0
59.90	511.0
60.90	2657.0
62.00	2716.0
63.00	1970.0
63.90	295.0
65.00	283.0
66.90	119.0
67.90	5692.0
69.00	5994.0
69.90	435.0
71.90	276.0
72.90	2463.0
74.00	9210.0
75.00	27264.0
75.90	2301.0
76.90	220.0
77.80	215.0
78.80	1677.0
79.80	495.0
80.90	1652.0
81.80	333.0
86.90	1935.0
87.90	1951.0
90.80	191.0
92.00	1366.0
92.90	1977.0
94.00	5623.0
95.00	50400.0
95.90	3555.0
103.80	216.0
105.80	188.0
115.80	182.0
116.90	290.0
117.90	136.0
118.80	210.0
127.80	111.0
129.80	149.0
140.80	383.0
142.90	454.0
154.90	116.0
171.80	261.0
173.00	535.0
173.90	36424.0
174.90	2528.0
175.90	34824.0
176.90	2248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
35.90	452.0
36.90	2506.0
37.90	2171.0
38.90	948.0
39.90	120.0
43.90	612.0
44.90	378.0
46.90	593.0
47.90	342.0
48.90	2196.0
50.00	9210.0
51.00	2874.0
54.90	155.0
55.90	781.0
56.90	1308.0
59.90	457.0
60.90	2349.0
61.90	2590.0
62.90	1779.0
63.90	281.0
65.00	232.0
66.90	102.0
67.90	5191.0
69.00	5397.0
69.80	455.0
72.00	241.0
72.90	2235.0
74.00	8514.0
75.00	25448.0
75.90	2078.0
76.90	195.0
77.80	171.0
78.80	1659.0
79.80	502.0
80.90	1549.0
81.80	315.0
86.90	1842.0
87.90	1651.0
90.80	193.0
91.90	1247.0
92.90	1933.0
94.00	5346.0
95.00	46688.0
95.90	3227.0
103.80	215.0
105.80	197.0
115.80	189.0
116.90	245.0
117.90	141.0
118.70	243.0
127.80	114.0
129.80	120.0
140.80	406.0
142.90	449.0
171.90	269.0
173.00	495.0
173.90	34736.0
174.90	2450.0
175.90	33248.0
176.90	2063.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007