

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051193.D
 Acq On : 07 Oct 2022 00:03
 Operator : JC/MD
 Sample : N4890-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E4

Quant Time: Oct 07 06:29:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 07 02:51:40 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.246	114	341029	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	366364	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	119952	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	141116	40.830	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	81.660%	
7) Chloroethane-d5	1.903	69	125342	39.041	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	78.080%	
11) 1,1-Dichloroethene-d2	2.562	63	162494	31.829	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	63.660%	
21) 2-Butanone-d5	4.620	46	187159	83.493	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	83.490%	
24) Chloroform-d	5.060	84	258120	46.355	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.720%	
26) 1,2-Dichloroethane-d4	5.700	65	167488	48.595	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.200%	
32) Benzene-d6	5.726	84	497963	46.415	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.820%	
36) 1,2-Dichloropropane-d6	6.690	67	176052	50.571	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	101.140%	
41) Toluene-d8	7.896	98	387150	39.057	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	78.120%#	
43) trans-1,3-Dichloroprop...	8.179	79	63633	38.322	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	76.640%	
47) 2-Hexanone-d5	8.632	63	81209	57.771	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	57.770%	
56) 1,1,2,2-Tetrachloroeth...	10.754	84	259990	42.732	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	85.460%	
66) 1,2-Dichlorobenzene-d4	12.192	152	124373	48.536	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	97.080%	
Target Compounds						
					Qvalue	
34) Trichloroethene	6.539	95	76558	26.464	ug/L	97
46) Tetrachloroethene	8.552	164	8716	3.976	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051193.D
Acq On : 07 Oct 2022 00:03
Operator : JC/MD
Sample : N4890-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E4

Quant Time: Oct 07 06:29:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 07 02:51:40 2022
Response via : Initial Calibration




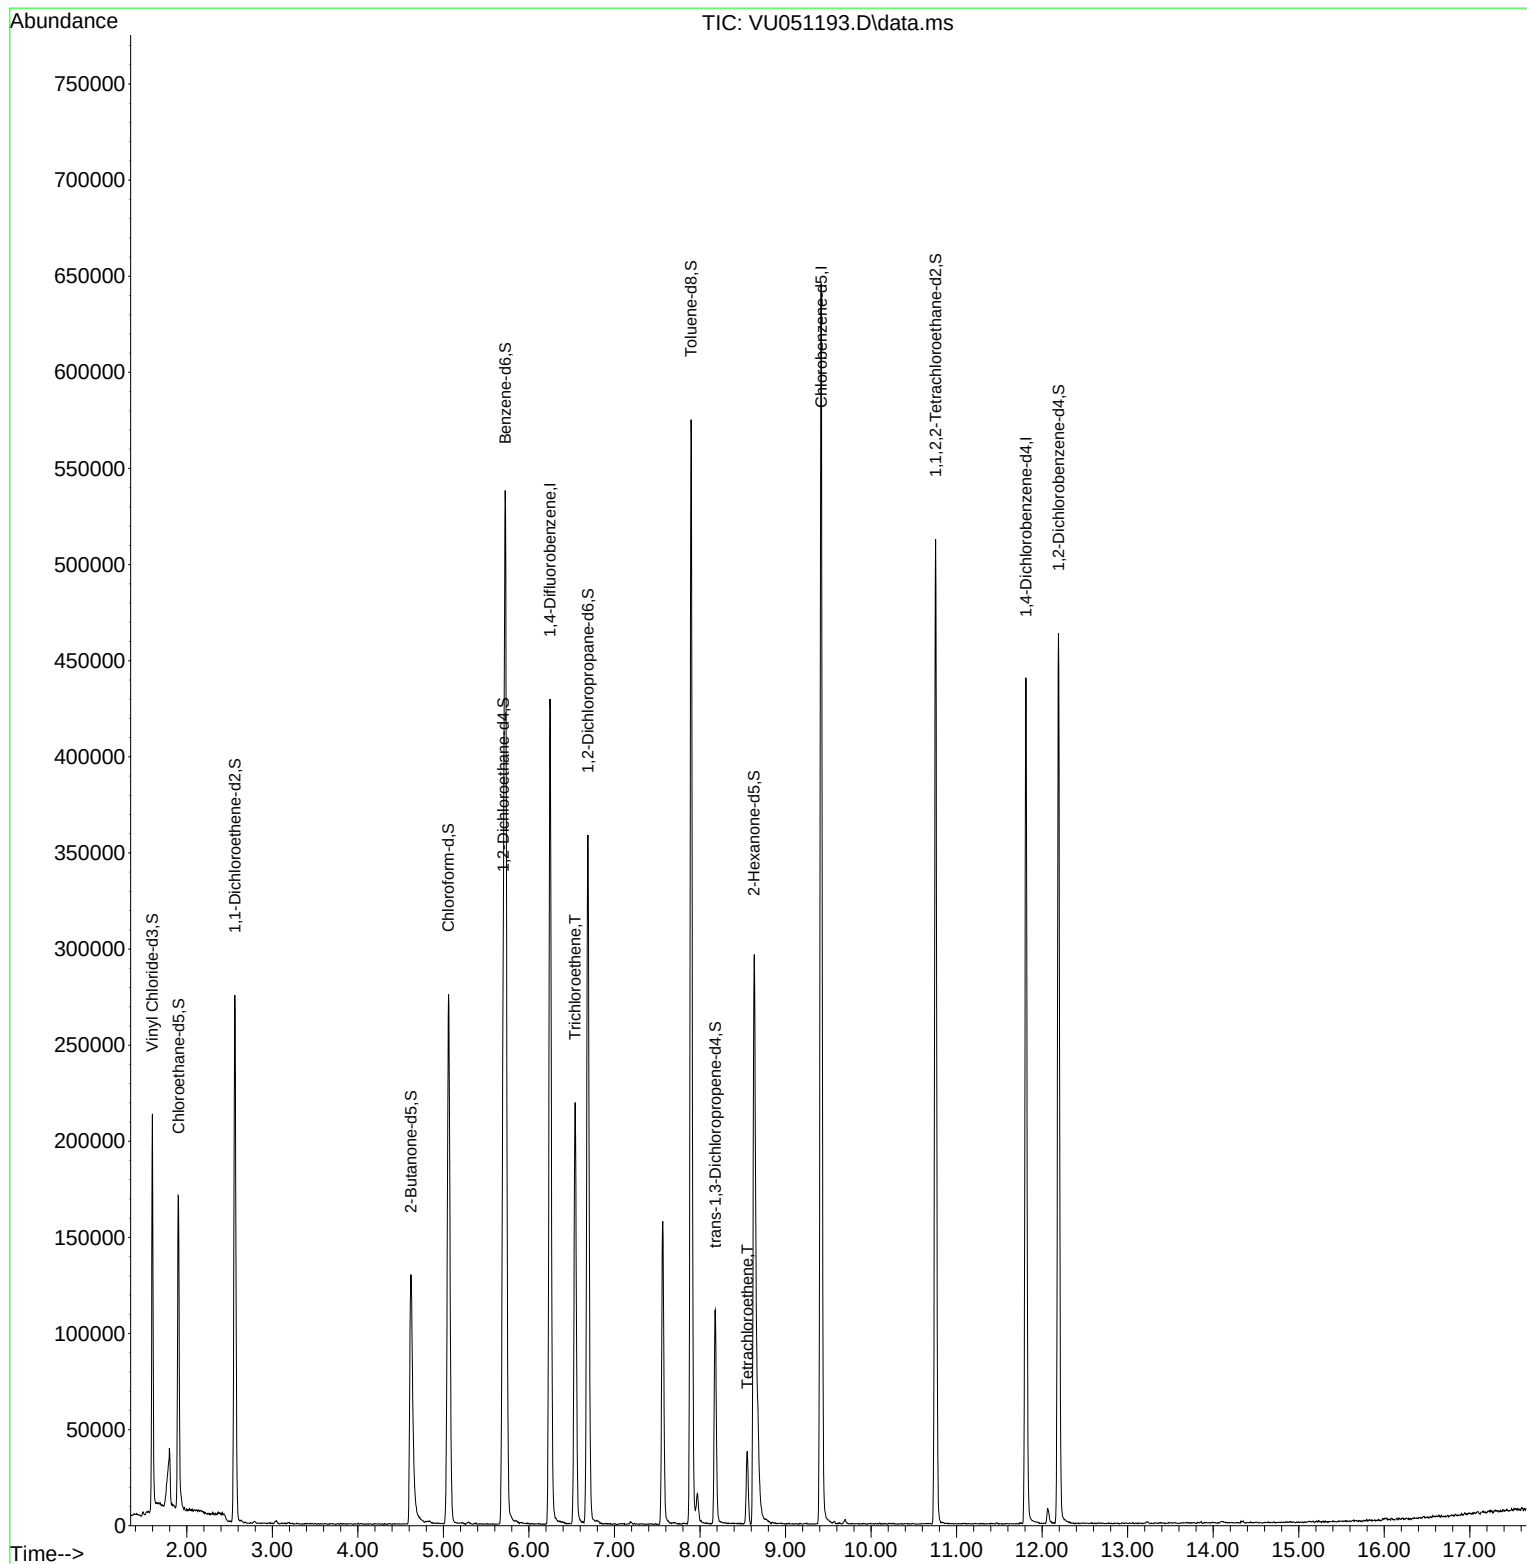


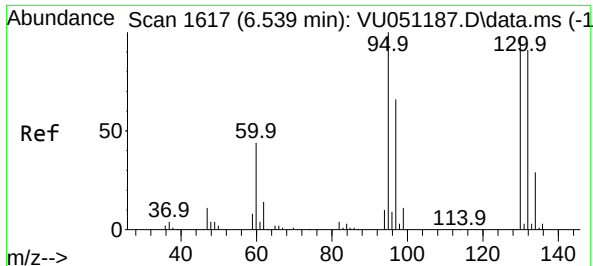

#34
Trichloroethene
Concen: 26.464 ug/L
RT: 6.539 min Scan# 1
Delta R.T. -0.000 min
Lab File: VU051193.D
Acq: 07 Oct 2022 00:03

Instrument :
MSVOA_U
ClientSampleId :
EY0E4

Tgt Ion: 95 Resp: 76558
Ion Ratio Lower Upper
95 100
97 64.2 45.9 85.3
132 88.2 64.0 119.0
130 93.5 67.9 126.1

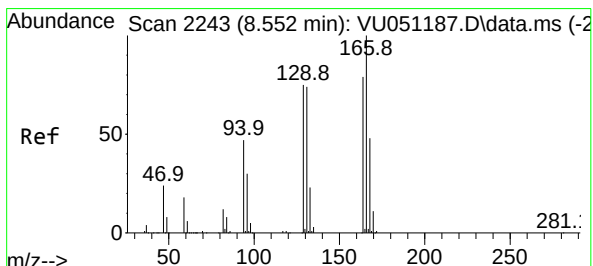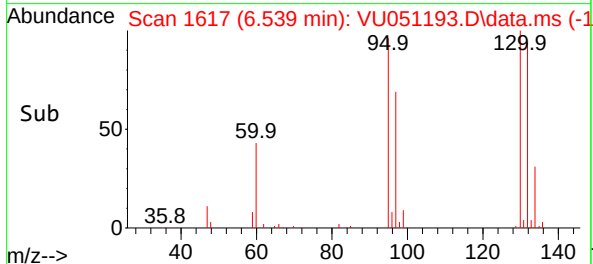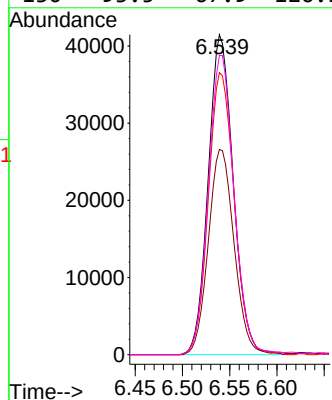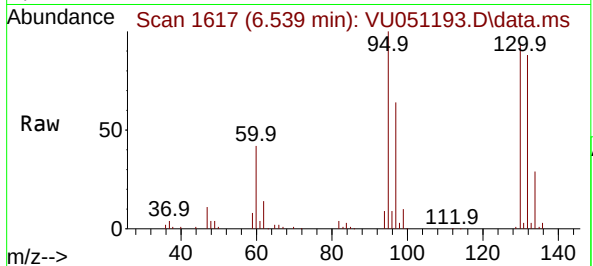

#46
Tetrachloroethene
Concen: 3.976 ug/L
RT: 8.552 min Scan# 2243
Delta R.T. -0.000 min
Lab File: VU051193.D
Acq: 07 Oct 2022 00:03

Tgt Ion: 164 Resp: 8716
Ion Ratio Lower Upper
164 100
129 88.4 68.1 126.5
131 85.6 67.8 126.0
166 108.5 90.5 168.1

